

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026492.D
 Acq On : 21 Jun 2022 16:38
 Operator : SY/MD
 Sample : N3355-14DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	80	88	103	rBV	84778	92883	15.26%	1.891%
2	1.584	162	169	182	rBV	78470	90759	14.91%	1.848%
3	2.124	328	337	353	rVB	160111	229950	37.79%	4.681%
4	2.526	452	462	476	rVB	14921	24971	4.10%	0.508%
5	3.934	887	900	928	rBV2	38436	162547	26.71%	3.309%
6	4.365	1015	1034	1059	rBV2	106377	267795	44.01%	5.452%
7	4.625	1101	1115	1124	rBV6	4529	9953	1.64%	0.203%
8	5.060	1234	1250	1283	rBV2	221907	553760	91.00%	11.273%
9	5.625	1411	1426	1453	rBV	178665	370999	60.97%	7.553%
10	5.921	1506	1518	1544	rBV	308240	608542	100.00%	12.388%
11	6.079	1554	1567	1586	rBV2	129038	265740	43.67%	5.410%
12	6.995	1840	1852	1870	rBV	42745	82020	13.48%	1.670%
13	7.320	1940	1953	1973	rBV	252236	447788	73.58%	9.116%
14	7.632	2038	2050	2073	rBV2	22480	43873	7.21%	0.893%
15	7.940	2132	2146	2166	rVB3	6603	11786	1.94%	0.240%
16	8.095	2184	2194	2231	rBV	160584	342268	56.24%	6.968%
17	8.854	2419	2430	2455	rBV	270752	445231	73.16%	9.064%
18	10.217	2842	2854	2868	rBV	86810	136486	22.43%	2.778%
19	10.381	2894	2905	2919	rVB2	16464	26407	4.34%	0.538%
20	11.249	3164	3175	3196	rBV	237575	365312	60.03%	7.437%
21	11.622	3280	3291	3311	rBV	211995	333159	54.75%	6.782%




Sum of corrected areas: 4912229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026492.D
Acq On : 21 Jun 2022 16:38
Operator : SY/MD
Sample : N3355-14DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

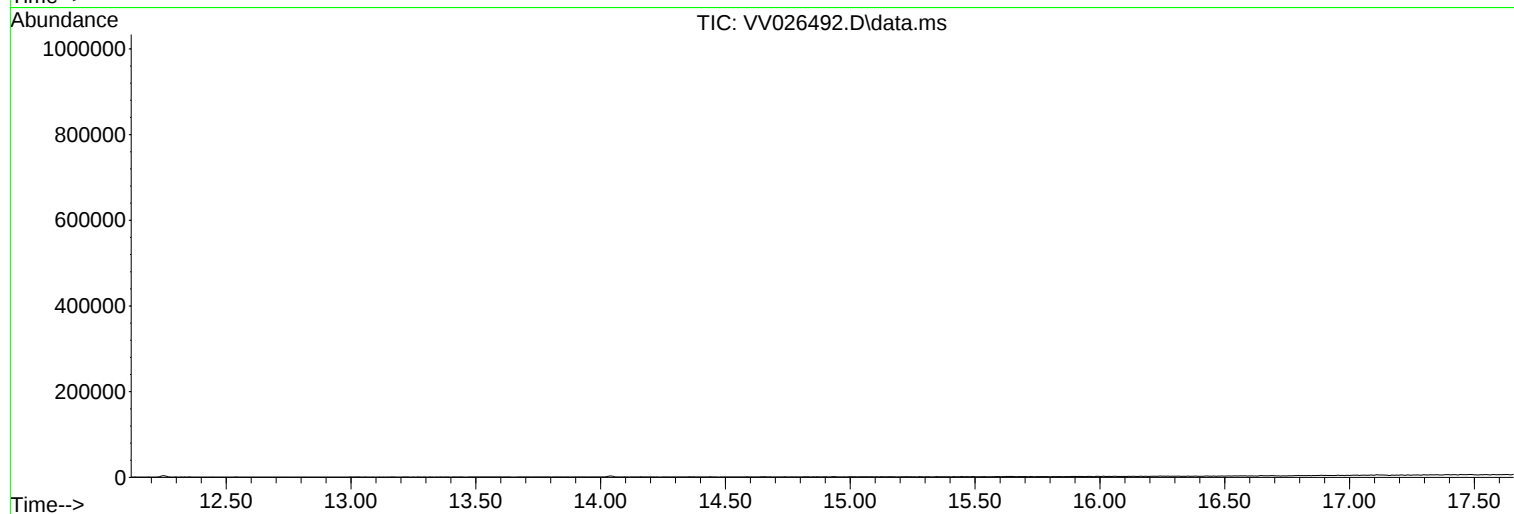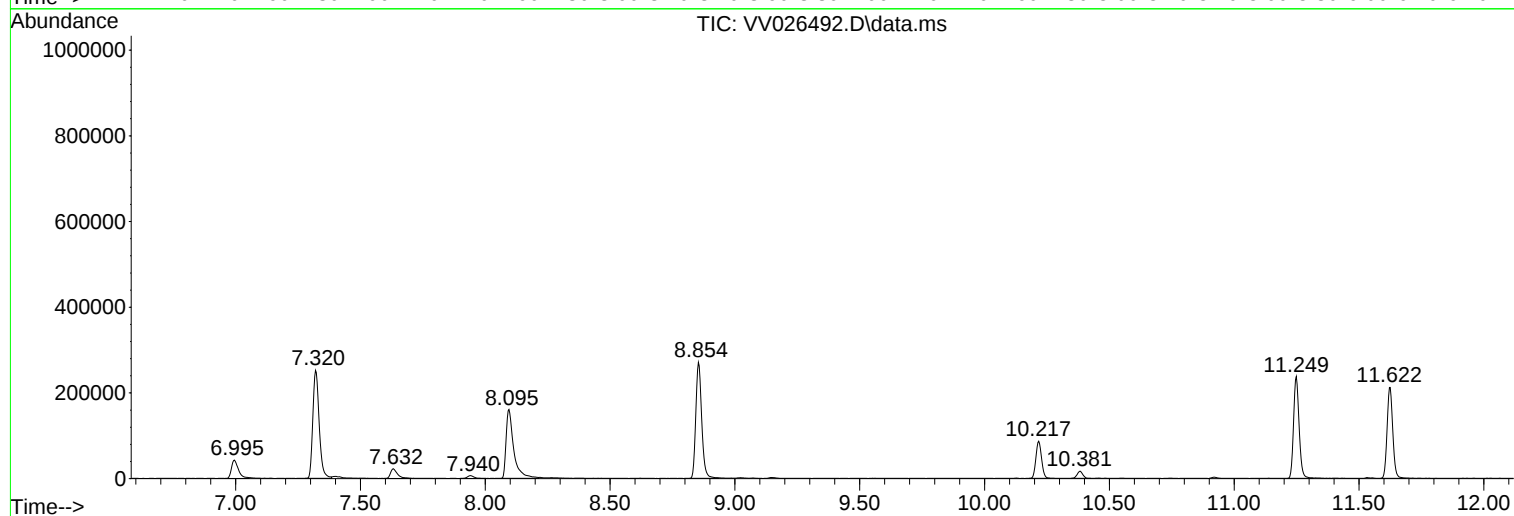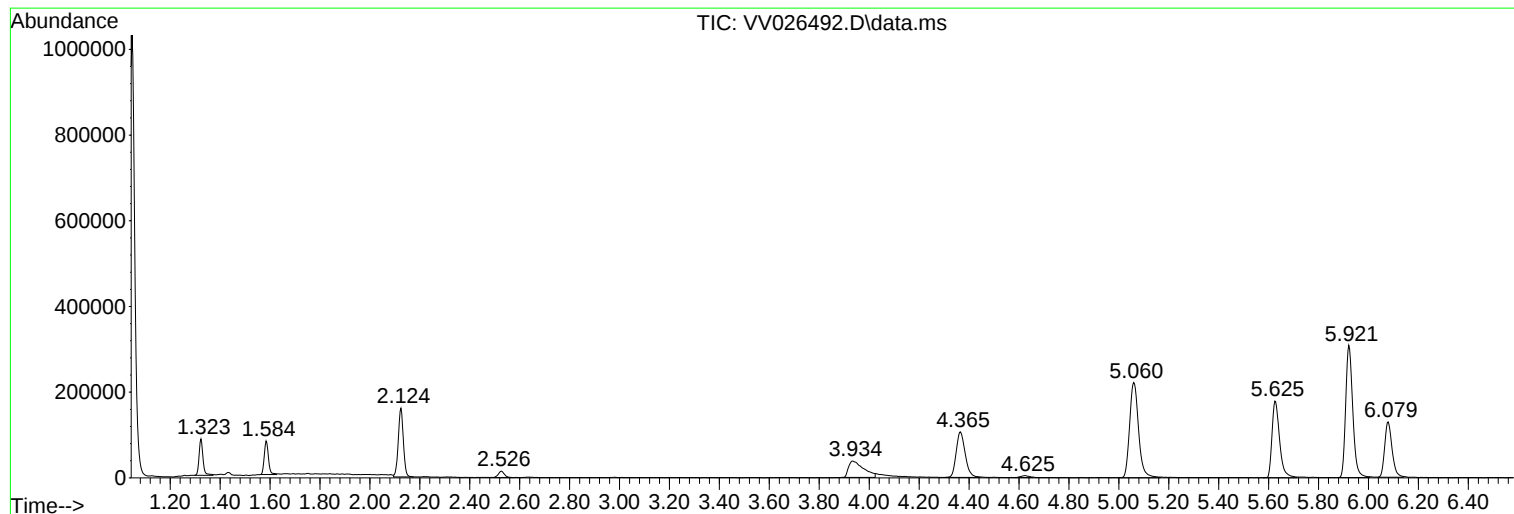

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026492.D
Acq On : 21 Jun 2022 16:38
Operator : SY/MD
Sample : N3355-14DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026492.D
Acq On : 21 Jun 2022 16:38
Operator : SY/MD
Sample : N3355-14DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc