

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026495.D
 Acq On : 21 Jun 2022 17:50
 Operator : SY/MD
 Sample : N3355-17DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0D3DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	103	rBV	84640	91020	16.02%	1.865%
2	1.584	162	169	180	rBV	78678	93258	16.41%	1.911%
3	2.124	327	337	354	rVB	162897	239730	42.19%	4.913%
4	2.526	453	462	475	rBB	18792	30807	5.42%	0.631%
5	3.944	884	903	941	rBV2	36644	178192	31.36%	3.652%
6	4.365	1017	1034	1060	rBV2	107973	269480	47.43%	5.523%
7	5.059	1233	1250	1277	rBV2	230050	568149	100.00%	11.644%
8	5.625	1415	1426	1455	rBV	185976	385585	67.87%	7.903%
9	5.921	1506	1518	1543	rBV	221485	443987	78.15%	9.100%
10	6.079	1553	1567	1590	rBV	133010	275318	48.46%	5.643%
11	6.995	1842	1852	1877	rBV2	43530	85532	15.05%	1.753%
12	7.320	1940	1953	1975	rBV	255980	456319	80.32%	9.352%
13	7.632	2041	2050	2068	rBV2	23308	43148	7.59%	0.884%
14	7.940	2134	2146	2156	rBV2	7040	11941	2.10%	0.245%
15	8.095	2182	2194	2228	rBV	163410	349190	61.46%	7.157%
16	8.854	2419	2430	2455	rBV	287793	468941	82.54%	9.611%
17	10.217	2843	2854	2869	rBV	87881	139300	24.52%	2.855%
18	10.381	2894	2905	2919	rVB2	16901	27082	4.77%	0.555%
19	11.249	3164	3175	3195	rBV	243862	377910	66.52%	7.745%
20	11.625	3278	3292	3312	rBV	217163	344252	60.59%	7.056%




Sum of corrected areas: 4879141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026495.D
Acq On : 21 Jun 2022 17:50
Operator : SY/MD
Sample : N3355-17DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

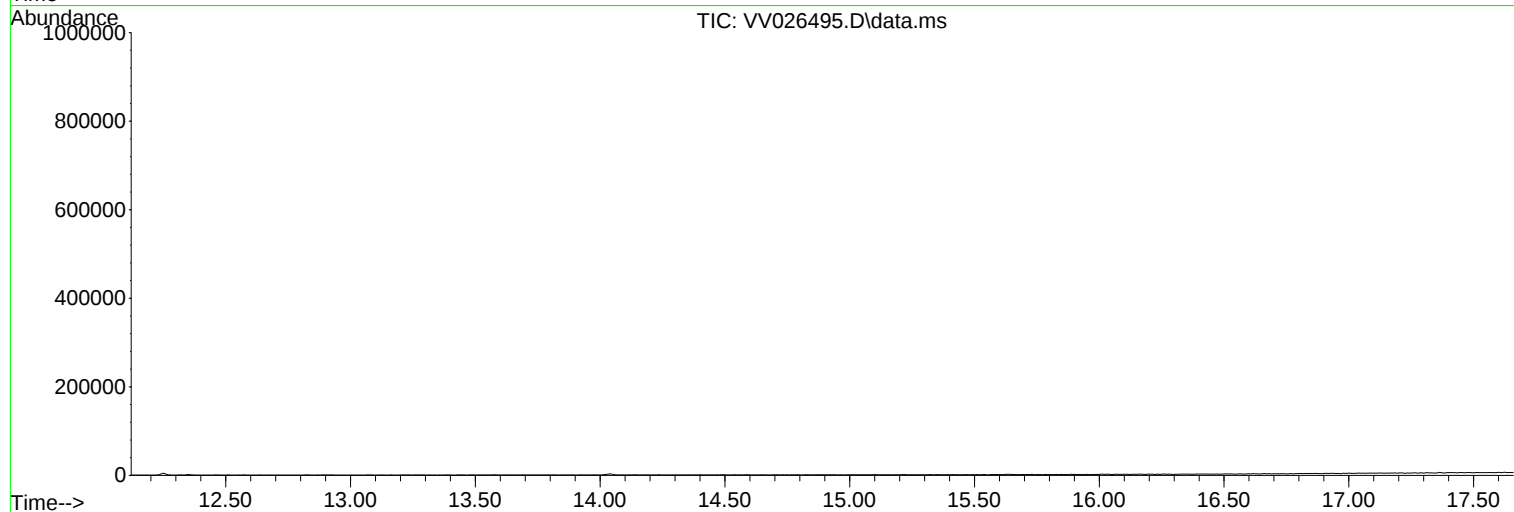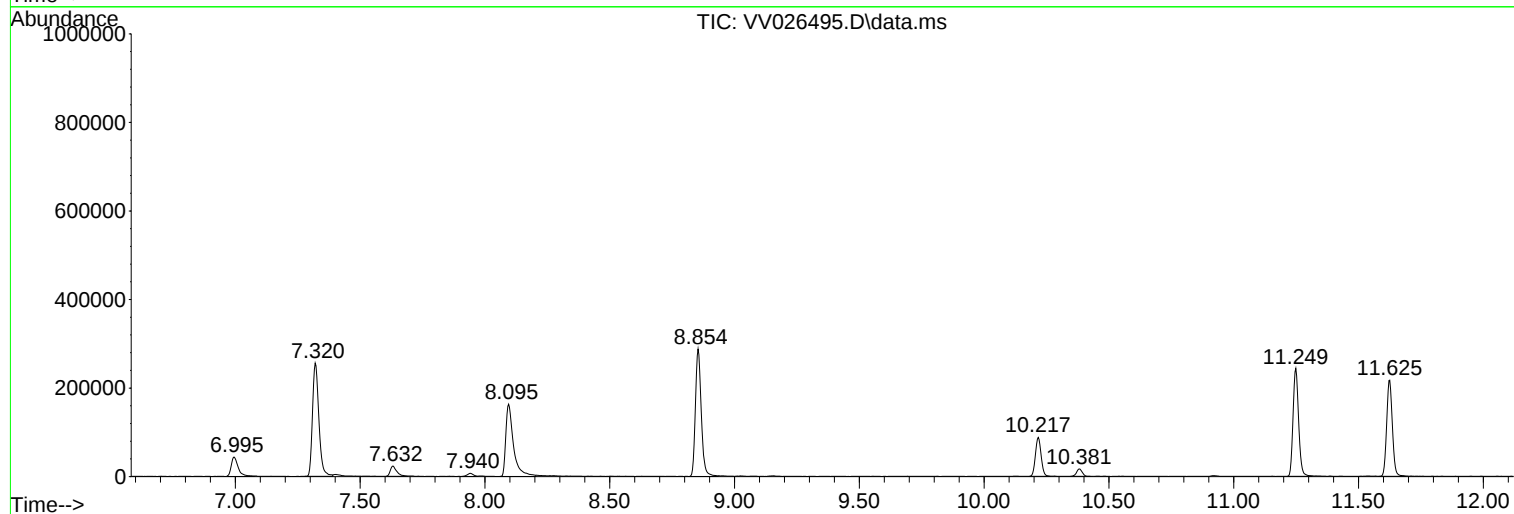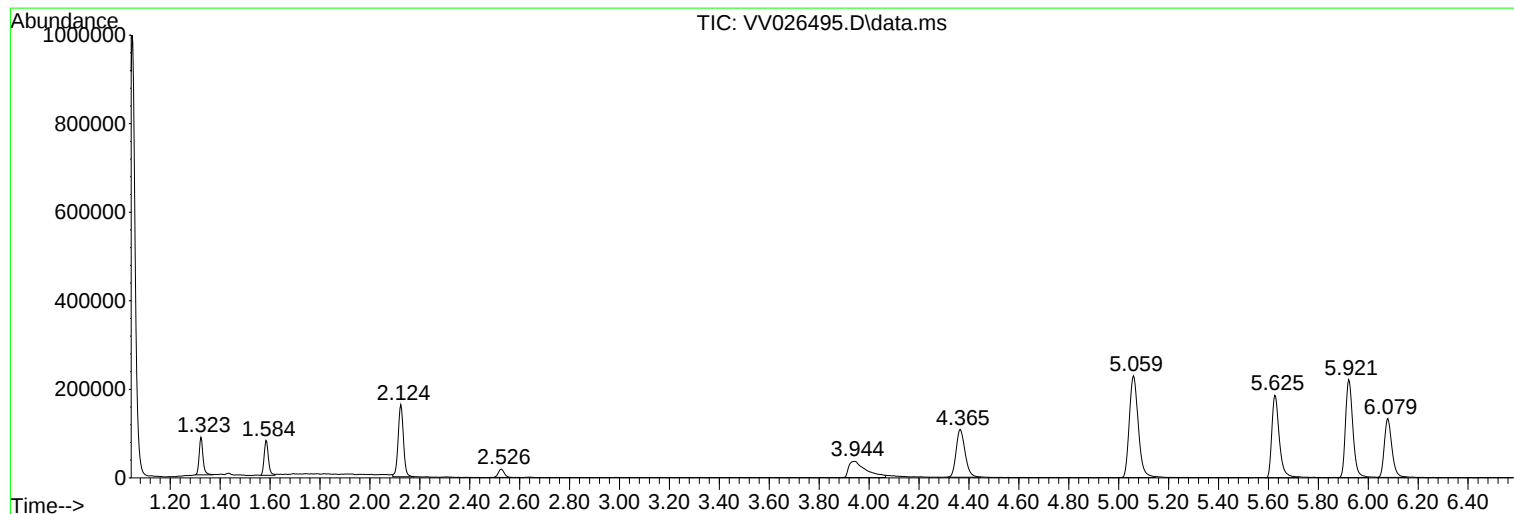

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026495.D
Acq On : 21 Jun 2022 17:50
Operator : SY/MD
Sample : N3355-17DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026495.D
Acq On : 21 Jun 2022 17:50
Operator : SY/MD
Sample : N3355-17DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0D3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc