

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
 Data File : VV026496.D
 Acq On : 21 Jun 2022 18:14
 Operator : SY/MD
 Sample : N3355-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY0C7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.262	56	69	75	rBV2	9051	17307	3.12%	0.395%
2	1.323	81	88	100	rBV	82058	87608	15.82%	1.998%
3	1.587	162	170	183	rBV	76865	91306	16.48%	2.083%
4	2.124	328	337	351	rVB	159119	227458	41.07%	5.188%
5	3.934	882	900	940	rBV	31498	138646	25.03%	3.162%
6	4.365	1017	1034	1065	rBV	106988	264493	47.75%	6.033%
7	5.060	1234	1250	1280	rBV2	222466	553890	100.00%	12.633%
8	5.625	1415	1426	1456	rBV2	181190	374357	67.59%	8.538%
9	5.928	1508	1520	1540	rBV2	43239	91961	16.60%	2.097%
10	6.079	1554	1567	1592	rBV	131054	271056	48.94%	6.182%
11	6.992	1840	1851	1868	rBV	43703	82267	14.85%	1.876%
12	7.320	1942	1953	1973	rBV	253728	446014	80.52%	10.173%
13	7.629	2041	2049	2066	rBV	22914	42872	7.74%	0.978%
14	8.095	2184	2194	2231	rBV2	167191	346931	62.64%	7.913%
15	8.854	2419	2430	2453	rBV	276935	454461	82.05%	10.365%
16	10.217	2843	2854	2871	rBV	86672	136189	24.59%	3.106%
17	10.381	2891	2905	2919	rBV	17028	27255	4.92%	0.622%
18	11.249	3162	3175	3195	rBV	241753	374182	67.56%	8.534%
19	11.532	3255	3263	3278	rBV4	8849	16575	2.99%	0.378%
20	11.622	3280	3291	3313	rVV	216553	339540	61.30%	7.744%




Sum of corrected areas: 4384368

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026496.D
Acq On : 21 Jun 2022 18:14
Operator : SY/MD
Sample : N3355-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

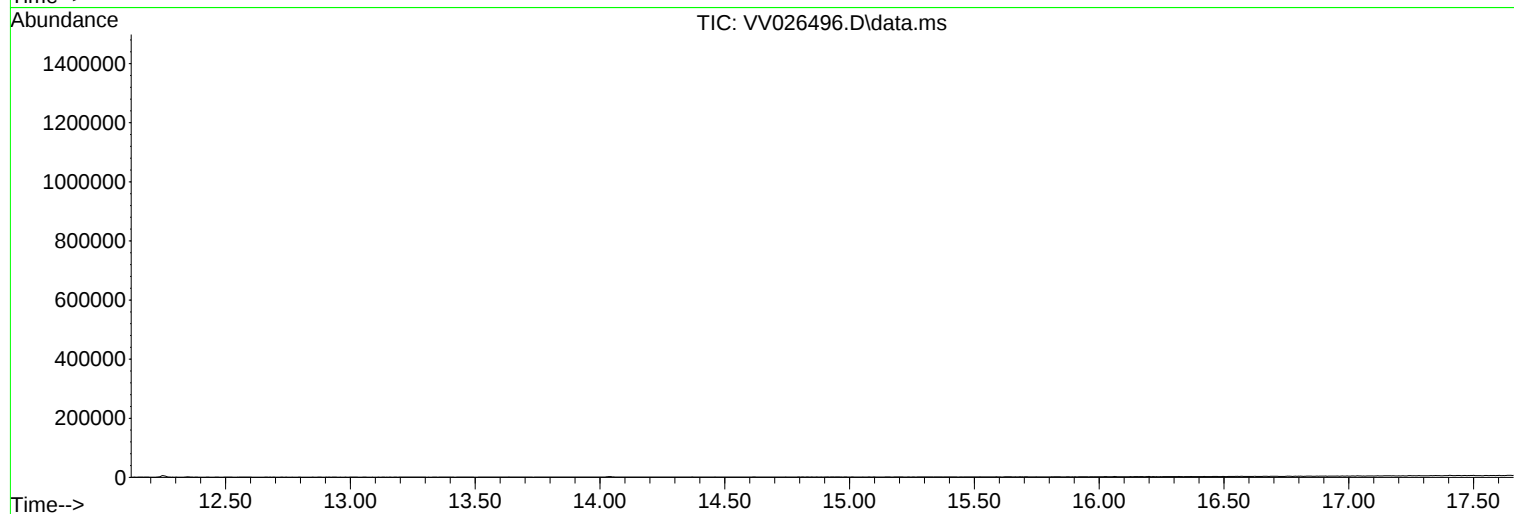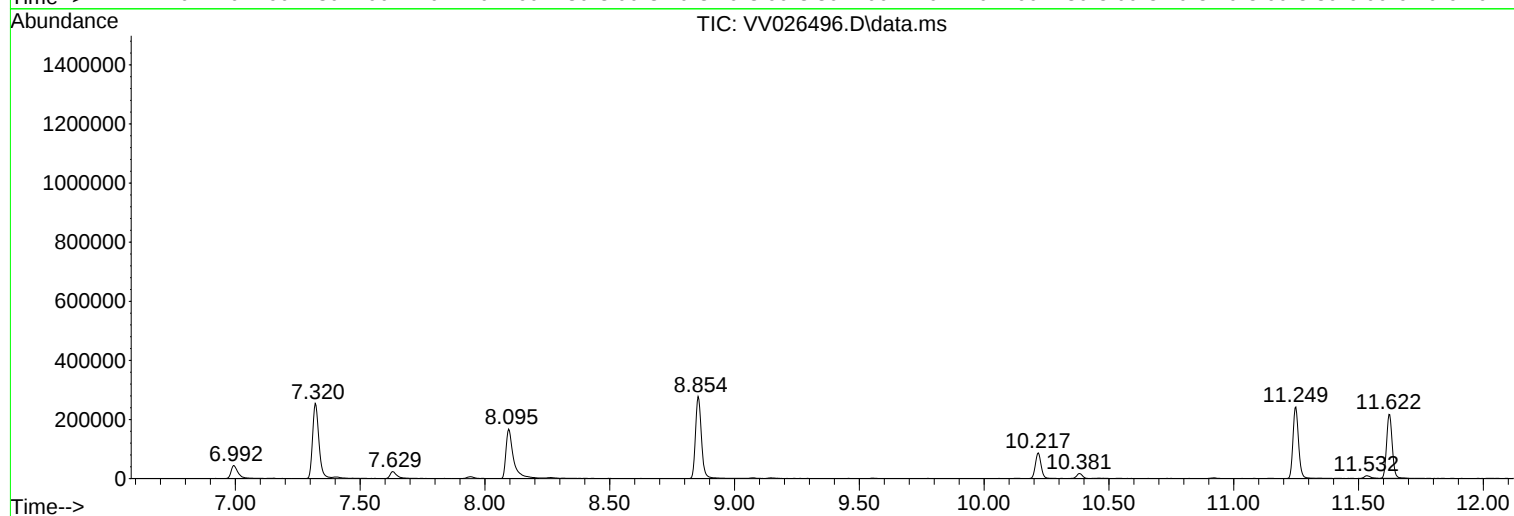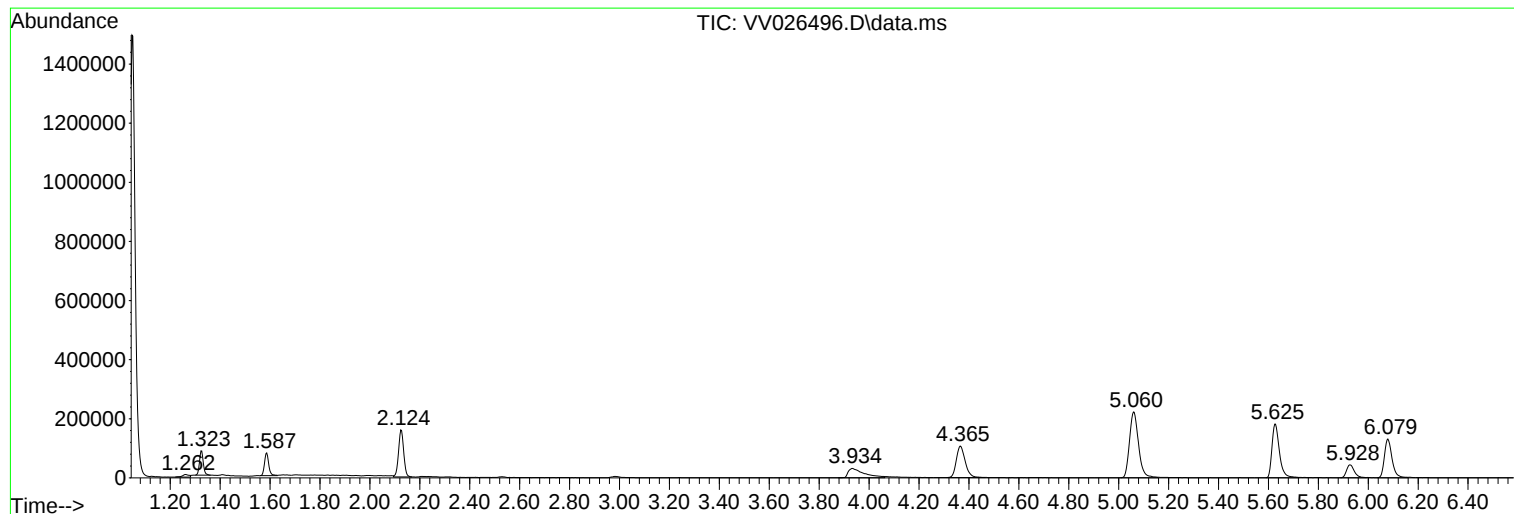

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026496.D
Acq On : 21 Jun 2022 18:14
Operator : SY/MD
Sample : N3355-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026496.D
Acq On : 21 Jun 2022 18:14
Operator : SY/MD
Sample : N3355-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY0C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
