


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062122\
Data File : VV026476.D
Acq On : 21 Jun 2022 08:54
Operator : SY/MD
Sample : BFB334
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB334

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jun 23 11:28:24 2022

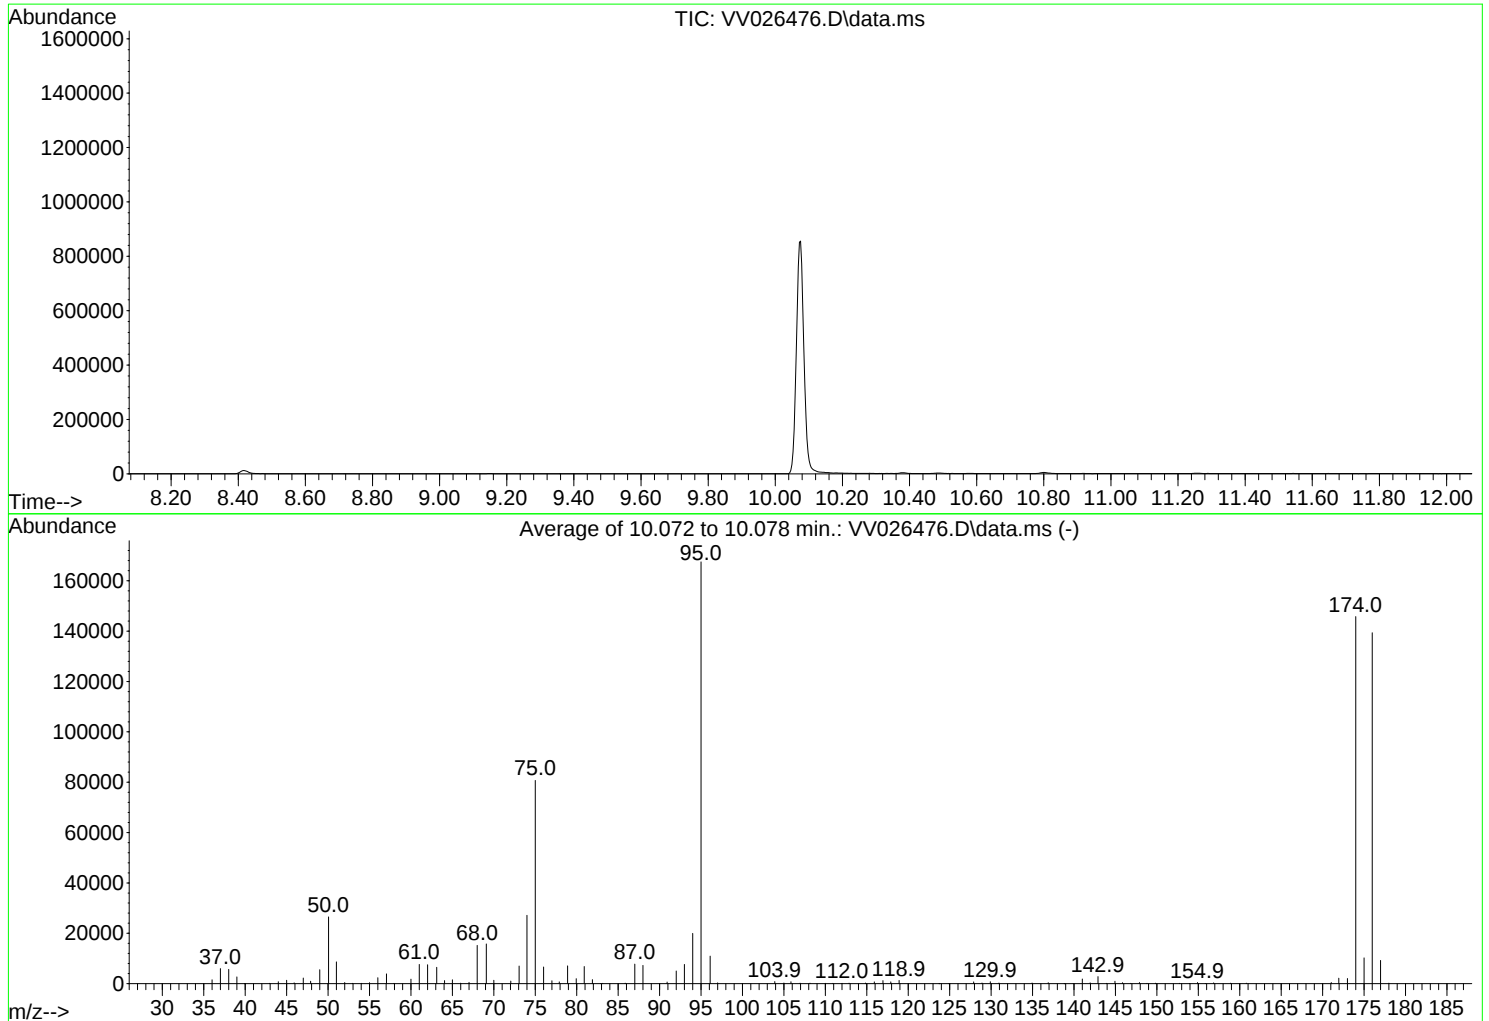

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	26488	PASS
75	95	30	80	48.2	80736	PASS
95	95	100	100	100.0	167531	PASS
96	95	5	9	6.5	10906	PASS
173	174	0.00	2	1.4	2016	PASS
174	95	50	120	87.0	145771	PASS
175	174	5	9	7.0	10239	PASS
176	174	95	105	95.6	139371	PASS
177	176	5	10	6.6	9253	PASS

m/z	Abundance
39.90	318.0
44.00	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

m/z	Abundance
36.00	1572.0
37.00	6234.0
38.00	5838.0
39.00	2787.0
40.00	398.0
43.00	147.0
44.00	1193.0
45.00	1482.0
45.90	304.0
47.00	2221.0
47.90	1017.0
49.00	5938.0
50.10	27736.0
51.00	9235.0
52.00	489.0
53.00	141.0
54.00	134.0
55.00	373.0
56.00	2423.0
57.10	4031.0
58.00	171.0
60.00	1903.0
61.00	8003.0
62.00	7901.0
63.10	6843.0
64.10	1260.0
65.00	1599.0
66.00	191.0
67.00	478.0
68.00	16363.0
69.10	16624.0
70.00	1311.0
72.00	1061.0
73.10	7251.0
74.00	28504.0
75.00	83536.0
76.00	7053.0
77.00	1206.0
77.90	708.0
78.90	7471.0
80.00	1950.0
80.90	7203.0
81.90	1594.0
83.20	222.0
85.90	200.0
87.00	8096.0
88.00	7796.0
90.90	690.0
92.00	5325.0
93.00	7776.0
94.00	20416.0
95.00	171904.0
96.10	11533.0
97.00	286.0
103.90	824.0
105.00	268.0
105.80	799.0
106.90	171.0
108.10	192.0
110.00	132.0
110.90	182.0
111.90	177.0
112.80	176.0
115.00	251.0
115.90	698.0
116.90	1368.0
117.90	787.0
118.90	1234.0
127.90	681.0
128.90	322.0
129.90	750.0
131.00	275.0
135.00	283.0
136.90	310.0
138.80	111.0
141.00	1982.0
142.00	304.0
142.90	2857.0
143.90	167.0
144.90	1140.0
145.90	364.0
146.80	104.0
147.90	440.0
148.80	123.0
149.80	169.0
152.70	176.0
154.00	127.0
154.90	425.0
155.80	140.0
156.90	328.0
158.90	207.0
160.80	208.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

171.10	451.0
172.00	2015.0
173.00	1984.0
174.00	148608.0
175.00	10516.0
176.00	141056.0
177.00	9716.0
178.10	217.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

m/z	Abundance
36.00	1560.0
37.00	6222.0
38.00	5801.0
39.00	2681.0
39.90	328.0
43.00	126.0
44.00	1151.0
45.00	1383.0
45.90	307.0
47.00	2335.0
47.90	957.0
49.00	5755.0
50.00	27400.0
51.00	8957.0
52.00	482.0
53.00	163.0
54.10	155.0
55.00	411.0
56.00	2438.0
57.10	4005.0
57.90	170.0
60.00	1830.0
61.00	7943.0
62.00	7814.0
63.10	6752.0
64.00	1261.0
65.00	1566.0
66.00	196.0
67.00	430.0
68.00	15701.0
69.10	16271.0
70.00	1428.0
72.00	1034.0
73.10	7188.0
74.00	28008.0
75.00	83776.0
76.00	6893.0
77.00	1165.0
77.90	721.0
78.90	7298.0
79.90	2024.0
80.90	7002.0
81.90	1608.0
83.10	178.0
85.80	208.0
87.00	8021.0
88.00	7490.0
90.90	670.0
92.00	5211.0
93.00	7981.0
94.00	20632.0
95.00	173696.0
96.10	11285.0
97.00	321.0
103.90	841.0
105.00	264.0
105.80	767.0
107.00	191.0
108.20	197.0
110.00	140.0
110.90	147.0
112.00	163.0
112.90	210.0
114.80	254.0
115.90	766.0
116.90	1255.0
117.90	708.0
118.90	1297.0
127.90	699.0
128.90	279.0
129.90	818.0
131.00	259.0
134.90	289.0
136.90	393.0
139.90	112.0
141.00	1916.0
142.00	310.0
142.90	2920.0
144.00	152.0
144.90	982.0
145.80	397.0
146.90	114.0
147.90	494.0
148.80	122.0
149.80	199.0
152.70	183.0
153.90	121.0
154.90	450.0
155.90	101.0
156.80	350.0
158.90	226.0
160.80	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

171.10	434.0
172.00	2232.0
173.00	2138.0
174.00	150848.0
175.00	10621.0
176.00	144128.0
177.00	9560.0
178.00	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

m/z	Abundance
36.00	1456.0
37.00	5560.0
38.00	5310.0
39.00	2472.0
40.00	278.0
42.90	102.0
44.00	1039.0
45.00	1242.0
45.90	262.0
47.00	2072.0
47.90	813.0
49.00	4996.0
50.00	24328.0
51.00	7795.0
52.00	432.0
52.90	196.0
54.10	146.0
55.00	401.0
56.00	2163.0
57.00	3545.0
57.90	142.0
60.00	1547.0
61.00	6989.0
62.00	6877.0
63.10	5835.0
64.00	1110.0
65.00	1430.0
66.00	172.0
66.90	347.0
67.10	343.0
68.00	13600.0
69.10	14447.0
70.00	1292.0
72.10	906.0
73.00	6520.0
74.00	24960.0
75.00	74896.0
76.00	5989.0
77.00	1021.0
77.90	714.0
78.90	6403.0
79.90	1887.0
80.90	6219.0
81.90	1498.0
82.90	136.0
85.80	200.0
87.00	7212.0
88.00	6433.0
90.90	583.0
92.00	4522.0
93.00	7183.0
94.00	18880.0
95.00	156992.0
96.10	9901.0
97.00	327.0
103.90	742.0
105.00	235.0
105.90	703.0
107.00	175.0
108.20	193.0
110.00	134.0
110.90	118.0
112.10	135.0
112.90	222.0
114.80	228.0
115.90	668.0
117.00	1108.0
117.90	600.0
118.90	1223.0
123.70	113.0
124.90	105.0
127.90	657.0
128.90	235.0
129.90	767.0
130.90	273.0
134.90	268.0
136.90	358.0
139.90	101.0
141.00	1633.0
141.90	282.0
142.90	2692.0
143.90	135.0
145.00	740.0
145.80	365.0
146.80	112.0
147.90	485.0
148.80	113.0
149.90	181.0
152.80	136.0
154.90	397.0
156.80	351.0
158.90	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334

160.80	177.0
171.00	388.0
171.90	2181.0
173.00	1926.0
174.00	137856.0
175.00	9581.0
176.00	132928.0
177.00	8482.0
177.90	225.0

Instrument :
MSVOA_V
ClientSampleId :
BFB334