

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031601.D
 Acq On : 21 Jun 2023 12:08
 Operator : SY/MD
 Sample : VV0621WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031601.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	97	rVB	117041	124770	14.01%	1.897%
2	1.539	148	155	171	rVB	98484	119738	13.45%	1.820%
3	2.063	308	318	336	rBV	206772	304998	34.25%	4.636%
4	2.253	368	377	384	rBV3	1781	2703	0.30%	0.041%
5	2.355	406	409	413	rVB4	677	536	0.06%	0.008%
6	2.455	431	440	454	rVB2	6716	11624	1.31%	0.177%
7	2.507	454	456	458	rBV2	183	120	0.01%	0.002%
8	2.709	514	519	521	rBV3	708	544	0.06%	0.008%
9	2.761	532	535	538	rBV	252	154	0.02%	0.002%
10	2.838	556	559	563	rBV2	384	363	0.04%	0.006%
11	2.950	591	594	595	rBV2	254	133	0.01%	0.002%
12	3.079	631	634	636	rBV2	283	136	0.02%	0.002%
13	3.108	641	643	647	rVB	185	143	0.02%	0.002%
14	3.130	647	650	652	rBV	174	99	0.01%	0.002%
15	3.143	652	654	656	rBV	241	145	0.02%	0.002%
16	3.217	675	677	681	rBV2	263	237	0.03%	0.004%
17	3.285	695	698	699	rBV	131	75	0.01%	0.001%
18	3.359	718	721	722	rBV	154	90	0.01%	0.001%
19	3.391	727	731	732	rBV	172	138	0.02%	0.002%
20	3.407	735	736	739	rBV	138	65	0.01%	0.001%
21	3.433	741	744	747	rBV	291	196	0.02%	0.003%
22	3.545	776	779	781	rBV	191	118	0.01%	0.002%
23	3.590	790	793	797	rVB	273	177	0.02%	0.003%
24	3.606	797	798	801	rBV	238	122	0.01%	0.002%
25	3.626	801	804	808	rVV	340	240	0.03%	0.004%
26	3.683	818	822	824	rBV	153	100	0.01%	0.002%
27	3.802	849	859	894	rBV2	61202	186433	20.94%	2.834%
28	4.256	984	1000	1039	rBV	140848	376598	42.29%	5.724%
29	4.555	1086	1093	1095	rBV3	421	481	0.05%	0.007%
30	4.667	1124	1128	1130	rBV2	386	261	0.03%	0.004%
31	4.706	1135	1140	1142	rBV	395	270	0.03%	0.004%
32	4.963	1201	1220	1246	rBV2	333579	890508	100.00%	13.536%
33	5.359	1339	1343	1345	rBV2	338	254	0.03%	0.004%
34	5.442	1367	1369	1372	rVB	234	94	0.01%	0.001%
35	5.484	1378	1382	1385	rBV3	271	230	0.03%	0.003%
36	5.539	1387	1399	1431	rBV	247588	510778	57.36%	7.764%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031601.D
 Acq On : 21 Jun 2023 12:08
 Operator : SY/MD
 Sample : VV0621WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.831	1482	1490	1491	rBV4	1855	1912	0.21%	0.029%
38	5.941	1522	1524	1527	rBV	214	140	0.02%	0.002%
39	5.992	1527	1540	1562	rBV	198902	412198	46.29%	6.266%
40	6.201	1603	1605	1608	rBV2	412	219	0.02%	0.003%
41	6.410	1667	1670	1672	rBV2	262	132	0.01%	0.002%
42	6.455	1681	1684	1687	rBV	269	224	0.03%	0.003%
43	6.568	1715	1719	1720	rBV	387	238	0.03%	0.004%
44	6.606	1728	1731	1737	rBV3	265	250	0.03%	0.004%
45	6.696	1757	1759	1760	rBV	207	108	0.01%	0.002%
46	6.760	1777	1779	1784	rBV2	266	233	0.03%	0.004%
47	6.812	1793	1795	1798	rBV	137	75	0.01%	0.001%
48	6.918	1816	1828	1848	rBV	83549	154165	17.31%	2.343%
49	7.166	1901	1905	1906	rBV2	330	265	0.03%	0.004%
50	7.249	1919	1931	1960	rBV	355714	633329	71.12%	9.627%
51	7.503	2008	2010	2012	rVB2	266	64	0.01%	0.001%
52	7.558	2017	2027	2055	rBV2	60382	111696	12.54%	1.698%
53	7.757	2086	2089	2091	rBV2	268	151	0.02%	0.002%
54	7.789	2096	2099	2100	rBV	225	161	0.02%	0.002%
55	7.873	2120	2125	2127	rBV4	413	410	0.05%	0.006%
56	7.918	2135	2139	2143	rVB4	396	300	0.03%	0.005%
57	7.985	2156	2160	2163	rBV	212	171	0.02%	0.003%
58	8.030	2163	2174	2199	rBV	201976	363769	40.85%	5.529%
59	8.365	2272	2278	2292	rVB3	6311	10338	1.16%	0.157%
60	8.600	2345	2351	2352	rBV	287	290	0.03%	0.004%
61	8.709	2382	2385	2386	rBV	317	181	0.02%	0.003%
62	8.728	2389	2391	2392	rBV	168	61	0.01%	0.001%
63	8.789	2399	2410	2434	rBV	376126	617789	69.37%	9.391%
64	9.014	2476	2480	2482	rBV	293	177	0.02%	0.003%
65	9.027	2482	2484	2487	rBV2	303	201	0.02%	0.003%
66	9.088	2498	2503	2504	rBV	455	353	0.04%	0.005%
67	9.249	2551	2553	2557	rBV	289	230	0.03%	0.003%
68	9.297	2565	2568	2570	rBV2	281	212	0.02%	0.003%
69	9.416	2603	2605	2609	rVB	294	185	0.02%	0.003%
70	9.490	2623	2628	2632	rBV2	410	539	0.06%	0.008%
71	9.741	2704	2706	2708	rVB	345	165	0.02%	0.003%
72	9.764	2708	2713	2717	rBV2	373	427	0.05%	0.006%
73	9.908	2756	2758	2759	rBV	171	71	0.01%	0.001%
74	10.014	2788	2791	2792	rBV	258	179	0.02%	0.003%
75	10.092	2811	2815	2818	rBV	310	294	0.03%	0.004%
76	10.159	2824	2836	2861	rBV	285660	460088	51.67%	6.994%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031601.D
 Acq On : 21 Jun 2023 12:08
 Operator : SY/MD
 Sample : VV0621WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK360

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	10.455	2925	2928	2933	rBV	230	230	0.03%	0.003%
78	10.481	2933	2936	2941	rBV2	537	526	0.06%	0.008%
79	10.693	3001	3002	3004	rBV	115	62	0.01%	0.001%
80	10.828	3041	3044	3046	rBV	281	180	0.02%	0.003%
81	10.927	3073	3075	3079	rBV	275	153	0.02%	0.002%
82	10.963	3083	3086	3088	rBV	208	160	0.02%	0.002%
83	11.127	3130	3137	3146	rVB4	1635	2470	0.28%	0.038%
84	11.191	3146	3157	3179	rBV	384424	590263	66.28%	8.972%
85	11.403	3220	3223	3226	rBV2	454	284	0.03%	0.004%
86	11.564	3262	3273	3296	rBV	389497	609152	68.41%	9.259%
87	11.953	3393	3394	3395	rBV	201	61	0.01%	0.001%
88	12.017	3408	3414	3418	rBV3	411	466	0.05%	0.007%
89	12.268	3489	3492	3493	rBV3	304	167	0.02%	0.003%
90	12.371	3521	3524	3526	rBV	754	532	0.06%	0.008%
91	12.442	3544	3546	3549	rBV2	299	161	0.02%	0.002%
92	12.590	3588	3592	3603	rVB5	3143	4014	0.45%	0.061%
93	12.918	3691	3694	3695	rBV	265	170	0.02%	0.003%
94	13.207	3775	3784	3793	rBV5	6520	10169	1.14%	0.155%
95	13.394	3840	3842	3847	rBV2	351	280	0.03%	0.004%
96	13.445	3850	3858	3875	rVB	23879	37497	4.21%	0.570%
97	13.689	3924	3934	3943	rBV4	9977	14859	1.67%	0.226%
98	13.934	4008	4010	4013	rBV	474	379	0.04%	0.006%
99	14.037	4040	4042	4045	rBV	318	221	0.02%	0.003%
100	14.197	4089	4092	4097	rBV3	615	666	0.07%	0.010%




Sum of corrected areas: 6578783

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031601.D
Acq On : 21 Jun 2023 12:08
Operator : SY/MD
Sample : VV0621WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

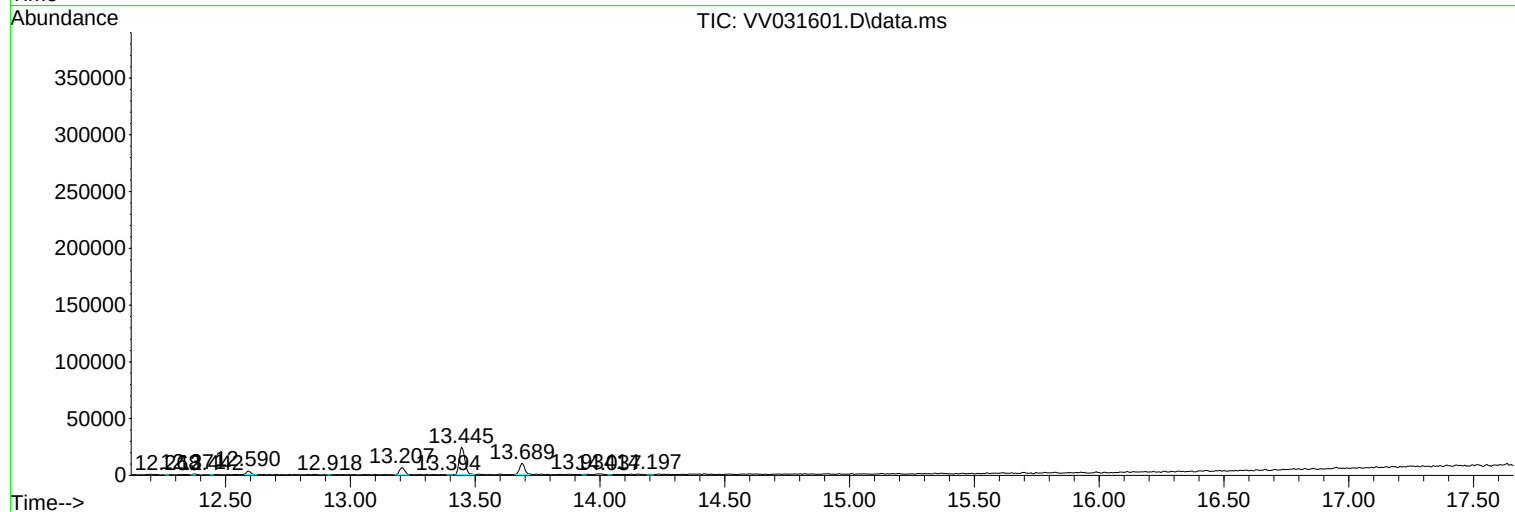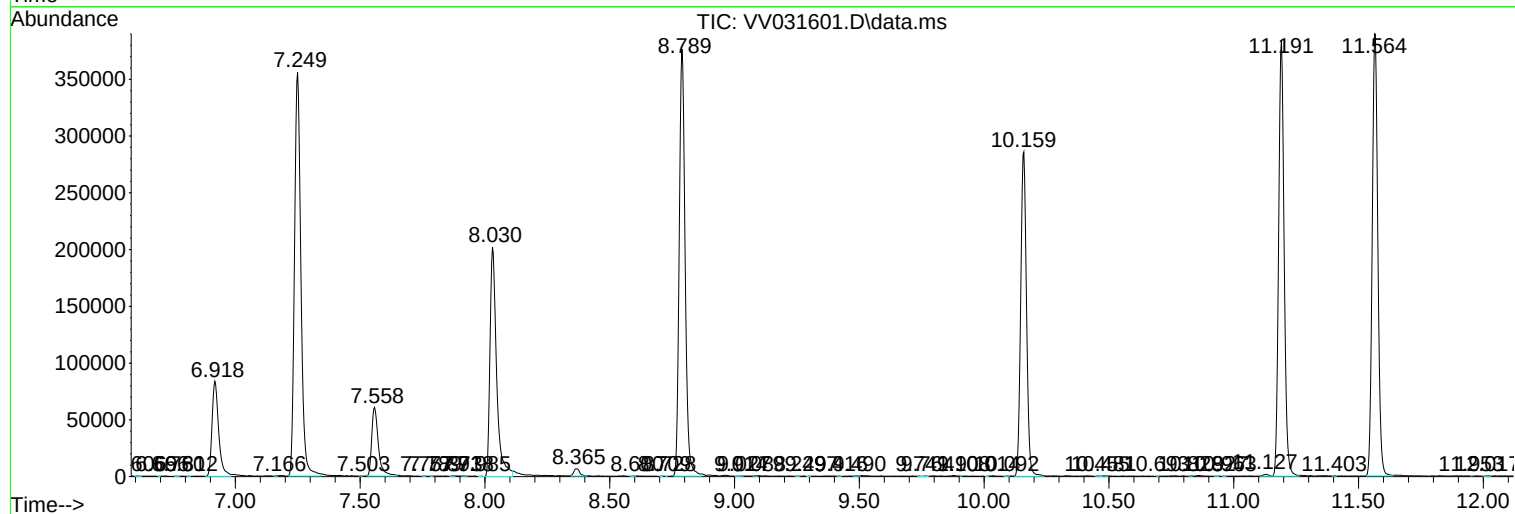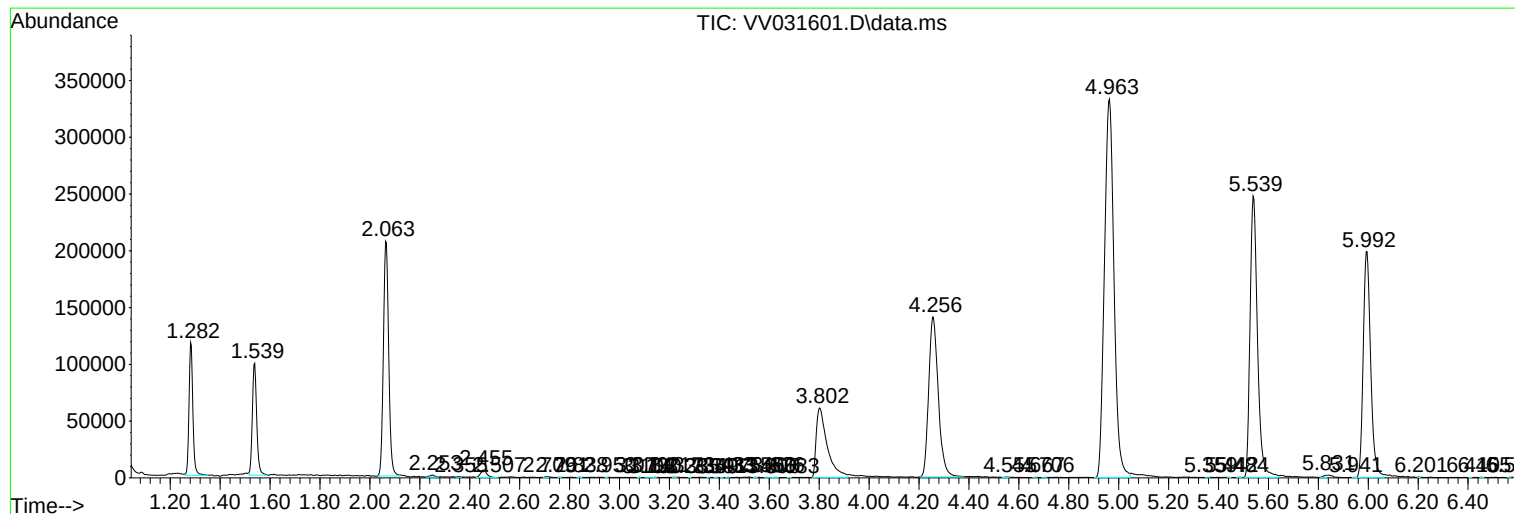

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031601.D
Acq On : 21 Jun 2023 12:08
Operator : SY/MD
Sample : VV0621WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031601.D
Acq On : 21 Jun 2023 12:08
Operator : SY/MD
Sample : VV0621WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK360

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------