

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031602.D
 Acq On : 21 Jun 2023 12:31
 Operator : SY/MD
 Sample : VV0621MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	93	rVB	112860	121543	13.89%	1.901%
2	1.535	147	154	167	rVB	97807	116305	13.29%	1.819%
3	2.066	308	319	336	rBV	201780	297142	33.96%	4.646%
4	2.397	420	422	423	rBV	173	64	0.01%	0.001%
5	2.458	432	441	452	rVB3	6642	11419	1.31%	0.179%
6	2.506	454	456	459	rVV	303	149	0.02%	0.002%
7	2.535	462	465	467	rVB	364	173	0.02%	0.003%
8	2.564	467	474	479	rVB3	834	1218	0.14%	0.019%
9	2.590	479	482	486	rBV3	271	241	0.03%	0.004%
10	2.706	516	518	522	rVB2	347	251	0.03%	0.004%
11	2.764	530	536	537	rBV2	270	271	0.03%	0.004%
12	2.809	545	550	551	rBV	250	214	0.02%	0.003%
13	2.870	566	569	571	rBV	79	62	0.01%	0.001%
14	2.879	571	572	573	rVB	119	23	0.00%	0.000%
15	2.892	573	576	577	rBV	215	100	0.01%	0.002%
16	2.976	599	602	604	rBV	211	112	0.01%	0.002%
17	3.088	634	637	641	rBV2	216	190	0.02%	0.003%
18	3.201	670	672	675	rBV	164	92	0.01%	0.001%
19	3.246	683	686	689	rVB2	219	148	0.02%	0.002%
20	3.265	689	692	694	rBV	242	140	0.02%	0.002%
21	3.314	699	707	711	rBV2	283	340	0.04%	0.005%
22	3.362	718	722	724	rBV	213	136	0.02%	0.002%
23	3.375	724	726	728	rBV2	252	150	0.02%	0.002%
24	3.423	734	741	743	rBV2	228	248	0.03%	0.004%
25	3.436	743	745	748	rBV	117	38	0.00%	0.001%
26	3.455	748	751	754	rBV2	310	252	0.03%	0.004%
27	3.523	767	772	773	rBV2	223	145	0.02%	0.002%
28	3.613	796	800	801	rBV	284	193	0.02%	0.003%
29	3.654	811	813	817	rVB	110	64	0.01%	0.001%
30	3.670	817	818	821	rBV	108	38	0.00%	0.001%
31	3.683	821	822	825	rBV	114	71	0.01%	0.001%
32	3.715	828	832	833	rBV	238	154	0.02%	0.002%
33	3.748	840	842	845	rVB	200	87	0.01%	0.001%
34	3.799	845	858	894	rBV2	59677	182299	20.83%	2.851%
35	4.256	984	1000	1029	rBV	137176	372850	42.61%	5.830%
36	4.490	1069	1073	1075	rBV2	345	327	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031602.D
 Acq On : 21 Jun 2023 12:31
 Operator : SY/MD
 Sample : VV0621MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	4.596	1103	1106	1110	rVB2	443	373	0.04%	0.006%
38	4.715	1141	1143	1146	rBV	122	52	0.01%	0.001%
39	4.754	1153	1155	1160	rVB	196	83	0.01%	0.001%
40	4.892	1196	1198	1199	rBV	213	89	0.01%	0.001%

41	4.963	1203	1220	1251	rBV2	326720	875014	100.00%	13.683%
42	5.330	1331	1334	1339	rVB3	272	227	0.03%	0.004%
43	5.355	1339	1342	1345	rBV2	299	188	0.02%	0.003%
44	5.381	1347	1350	1351	rBV	309	132	0.02%	0.002%
45	5.542	1387	1400	1420	rBV	236907	490204	56.02%	7.665%

46	5.789	1474	1477	1480	rBV	328	183	0.02%	0.003%
47	5.834	1484	1491	1496	rBV4	1724	2579	0.29%	0.040%
48	5.918	1515	1517	1522	rVB2	186	127	0.01%	0.002%
49	5.995	1527	1541	1559	rBV	194191	405680	46.36%	6.344%
50	6.211	1606	1608	1613	rVB2	296	154	0.02%	0.002%

51	6.233	1613	1615	1620	rBV2	265	239	0.03%	0.004%
52	6.368	1654	1657	1659	rBV2	223	144	0.02%	0.002%
53	6.497	1693	1697	1698	rBV	127	63	0.01%	0.001%
54	6.641	1737	1742	1744	rBV	153	161	0.02%	0.003%
55	6.786	1784	1787	1790	rBV2	337	269	0.03%	0.004%

56	6.799	1790	1791	1799	rVB2	270	219	0.03%	0.003%
57	6.918	1818	1828	1855	rBV	79923	149960	17.14%	2.345%
58	7.182	1908	1910	1919	rVB3	692	832	0.10%	0.013%
59	7.249	1919	1931	1964	rBV	349021	618918	70.73%	9.678%
60	7.558	2017	2027	2044	rBV	61298	109190	12.48%	1.707%

61	7.783	2096	2097	2099	rBV	269	130	0.01%	0.002%
62	7.828	2108	2111	2117	rVB3	341	270	0.03%	0.004%
63	7.953	2147	2150	2151	rBV	232	108	0.01%	0.002%
64	8.030	2163	2174	2212	rBV	196444	362531	41.43%	5.669%
65	8.365	2271	2278	2295	rVB3	6885	12221	1.40%	0.191%

66	8.516	2323	2325	2327	rBV	265	83	0.01%	0.001%
67	8.599	2349	2351	2354	rBV2	328	216	0.02%	0.003%
68	8.699	2380	2382	2385	rBV2	164	98	0.01%	0.002%
69	8.789	2398	2410	2441	rBV	376578	609932	69.71%	9.538%
70	8.956	2459	2462	2465	rBV	382	272	0.03%	0.004%

71	9.017	2479	2481	2483	rBV	208	77	0.01%	0.001%
72	9.030	2483	2485	2487	rVB	257	102	0.01%	0.002%
73	9.181	2529	2532	2535	rBV	416	272	0.03%	0.004%
74	9.516	2634	2636	2638	rVB	315	112	0.01%	0.002%
75	9.564	2646	2651	2654	rBV2	374	317	0.04%	0.005%

76	9.947	2768	2770	2772	rVB	210	91	0.01%	0.001%
----	-------	------	------	------	-----	-----	----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031602.D
 Acq On : 21 Jun 2023 12:31
 Operator : SY/MD
 Sample : VV0621MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	9.966	2772	2776	2780	rBV2	298	265	0.03%	0.004%
78	10.159	2824	2836	2857	rBV	286933	454586	51.95%	7.108%
79	10.329	2881	2889	2892	rBV	651	824	0.09%	0.013%
80	10.419	2914	2917	2919	rBV2	210	157	0.02%	0.002%
81	10.452	2924	2927	2929	rBV	174	150	0.02%	0.002%
82	10.731	3010	3014	3016	rBV2	306	219	0.03%	0.003%
83	10.744	3016	3018	3019	rBV	319	136	0.02%	0.002%
84	10.786	3029	3031	3032	rBV	159	66	0.01%	0.001%
85	11.130	3134	3138	3143	rVB4	646	695	0.08%	0.011%
86	11.191	3145	3157	3179	rBV	378666	577274	65.97%	9.027%
87	11.365	3208	3211	3214	rVB2	387	222	0.03%	0.003%
88	11.500	3245	3253	3256	rBV2	337	500	0.06%	0.008%
89	11.564	3262	3273	3297	rBV	378841	598151	68.36%	9.353%
90	11.853	3361	3363	3366	rVB	315	106	0.01%	0.002%
91	11.966	3396	3398	3400	rBV2	240	110	0.01%	0.002%
92	12.345	3513	3516	3518	rBV2	366	239	0.03%	0.004%
93	12.429	3539	3542	3546	rBV	366	266	0.03%	0.004%
94	12.590	3587	3592	3598	rBV2	926	1081	0.12%	0.017%
95	13.017	3722	3725	3726	rBV	380	269	0.03%	0.004%
96	13.210	3778	3785	3792	rBV4	1940	2762	0.32%	0.043%
97	13.451	3854	3860	3870	rVB3	4822	7396	0.85%	0.116%
98	14.033	4038	4041	4045	rBV3	435	399	0.05%	0.006%




Sum of corrected areas: 6395034

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031602.D
Acq On : 21 Jun 2023 12:31
Operator : SY/MD
Sample : VV0621MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK361

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

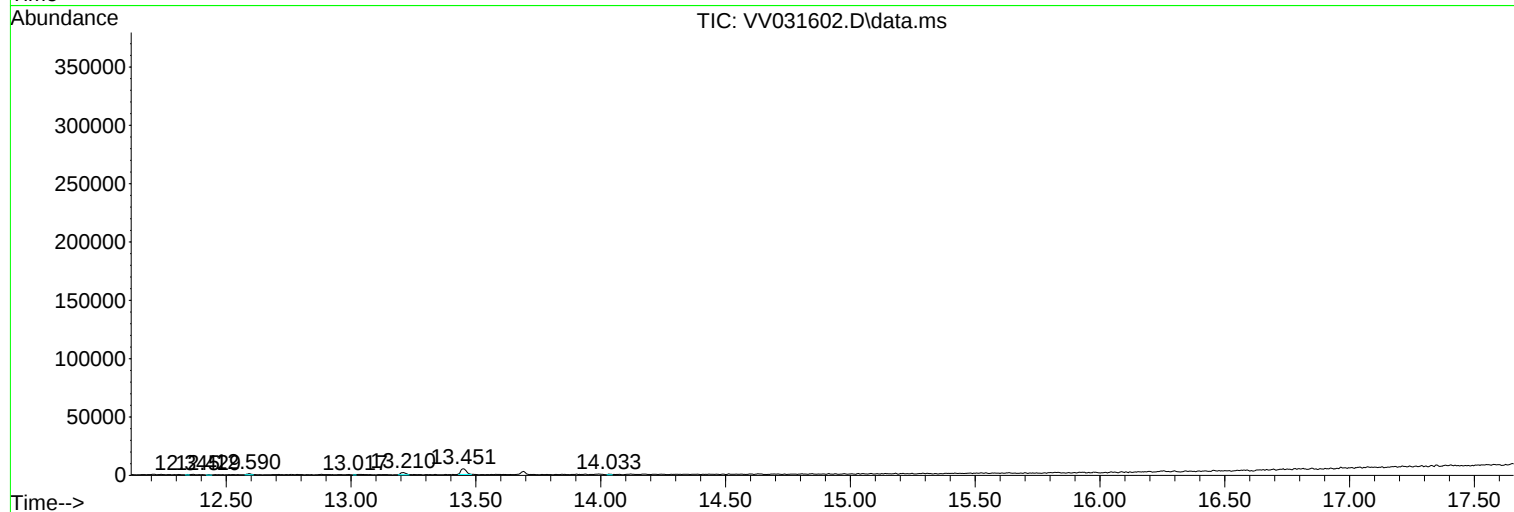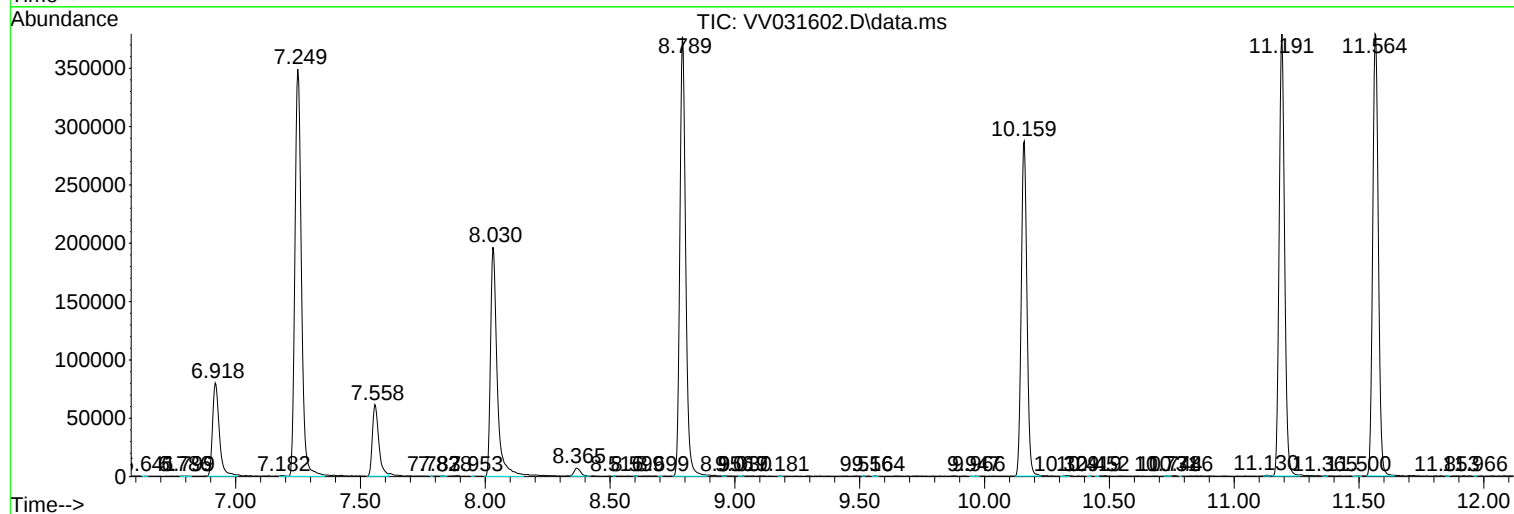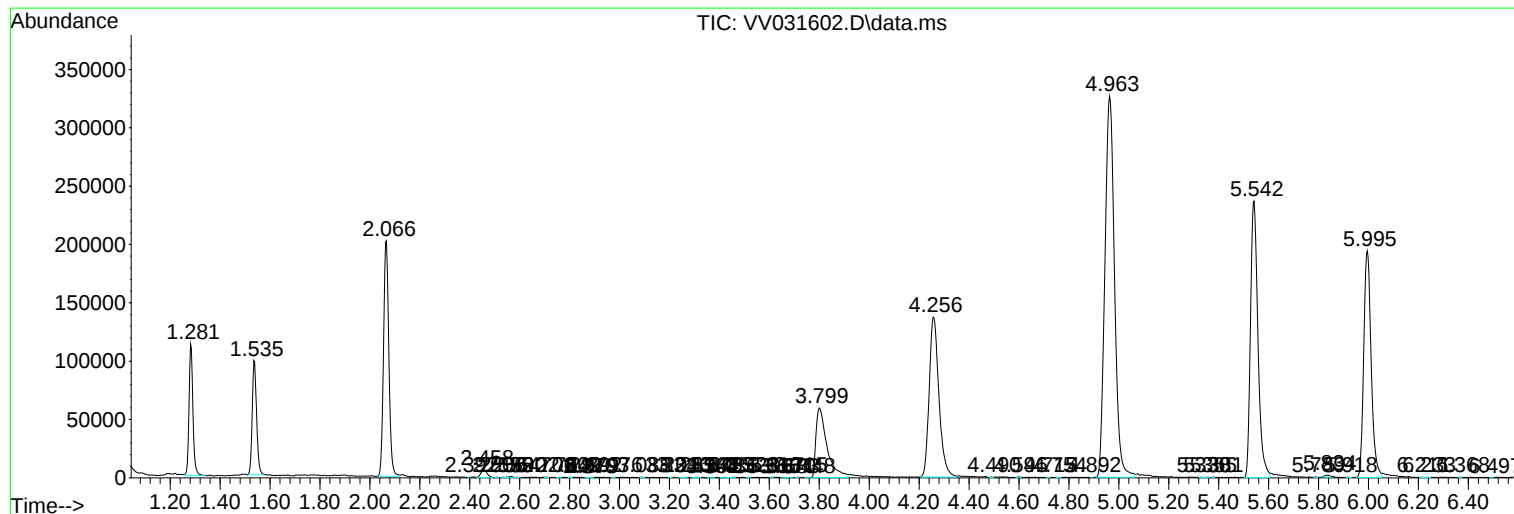

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031602.D
Acq On : 21 Jun 2023 12:31
Operator : SY/MD
Sample : VV0621MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK361

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031602.D
Acq On : 21 Jun 2023 12:31
Operator : SY/MD
Sample : VV0621MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK361

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------