

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031604.D
 Acq On : 21 Jun 2023 13:18
 Operator : SY/MD
 Sample : 03236-04ME
 Misc : 5.48g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBTY1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VV031604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	94	rVB	88565	118876	13.56%	1.691%
2	1.532	147	153	169	rBV	46401	70217	8.01%	0.999%
3	2.047	303	313	331	rBV	218670	318809	36.38%	4.536%
4	2.445	430	437	452	rBV3	2395	4765	0.54%	0.068%
5	2.510	454	457	461	rBV3	342	272	0.03%	0.004%
6	2.863	563	567	569	rBV	298	170	0.02%	0.002%
7	3.034	617	620	623	rBV	289	174	0.02%	0.002%
8	3.088	633	637	641	rBV2	219	269	0.03%	0.004%
9	3.317	705	708	715	rBV2	254	286	0.03%	0.004%
10	3.355	718	720	722	rBV	155	51	0.01%	0.001%
11	3.368	722	724	728	rBV	375	289	0.03%	0.004%
12	3.387	728	730	731	rBV	151	79	0.01%	0.001%
13	3.465	752	754	757	rVB2	288	169	0.02%	0.002%
14	3.484	757	760	763	rBV2	401	340	0.04%	0.005%
15	3.571	784	787	789	rBV2	159	102	0.01%	0.001%
16	3.674	817	819	821	rBV2	170	102	0.01%	0.001%
17	3.706	827	829	832	rBV	315	214	0.02%	0.003%
18	3.741	836	840	843	rBV	283	204	0.02%	0.003%
19	3.760	845	846	847	rVB	118	23	0.00%	0.000%
20	3.777	847	851	854	rBV2	204	171	0.02%	0.002%
21	3.822	854	865	906	rBV2	34255	142280	16.24%	2.024%
22	4.259	985	1001	1036	rBV2	115292	365022	41.65%	5.193%
23	4.494	1072	1074	1075	rVB	248	74	0.01%	0.001%
24	4.506	1075	1078	1079	rBV2	220	121	0.01%	0.002%
25	4.590	1101	1104	1107	rVB	327	210	0.02%	0.003%
26	4.706	1137	1140	1148	rBV2	269	304	0.03%	0.004%
27	4.738	1148	1150	1154	rBV2	159	118	0.01%	0.002%
28	4.895	1197	1199	1203	rBB2	137	58	0.01%	0.001%
29	4.960	1203	1219	1253	rBV2	343349	876366	100.00%	12.468%
30	5.278	1316	1318	1320	rBV2	359	203	0.02%	0.003%
31	5.538	1387	1399	1429	rBV	298983	644618	73.56%	9.171%
32	5.841	1481	1493	1511	rBV3	61768	129974	14.83%	1.849%
33	5.995	1528	1541	1572	rBV	185033	399650	45.60%	5.686%
34	6.146	1585	1588	1594	rVB3	941	854	0.10%	0.012%
35	6.198	1602	1604	1606	rBV3	169	94	0.01%	0.001%
36	6.333	1643	1646	1648	rBV	279	143	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031604.D
 Acq On : 21 Jun 2023 13:18
 Operator : SY/MD
 Sample : 03236-04ME
 Misc : 5.48g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBTY1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.455	1683	1684	1685	rBV	108	30	0.00%	0.000%
38	6.465	1685	1687	1691	rVV2	246	141	0.02%	0.002%
39	6.558	1713	1716	1717	rBV2	177	85	0.01%	0.001%
40	6.571	1717	1720	1722	rVV	224	142	0.02%	0.002%
41	6.757	1775	1778	1781	rBV2	176	133	0.02%	0.002%
42	6.921	1818	1829	1851	rBV	93349	189141	21.58%	2.691%
43	7.140	1894	1897	1899	rBV2	304	209	0.02%	0.003%
44	7.249	1919	1931	1951	rBV	367824	662207	75.56%	9.421%
45	7.561	2018	2028	2063	rBV	63282	132007	15.06%	1.878%
46	7.728	2078	2080	2082	rBV	387	193	0.02%	0.003%
47	7.866	2120	2123	2125	rBV3	420	244	0.03%	0.003%
48	7.915	2129	2138	2150	rVB3	14575	25220	2.88%	0.359%
49	8.069	2170	2186	2214	rBV	128688	323946	36.96%	4.609%
50	8.397	2283	2288	2299	rVB5	1253	2072	0.24%	0.029%
51	8.596	2347	2350	2356	rBV2	187	208	0.02%	0.003%
52	8.792	2400	2411	2450	rBV	419273	788297	89.95%	11.215%
53	9.220	2542	2544	2548	rBV	255	176	0.02%	0.003%
54	9.596	2659	2661	2662	rBV	170	61	0.01%	0.001%
55	9.615	2663	2667	2670	rBV3	308	280	0.03%	0.004%
56	9.824	2730	2732	2735	rBV	161	89	0.01%	0.001%
57	9.870	2744	2746	2747	rBV	210	109	0.01%	0.002%
58	9.950	2767	2771	2773	rBV2	264	236	0.03%	0.003%
59	10.169	2827	2839	2861	rBV	264339	434218	49.55%	6.178%
60	10.320	2884	2886	2887	rBV	270	142	0.02%	0.002%
61	10.381	2902	2905	2908	rBV	211	158	0.02%	0.002%
62	10.448	2923	2926	2932	rVB2	260	220	0.03%	0.003%
63	10.490	2933	2939	2946	rBV3	477	747	0.09%	0.011%
64	10.648	2984	2988	2990	rBV2	429	310	0.04%	0.004%
65	10.802	3033	3036	3038	rBV	211	147	0.02%	0.002%
66	10.866	3053	3056	3059	rBV	407	311	0.04%	0.004%
67	10.921	3070	3073	3077	rBV2	351	295	0.03%	0.004%
68	10.940	3077	3079	3082	rBV2	295	198	0.02%	0.003%
69	11.197	3147	3159	3181	rBV	491541	767758	87.61%	10.923%
70	11.570	3263	3275	3294	rBV	395946	619883	70.73%	8.819%
71	11.741	3326	3328	3333	rBV3	384	331	0.04%	0.005%
72	12.545	3573	3578	3582	rBV	399	413	0.05%	0.006%
73	12.683	3619	3621	3624	rBV	341	209	0.02%	0.003%
74	13.455	3856	3861	3868	rVB3	1234	1540	0.18%	0.022%
75	13.850	3980	3984	3989	rBV3	703	738	0.08%	0.010%
76	14.291	4119	4121	4124	rBV2	519	250	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031604.D
Acq On : 21 Jun 2023 13:18
Operator : SY/MD
Sample : 03236-04ME
Misc : 5.48g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBTY1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis




Sum of corrected areas: 7028765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031604.D
Acq On : 21 Jun 2023 13:18
Operator : SY/MD
Sample : 03236-04ME
Misc : 5.48g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBTY1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

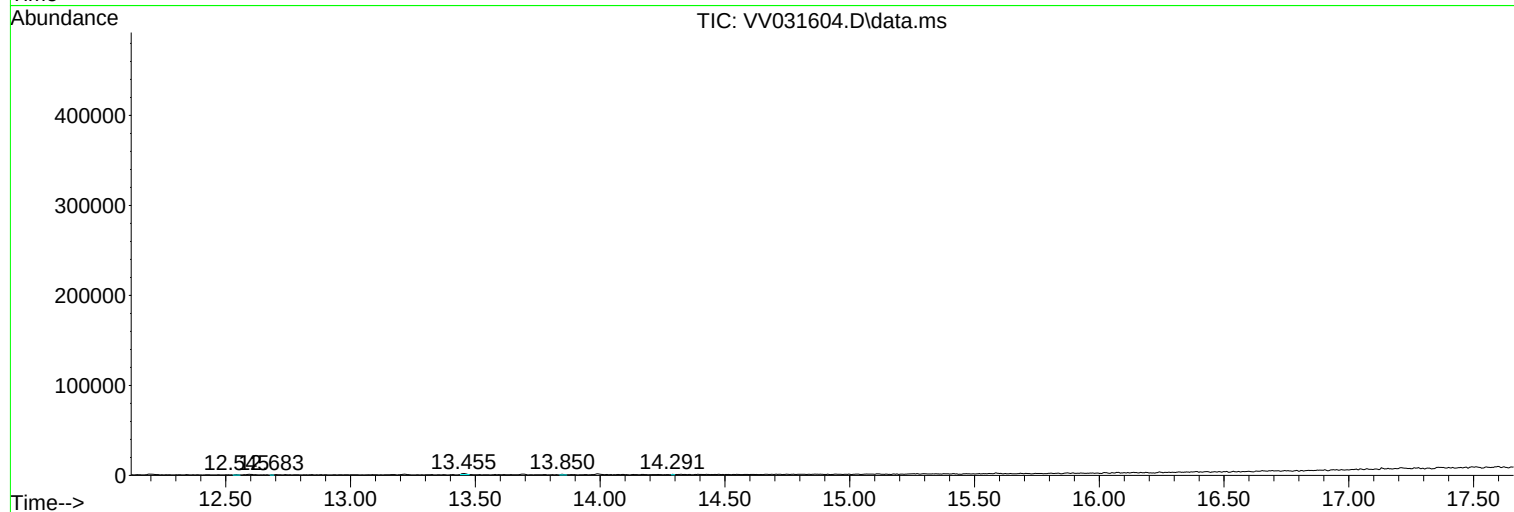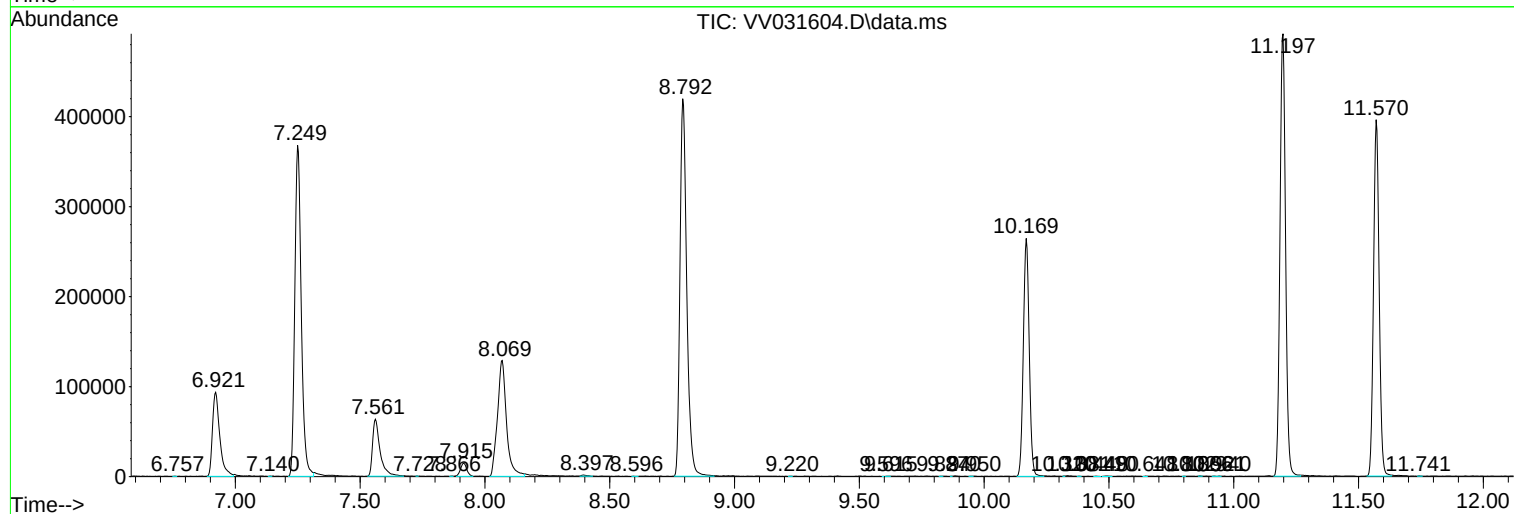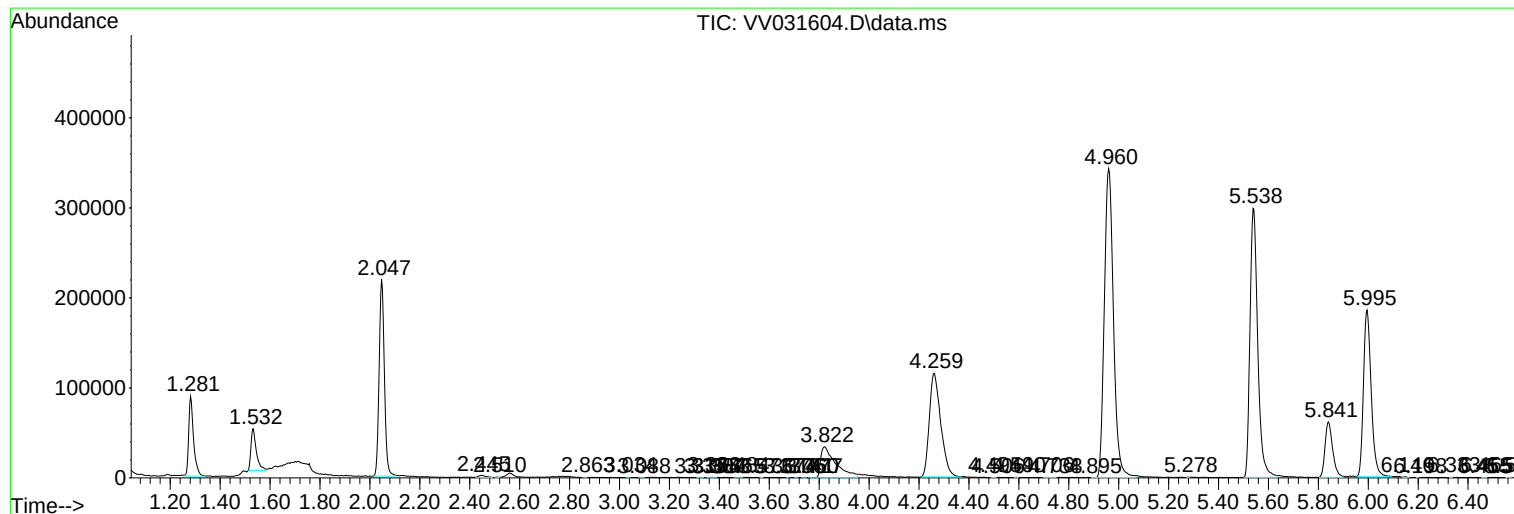

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031604.D
Acq On : 21 Jun 2023 13:18
Operator : SY/MD
Sample : 03236-04ME
Misc : 5.48g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBTY1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031604.D
Acq On : 21 Jun 2023 13:18
Operator : SY/MD
Sample : 03236-04ME
Misc : 5.48g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBTY1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------