

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031605.D
 Acq On : 21 Jun 2023 13:41
 Operator : SY/MD
 Sample : 03307-10ME
 Misc : 4.78g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBW11ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

Signal : TIC: VV031605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rBV	86026	112663	12.71%	1.627%
2	1.532	148	153	165	rVB	39286	54398	6.14%	0.785%
3	2.047	302	313	338	rBV2	246496	411735	46.44%	5.945%
4	2.863	565	567	572	rBV	319	229	0.03%	0.003%
5	2.892	572	576	577	rBV	287	209	0.02%	0.003%
6	2.992	603	607	608	rBV	245	166	0.02%	0.002%
7	3.117	636	646	658	rBV	3573	6773	0.76%	0.098%
8	3.198	669	671	673	rBV	186	78	0.01%	0.001%
9	3.227	677	680	683	rBV2	163	107	0.01%	0.002%
10	3.278	693	696	699	rBV	235	198	0.02%	0.003%
11	3.368	722	724	726	rBV2	153	87	0.01%	0.001%
12	3.407	735	736	737	rBV2	107	28	0.00%	0.000%
13	3.429	737	743	745	rBV3	334	316	0.04%	0.005%
14	3.468	753	755	756	rBV	185	75	0.01%	0.001%
15	3.481	756	759	765	rVV	197	259	0.03%	0.004%
16	3.506	765	767	770	rVB	139	56	0.01%	0.001%
17	3.580	787	790	793	rVB	184	125	0.01%	0.002%
18	3.703	827	828	834	rVB	197	174	0.02%	0.003%
19	3.738	834	839	840	rBV2	171	155	0.02%	0.002%
20	3.825	855	866	902	rBV	32452	137076	15.46%	1.979%
21	4.262	985	1002	1035	rBV3	115211	366845	41.38%	5.297%
22	4.455	1059	1062	1065	rBV	248	150	0.02%	0.002%
23	4.580	1098	1101	1105	rBV	262	231	0.03%	0.003%
24	4.613	1105	1111	1114	rVV3	423	391	0.04%	0.006%
25	4.641	1118	1120	1123	rBV	166	71	0.01%	0.001%
26	4.722	1142	1145	1146	rBV	154	88	0.01%	0.001%
27	4.786	1164	1165	1166	rBV	139	40	0.00%	0.001%
28	4.960	1202	1219	1248	rBV2	345028	886577	100.00%	12.802%
29	5.220	1298	1300	1302	rBV2	417	244	0.03%	0.004%
30	5.539	1387	1399	1430	rBV	292661	627634	70.79%	9.063%
31	5.834	1482	1491	1492	rBV5	1598	1898	0.21%	0.027%
32	5.902	1510	1512	1514	rVB	178	71	0.01%	0.001%
33	5.928	1516	1520	1521	rBV3	913	602	0.07%	0.009%
34	5.995	1528	1541	1574	rVB	185497	402094	45.35%	5.806%
35	6.143	1585	1587	1589	rBV2	524	284	0.03%	0.004%
36	6.194	1601	1603	1605	rBV	242	95	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062123\
 Data File : VW031605.D
 Acq On : 21 Jun 2023 13:41
 Operator : SY/MD
 Sample : 03307-10ME
 Misc : 4.78g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBW11ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	6.236	1614	1616	1618	rBV	270	116	0.01%	0.002%
38	6.355	1649	1653	1656	rBV2	280	249	0.03%	0.004%
39	6.442	1676	1680	1681	rBV	255	122	0.01%	0.002%
40	6.532	1706	1708	1710	rBV	258	189	0.02%	0.003%
41	6.612	1731	1733	1737	rBV	463	311	0.04%	0.004%
42	6.664	1747	1749	1752	rVB	219	78	0.01%	0.001%
43	6.677	1752	1753	1757	rBV2	145	74	0.01%	0.001%
44	6.825	1795	1799	1803	rBV	233	239	0.03%	0.003%
45	6.921	1818	1829	1859	rBV2	90866	189941	21.42%	2.743%
46	7.130	1892	1894	1896	rBV	346	224	0.03%	0.003%
47	7.162	1901	1904	1905	rBV	343	178	0.02%	0.003%
48	7.249	1919	1931	1958	rBV	369542	675435	76.18%	9.753%
49	7.500	2007	2009	2012	rBV	313	221	0.02%	0.003%
50	7.561	2018	2028	2054	rBV	64048	134508	15.17%	1.942%
51	7.780	2095	2096	2097	rBV	112	25	0.00%	0.000%
52	7.792	2098	2100	2105	rVV	159	91	0.01%	0.001%
53	7.866	2120	2123	2124	rBV	447	268	0.03%	0.004%
54	7.918	2135	2139	2140	rBV	270	224	0.03%	0.003%
55	8.069	2170	2186	2217	rBV	126114	327835	36.98%	4.734%
56	8.497	2316	2319	2320	rBV	313	127	0.01%	0.002%
57	8.522	2325	2327	2332	rVB2	221	125	0.01%	0.002%
58	8.545	2332	2334	2337	rBV2	321	170	0.02%	0.002%
59	8.651	2365	2367	2368	rBV2	197	77	0.01%	0.001%
60	8.792	2400	2411	2435	rBV	402828	775299	87.45%	11.195%
61	8.998	2473	2475	2481	rBV2	269	212	0.02%	0.003%
62	9.098	2501	2506	2510	rBV3	412	412	0.05%	0.006%
63	9.181	2529	2532	2537	rVB	279	177	0.02%	0.003%
64	9.220	2539	2544	2548	rBV2	267	277	0.03%	0.004%
65	9.339	2578	2581	2583	rBV	253	172	0.02%	0.002%
66	9.365	2586	2589	2590	rBV	79	39	0.00%	0.001%
67	9.432	2607	2610	2612	rBV2	360	218	0.02%	0.003%
68	9.673	2682	2685	2688	rBV	159	138	0.02%	0.002%
69	9.689	2688	2690	2692	rBV	187	133	0.02%	0.002%
70	9.776	2712	2717	2720	rBV2	354	370	0.04%	0.005%
71	9.866	2742	2745	2747	rBV	343	260	0.03%	0.004%
72	9.992	2781	2784	2787	rBV2	226	178	0.02%	0.003%
73	10.059	2802	2805	2808	rBV2	262	152	0.02%	0.002%
74	10.169	2826	2839	2858	rBV	259468	435002	49.07%	6.281%
75	10.480	2935	2936	2938	rBV	265	119	0.01%	0.002%
76	10.583	2962	2968	2969	rBV	217	252	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
 Data File : VV031605.D
 Acq On : 21 Jun 2023 13:41
 Operator : SY/MD
 Sample : 03307-10ME
 Misc : 4.78g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBW11ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M

Title : VOC Analysis

77	10.683	2996	2999	3003	rBV2	263	200	0.02%	0.003%
78	10.934	3074	3077	3078	rBV2	345	196	0.02%	0.003%
79	11.101	3126	3129	3131	rBV2	201	125	0.01%	0.002%
80	11.133	3136	3139	3140	rBV3	506	319	0.04%	0.005%
81	11.197	3147	3159	3182	rBV	475406	744934	84.02%	10.756%
82	11.570	3263	3275	3292	rBV	396383	622402	70.20%	8.987%
83	11.786	3340	3342	3344	rBV2	339	142	0.02%	0.002%
84	12.120	3442	3446	3451	rVB3	275	310	0.03%	0.004%
85	12.468	3552	3554	3558	rVB3	387	231	0.03%	0.003%
86	12.972	3708	3711	3713	rBV2	262	192	0.02%	0.003%




Sum of corrected areas: 6925510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031605.D
Acq On : 21 Jun 2023 13:41
Operator : SY/MD
Sample : 03307-10ME
Misc : 4.78g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBW11ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

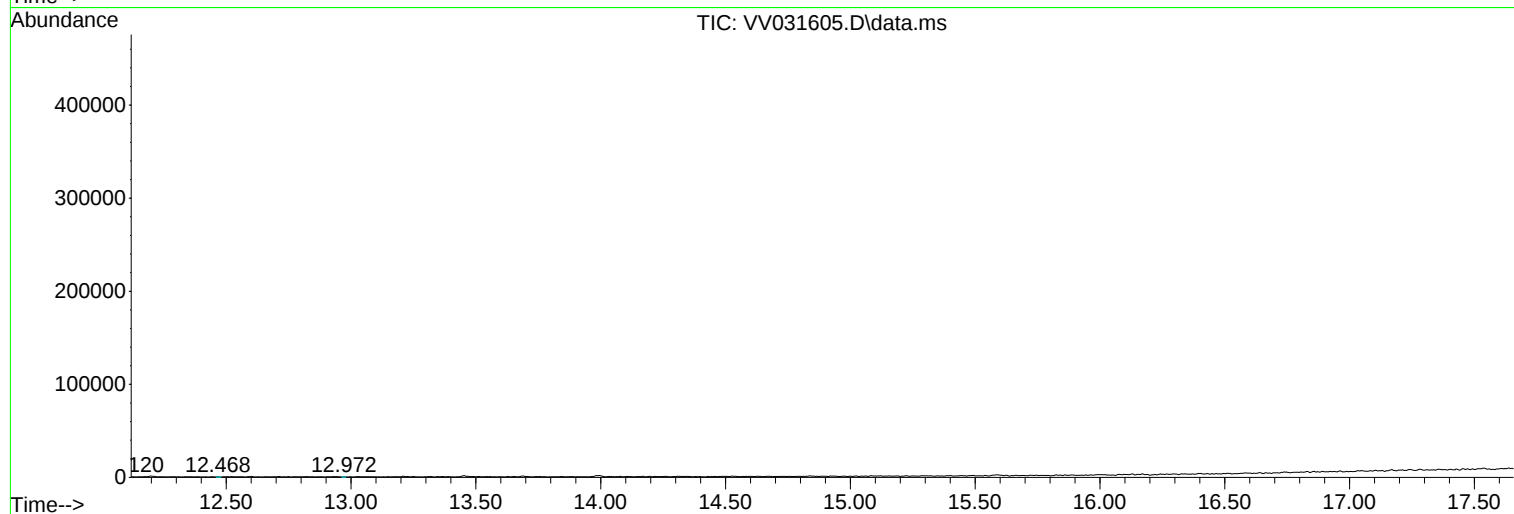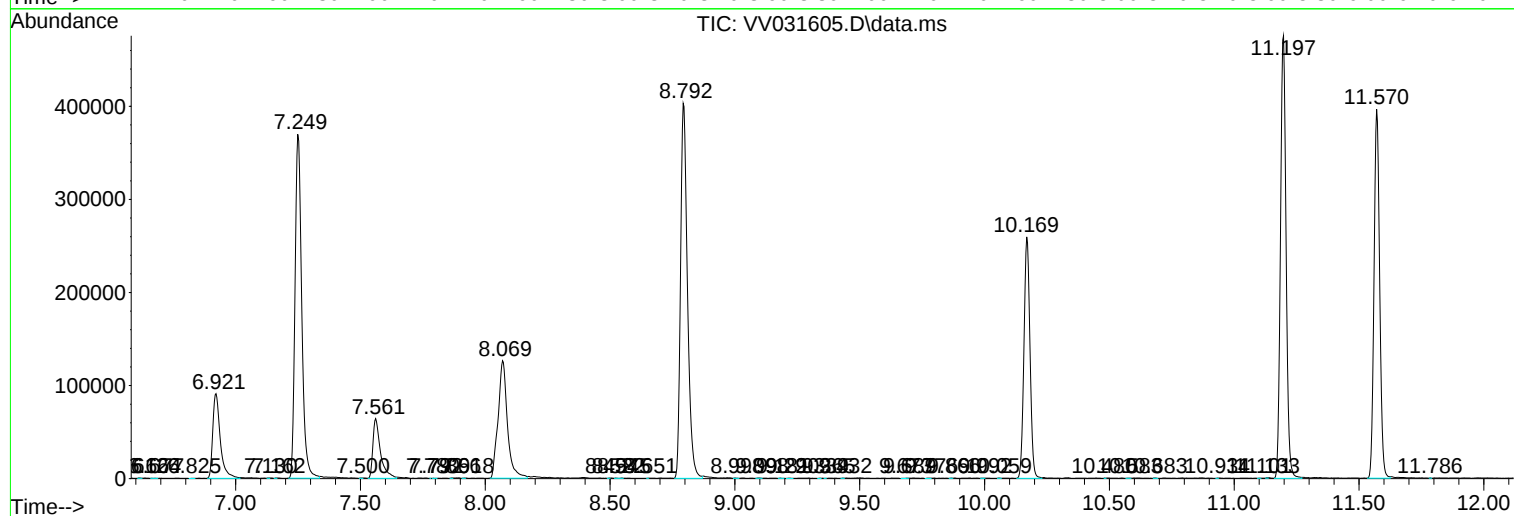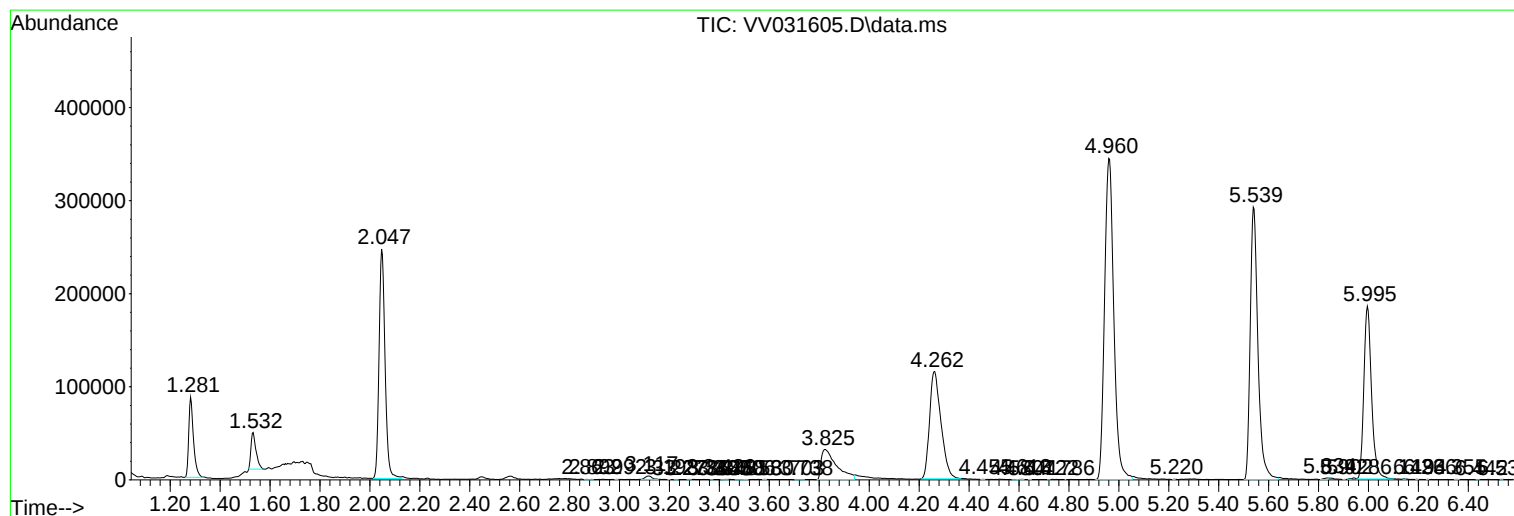

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031605.D
Acq On : 21 Jun 2023 13:41
Operator : SY/MD
Sample : 03307-10ME
Misc : 4.78g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBW11ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031605.D
Acq On : 21 Jun 2023 13:41
Operator : SY/MD
Sample : 03307-10ME
Misc : 4.78g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBW11ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------