

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062123\
 Data File : VW031606.D
 Acq On : 21 Jun 2023 14:06
 Operator : SY/MD
 Sample : 03334-07ME
 Misc : 5.36g/5.0mL/100uL/5.1mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBW02ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

Signal : TIC: VW031606.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	96	rVB	86857	122146	13.49%	1.726%
2	1.536	147	154	172	rBV	47724	82083	9.06%	1.160%
3	2.047	301	313	330	rBV2	237424	385717	42.59%	5.449%
4	2.233	366	371	378	rVB4	848	992	0.11%	0.014%
5	2.384	416	418	423	rVB2	373	281	0.03%	0.004%
6	2.445	430	437	447	rVV4	3455	5210	0.58%	0.074%
7	2.564	461	474	487	rBV2	5548	12306	1.36%	0.174%
8	2.651	499	501	504	rBV2	343	214	0.02%	0.003%
9	2.680	508	510	515	rVB	348	258	0.03%	0.004%
10	2.716	515	521	522	rBV	546	372	0.04%	0.005%
11	2.748	528	531	533	rBV3	473	395	0.04%	0.006%
12	2.783	538	542	545	rBV	850	791	0.09%	0.011%
13	2.802	545	548	551	rVV3	855	629	0.07%	0.009%
14	3.047	620	624	626	rBV2	281	248	0.03%	0.004%
15	3.076	631	633	636	rBV	274	199	0.02%	0.003%
16	3.111	640	644	646	rBV3	379	285	0.03%	0.004%
17	3.265	688	692	696	rBV3	365	325	0.04%	0.005%
18	3.323	707	710	715	rVB3	356	343	0.04%	0.005%
19	3.362	715	722	724	rBV	294	285	0.03%	0.004%
20	3.397	727	733	735	rVV2	313	375	0.04%	0.005%
21	3.410	735	737	741	rVV2	312	253	0.03%	0.004%
22	3.571	783	787	789	rBV3	410	330	0.04%	0.005%
23	3.751	839	843	848	rVB2	296	227	0.03%	0.003%
24	3.783	848	853	856	rBV2	250	256	0.03%	0.004%
25	3.828	856	867	905	rBV	32021	138795	15.33%	1.961%
26	4.259	982	1001	1035	rBV2	121775	379720	41.93%	5.365%
27	4.410	1045	1048	1049	rBV	478	286	0.03%	0.004%
28	4.506	1074	1078	1079	rBV2	1165	758	0.08%	0.011%
29	4.593	1102	1105	1110	rVB2	243	192	0.02%	0.003%
30	4.629	1113	1116	1120	rVB2	306	214	0.02%	0.003%
31	4.738	1148	1150	1157	rVB	312	223	0.02%	0.003%
32	4.902	1197	1201	1203	rBV2	232	212	0.02%	0.003%
33	4.960	1203	1219	1252	rBV2	356391	905665	100.00%	12.795%
34	5.175	1283	1286	1290	rVB2	517	356	0.04%	0.005%
35	5.207	1293	1296	1298	rBV2	306	228	0.03%	0.003%
36	5.291	1313	1322	1325	rBV3	611	814	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062123\
 Data File : VW031606.D
 Acq On : 21 Jun 2023 14:06
 Operator : SY/MD
 Sample : 03334-07ME
 Misc : 5.36g/5.0mL/100uL/5.1mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBW02ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

37	5.313	1325	1329	1334	rVB2	761	828	0.09%	0.012%
38	5.349	1334	1340	1342	rBV2	566	588	0.06%	0.008%
39	5.539	1386	1399	1432	rBV	290344	635051	70.12%	8.972%
40	5.834	1483	1491	1492	rBV3	2000	1951	0.22%	0.028%
41	5.937	1518	1523	1527	rVV5	1183	1466	0.16%	0.021%
42	5.995	1527	1541	1567	rVV	190421	414093	45.72%	5.850%
43	6.175	1595	1597	1608	rVB4	465	556	0.06%	0.008%
44	6.580	1719	1723	1725	rBV2	541	380	0.04%	0.005%
45	6.593	1725	1727	1730	rVV2	400	293	0.03%	0.004%
46	6.612	1730	1733	1739	rVB2	427	407	0.04%	0.006%
47	6.831	1795	1801	1803	rBV	195	221	0.02%	0.003%
48	6.918	1817	1828	1856	rBV	93208	192911	21.30%	2.725%
49	7.143	1894	1898	1903	rVB4	640	756	0.08%	0.011%
50	7.249	1918	1931	1956	rBV	384884	697336	77.00%	9.852%
51	7.510	2010	2012	2017	rVB2	292	208	0.02%	0.003%
52	7.561	2017	2028	2065	rBV	65799	140303	15.49%	1.982%
53	7.712	2073	2075	2079	rVB2	392	289	0.03%	0.004%
54	7.741	2079	2084	2089	rBV4	463	497	0.05%	0.007%
55	7.764	2089	2091	2096	rVB2	307	211	0.02%	0.003%
56	7.886	2125	2129	2134	rVV3	723	674	0.07%	0.010%
57	8.072	2171	2187	2216	rBV	120233	320841	35.43%	4.533%
58	8.397	2280	2288	2296	rBV6	1404	2205	0.24%	0.031%
59	8.593	2348	2349	2353	rVB2	424	200	0.02%	0.003%
60	8.648	2361	2366	2370	rVB2	475	420	0.05%	0.006%
61	8.709	2379	2385	2386	rBV2	325	279	0.03%	0.004%
62	8.792	2399	2411	2442	rVV	398303	776347	85.72%	10.968%
63	9.101	2502	2507	2515	rBV6	598	758	0.08%	0.011%
64	9.165	2523	2527	2530	rBV2	304	217	0.02%	0.003%
65	9.760	2708	2712	2717	rBV2	219	261	0.03%	0.004%
66	9.847	2736	2739	2744	rVB3	307	259	0.03%	0.004%
67	9.876	2744	2748	2749	rBV	353	212	0.02%	0.003%
68	10.172	2827	2840	2856	rBV	265086	438306	48.40%	6.192%
69	10.487	2935	2938	2942	rVB3	374	328	0.04%	0.005%
70	10.564	2958	2962	2967	rBV2	256	249	0.03%	0.004%
71	10.587	2967	2969	2974	rBV2	196	224	0.02%	0.003%
72	11.130	3135	3138	3140	rBV2	595	333	0.04%	0.005%
73	11.198	3147	3159	3184	rBV	483276	754942	83.36%	10.666%
74	11.442	3229	3235	3238	rBV2	352	438	0.05%	0.006%
75	11.490	3243	3250	3251	rBV	327	322	0.04%	0.005%
76	11.570	3263	3275	3298	rBV	405131	639639	70.63%	9.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062123\
 Data File : VW031606.D
 Acq On : 21 Jun 2023 14:06
 Operator : SY/MD
 Sample : 03334-07ME
 Misc : 5.36g/5.0mL/100uL/5.1mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YBW02ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
 Title : VOC Analysis

77	11.873	3365	3369	3373	rVB2	314	204	0.02%	0.003%
78	11.992	3403	3406	3411	rBV3	432	411	0.05%	0.006%
79	12.066	3425	3429	3433	rVB	460	338	0.04%	0.005%
80	12.127	3444	3448	3454	rBV2	244	395	0.04%	0.006%
81	12.201	3460	3471	3472	rBV3	860	1181	0.13%	0.017%
82	12.590	3589	3592	3593	rBV2	401	233	0.03%	0.003%
83	12.677	3615	3619	3624	rBV2	409	363	0.04%	0.005%
84	12.950	3701	3704	3707	rBV	272	190	0.02%	0.003%
85	13.210	3781	3785	3790	rBV3	582	569	0.06%	0.008%
86	13.233	3790	3792	3798	rVV3	421	395	0.04%	0.006%
87	13.265	3798	3802	3806	rVB2	541	456	0.05%	0.006%
88	13.390	3838	3841	3847	rBV2	385	382	0.04%	0.005%
89	13.558	3891	3893	3899	rVB	503	300	0.03%	0.004%
90	13.635	3915	3917	3922	rBV2	267	213	0.02%	0.003%
91	13.988	4021	4027	4028	rBV2	1279	1180	0.13%	0.017%
92	14.165	4078	4082	4085	rBV3	542	407	0.04%	0.006%
93	14.419	4158	4161	4163	rVB2	508	281	0.03%	0.004%
94	14.680	4239	4242	4245	rBV	526	403	0.04%	0.006%
95	14.831	4287	4289	4292	rVB2	531	259	0.03%	0.004%
96	14.911	4312	4314	4319	rVB4	476	383	0.04%	0.005%
97	14.953	4322	4327	4328	rBV2	632	547	0.06%	0.008%
98	14.963	4328	4330	4337	rVB2	771	690	0.08%	0.010%
99	14.992	4337	4339	4340	rBV	413	196	0.02%	0.003%
100	15.651	4541	4544	4546	rBV3	829	436	0.05%	0.006%




Sum of corrected areas: 7078194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031606.D
Acq On : 21 Jun 2023 14:06
Operator : SY/MD
Sample : 03334-07ME
Misc : 5.36g/5.0mL/100uL/5.1mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBW02ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

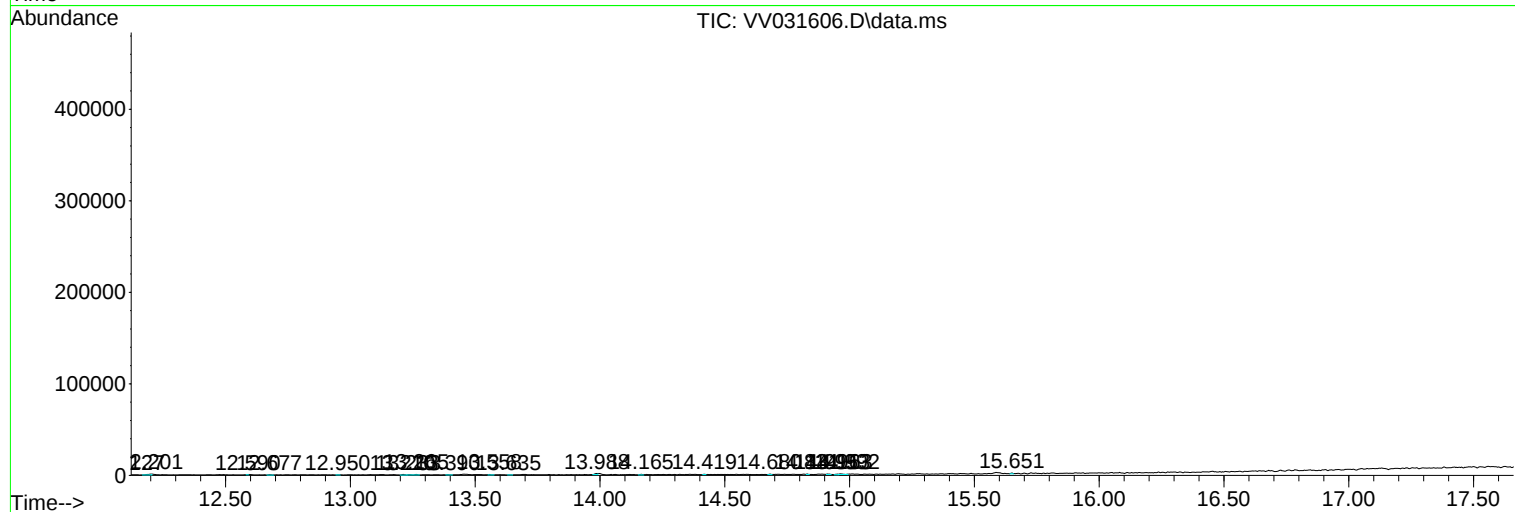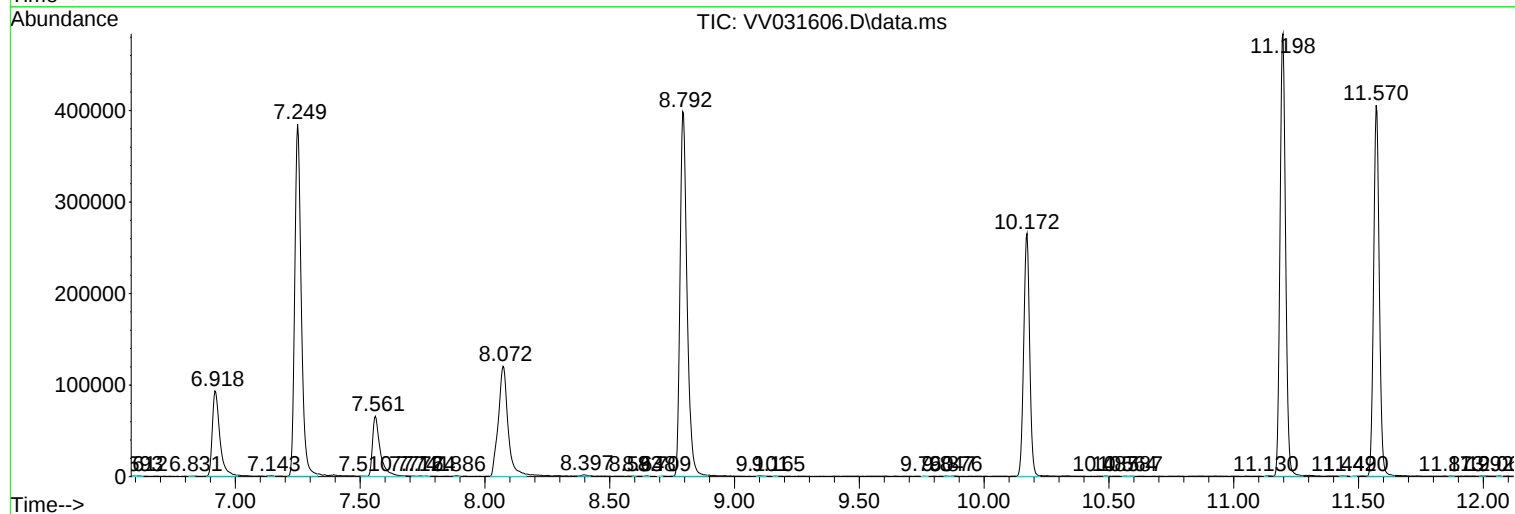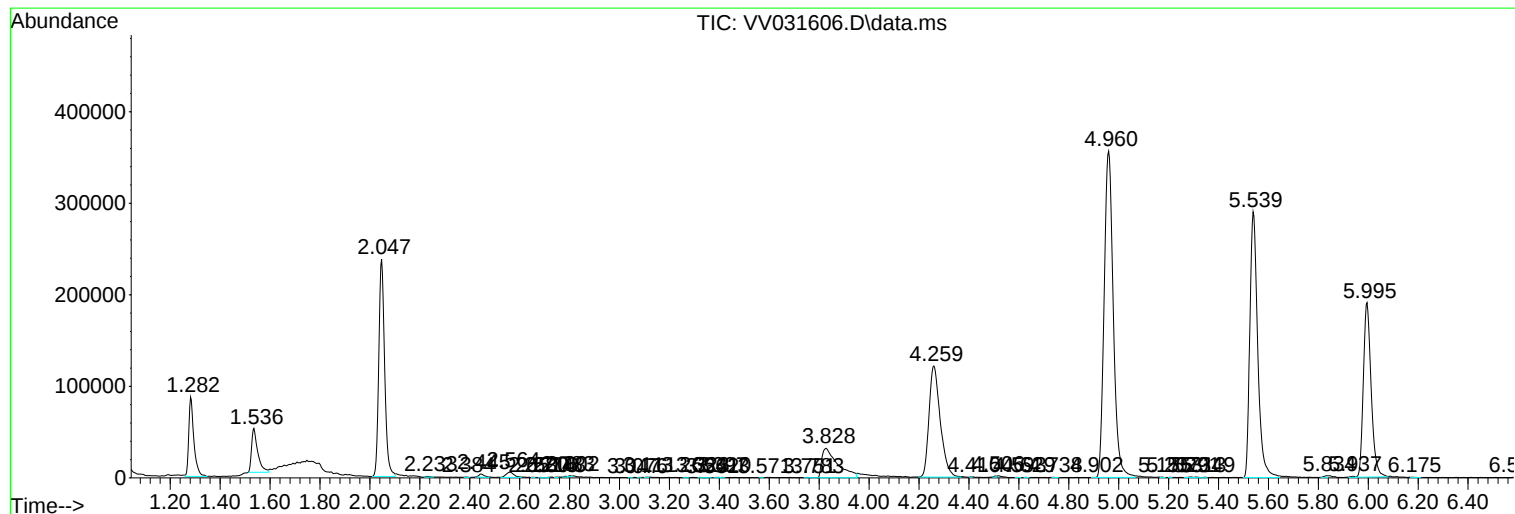

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031606.D
Acq On : 21 Jun 2023 14:06
Operator : SY/MD
Sample : 03334-07ME
Misc : 5.36g/5.0mL/100uL/5.1mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBW02ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031606.D
Acq On : 21 Jun 2023 14:06
Operator : SY/MD
Sample : 03334-07ME
Misc : 5.36g/5.0mL/100uL/5.1mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YBW02ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------