


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062123\
Data File : VV031599.D
Acq On : 21 Jun 2023 10:45
Operator : SY/MD
Sample : BFB391
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB391

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM061423WMA.M
Title : VOC Analysis
Last Update : Thu Jun 22 02:14:12 2023

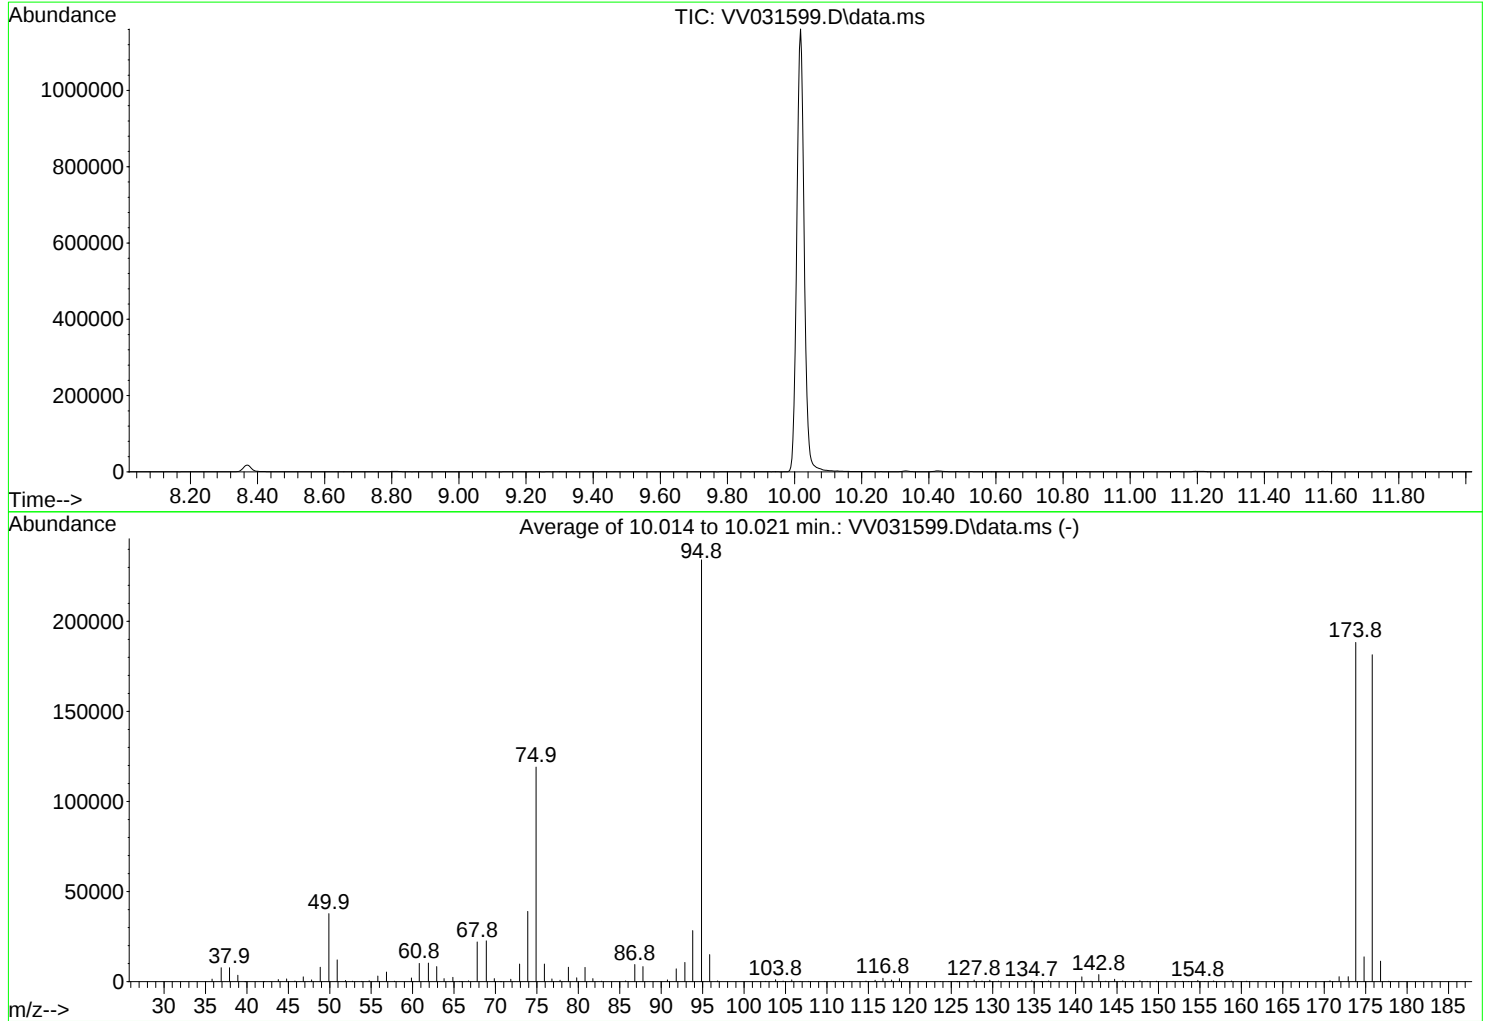

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	37768	PASS
75	95	30	80	50.9	119077	PASS
95	95	100	100	100.0	234155	PASS
96	95	5	9	6.4	15044	PASS
173	174	0.00	2	1.5	2752	PASS
174	95	50	120	80.4	188309	PASS
175	174	5	9	7.3	13751	PASS
176	174	95	105	96.4	181504	PASS
177	176	5	10	6.2	11335	PASS

m/z	Abundance
39.80	181.0
43.80	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.80	1567.0
36.90	7958.0
37.90	7706.0
38.90	3729.0
39.70	213.0
43.80	1300.0
44.80	1573.0
45.80	356.0
46.80	2686.0
47.80	907.0
48.90	7961.0
49.90	37520.0
50.90	12645.0
51.90	679.0
52.70	314.0
53.80	242.0
54.70	585.0
55.80	3116.0
56.80	5321.0
57.80	232.0
59.90	2141.0
60.80	10257.0
61.90	10224.0
62.90	8643.0
63.80	1750.0
64.80	2502.0
65.70	289.0
66.70	477.0
67.80	21920.0
68.90	22864.0
69.90	1680.0
70.60	101.0
71.80	1442.0
72.90	9412.0
73.90	39032.0
74.90	119128.0
75.90	10057.0
76.80	1536.0
77.80	684.0
78.80	8253.0
79.80	2181.0
80.80	7800.0
81.70	1633.0
82.80	236.0
85.70	475.0
86.80	9784.0
87.80	8440.0
90.80	896.0
91.80	7134.0
92.80	10600.0
93.80	27944.0
94.80	231744.0
95.80	15141.0
96.80	518.0
102.60	120.0
103.80	1103.0
104.70	393.0
105.80	1002.0
106.80	185.0
107.70	177.0
109.70	159.0
110.80	240.0
111.80	223.0
112.80	196.0
114.70	367.0
115.80	846.0
116.70	2024.0
117.80	829.0
118.80	1628.0
124.70	118.0
125.70	100.0
127.80	819.0
128.70	363.0
129.70	808.0
130.70	334.0
134.70	452.0
135.80	109.0
136.70	432.0
139.80	217.0
140.80	2661.0
141.80	264.0
142.80	3944.0
143.70	343.0
144.70	1502.0
145.70	440.0
146.80	150.0
147.70	522.0
148.70	183.0
149.70	295.0
151.70	157.0
152.90	125.0
153.60	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

154.80	618.0
155.60	113.0
156.70	444.0
158.80	287.0
160.60	272.0
161.00	176.0
170.70	563.0
171.80	2681.0
172.90	2661.0
173.80	182144.0
174.80	13567.0
175.80	174528.0
176.80	11412.0
177.80	251.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.80	1514.0
36.90	7998.0
37.90	8127.0
38.90	3618.0
39.80	232.0
42.80	133.0
43.80	1349.0
44.80	1561.0
45.80	301.0
46.80	2734.0
47.80	1028.0
48.80	8214.0
49.90	39064.0
50.90	12561.0
51.90	647.0
52.70	308.0
53.80	206.0
54.70	595.0
55.80	3227.0
56.90	5503.0
57.80	235.0
59.90	2162.0
60.80	10385.0
61.90	10674.0
62.90	8586.0
63.80	1758.0
64.90	2534.0
65.70	257.0
66.80	496.0
67.80	22736.0
68.90	23400.0
69.80	1784.0
71.90	1332.0
72.90	10087.0
73.90	40432.0
74.90	123528.0
75.90	10127.0
76.80	1619.0
77.80	778.0
78.80	8271.0
79.80	2250.0
80.80	8135.0
81.80	1700.0
82.80	260.0
85.70	450.0
86.80	9829.0
87.80	8606.0
90.80	971.0
91.80	7304.0
92.90	11147.0
93.80	29552.0
94.90	242688.0
95.90	15545.0
96.80	474.0
102.60	168.0
103.80	1161.0
104.70	401.0
105.70	1046.0
106.80	165.0
107.80	166.0
109.70	174.0
110.80	234.0
111.80	236.0
112.80	195.0
114.70	348.0
115.80	781.0
116.70	1934.0
117.80	924.0
118.80	1704.0
123.70	115.0
124.70	108.0
127.70	865.0
128.70	396.0
129.60	809.0
130.70	415.0
134.70	559.0
136.80	508.0
139.80	175.0
140.80	2739.0
141.90	294.0
142.80	4124.0
143.60	324.0
144.70	1404.0
145.70	505.0
146.80	186.0
147.70	519.0
148.70	189.0
149.70	324.0
151.80	150.0
152.90	149.0
153.60	131.0
154.70	711.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

155.60	101.0
156.60	491.0
158.80	353.0
160.60	277.0
170.70	537.0
171.80	2841.0
172.90	2906.0
173.80	194688.0
174.80	14167.0
175.80	188288.0
176.80	11777.0
177.80	241.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.80	1306.0
36.90	7256.0
37.90	7478.0
38.90	3219.0
39.80	240.0
42.00	103.0
42.80	176.0
43.80	1340.0
44.80	1404.0
45.80	305.0
46.80	2566.0
47.80	1022.0
48.80	7722.0
49.90	36720.0
50.90	11009.0
51.90	535.0
52.80	259.0
53.90	184.0
54.80	544.0
55.80	2894.0
56.90	5314.0
57.80	256.0
59.80	1935.0
60.80	9841.0
61.90	9897.0
62.90	7907.0
63.80	1476.0
64.90	2272.0
65.90	210.0
66.80	500.0
67.80	21560.0
68.90	21832.0
69.80	1666.0
71.90	1125.0
72.90	9799.0
73.90	37528.0
74.90	114576.0
75.90	9221.0
76.80	1431.0
77.80	893.0
78.80	7483.0
79.80	2070.0
80.80	7784.0
81.80	1668.0
82.80	244.0
85.70	349.0
86.80	8928.0
87.80	8000.0
90.70	956.0
91.80	6820.0
92.90	10340.0
93.80	27552.0
94.90	228032.0
95.90	14445.0
96.80	388.0
102.60	167.0
103.80	1068.0
104.70	394.0
105.70	1021.0
106.70	182.0
107.90	145.0
109.80	183.0
110.80	213.0
111.80	189.0
112.70	200.0
114.70	295.0
115.80	739.0
116.80	1755.0
117.80	966.0
118.70	1634.0
123.70	107.0
126.80	116.0
127.70	945.0
128.70	369.0
129.60	744.0
130.70	445.0
134.70	598.0
136.80	464.0
139.90	122.0
140.70	2627.0
141.90	349.0
142.80	3802.0
143.60	237.0
144.70	1095.0
145.70	471.0
146.70	171.0
147.80	483.0
148.60	158.0
149.80	314.0
151.70	149.0
152.90	162.0
154.70	708.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

156.60	449.0
158.80	350.0
160.70	288.0
170.70	483.0
171.80	2692.0
172.90	2689.0
173.80	188096.0
174.80	13519.0
175.80	181696.0
176.80	10816.0
177.80	276.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391