

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
 Data File : VV011680.D
 Acq On : 21 Jun 2019 13:13
 Operator : SY/MD
 Sample : K3276-03
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E1

Quant Time: Jun 24 04:06:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 24 03:42:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	162475	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	152589	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	61394	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47965	4.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.00%
7) Chloroethane-d5	1.56	69	36263	4.78	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.60%
11) 1,1-Dichloroethene-d2	2.12	63	72778	3.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.40%
20) 2-Butanone-d5	3.94	46	164867	58.04	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.08%
24) Chloroform-d	4.40	84	87151	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
26) 1,2-Dichloroethane-d4	5.08	65	60995	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.20%
32) Benzene-d6	5.09	84	204828	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.12	67	63915	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.36	98	173226	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.66	79	19421	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
46) 2-Hexanone-d5	8.13	63	120032	55.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.68%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	48056	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	59716	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	10762	5.245 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062219\
Data File : VV011680.D
Acq On : 21 Jun 2019 13:13
Operator : SY/MD
Sample : K3276-03
Misc : 25ML/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8E1

Quant Time: Jun 24 04:06:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 24 03:42:07 2019
Response via : Initial Calibration

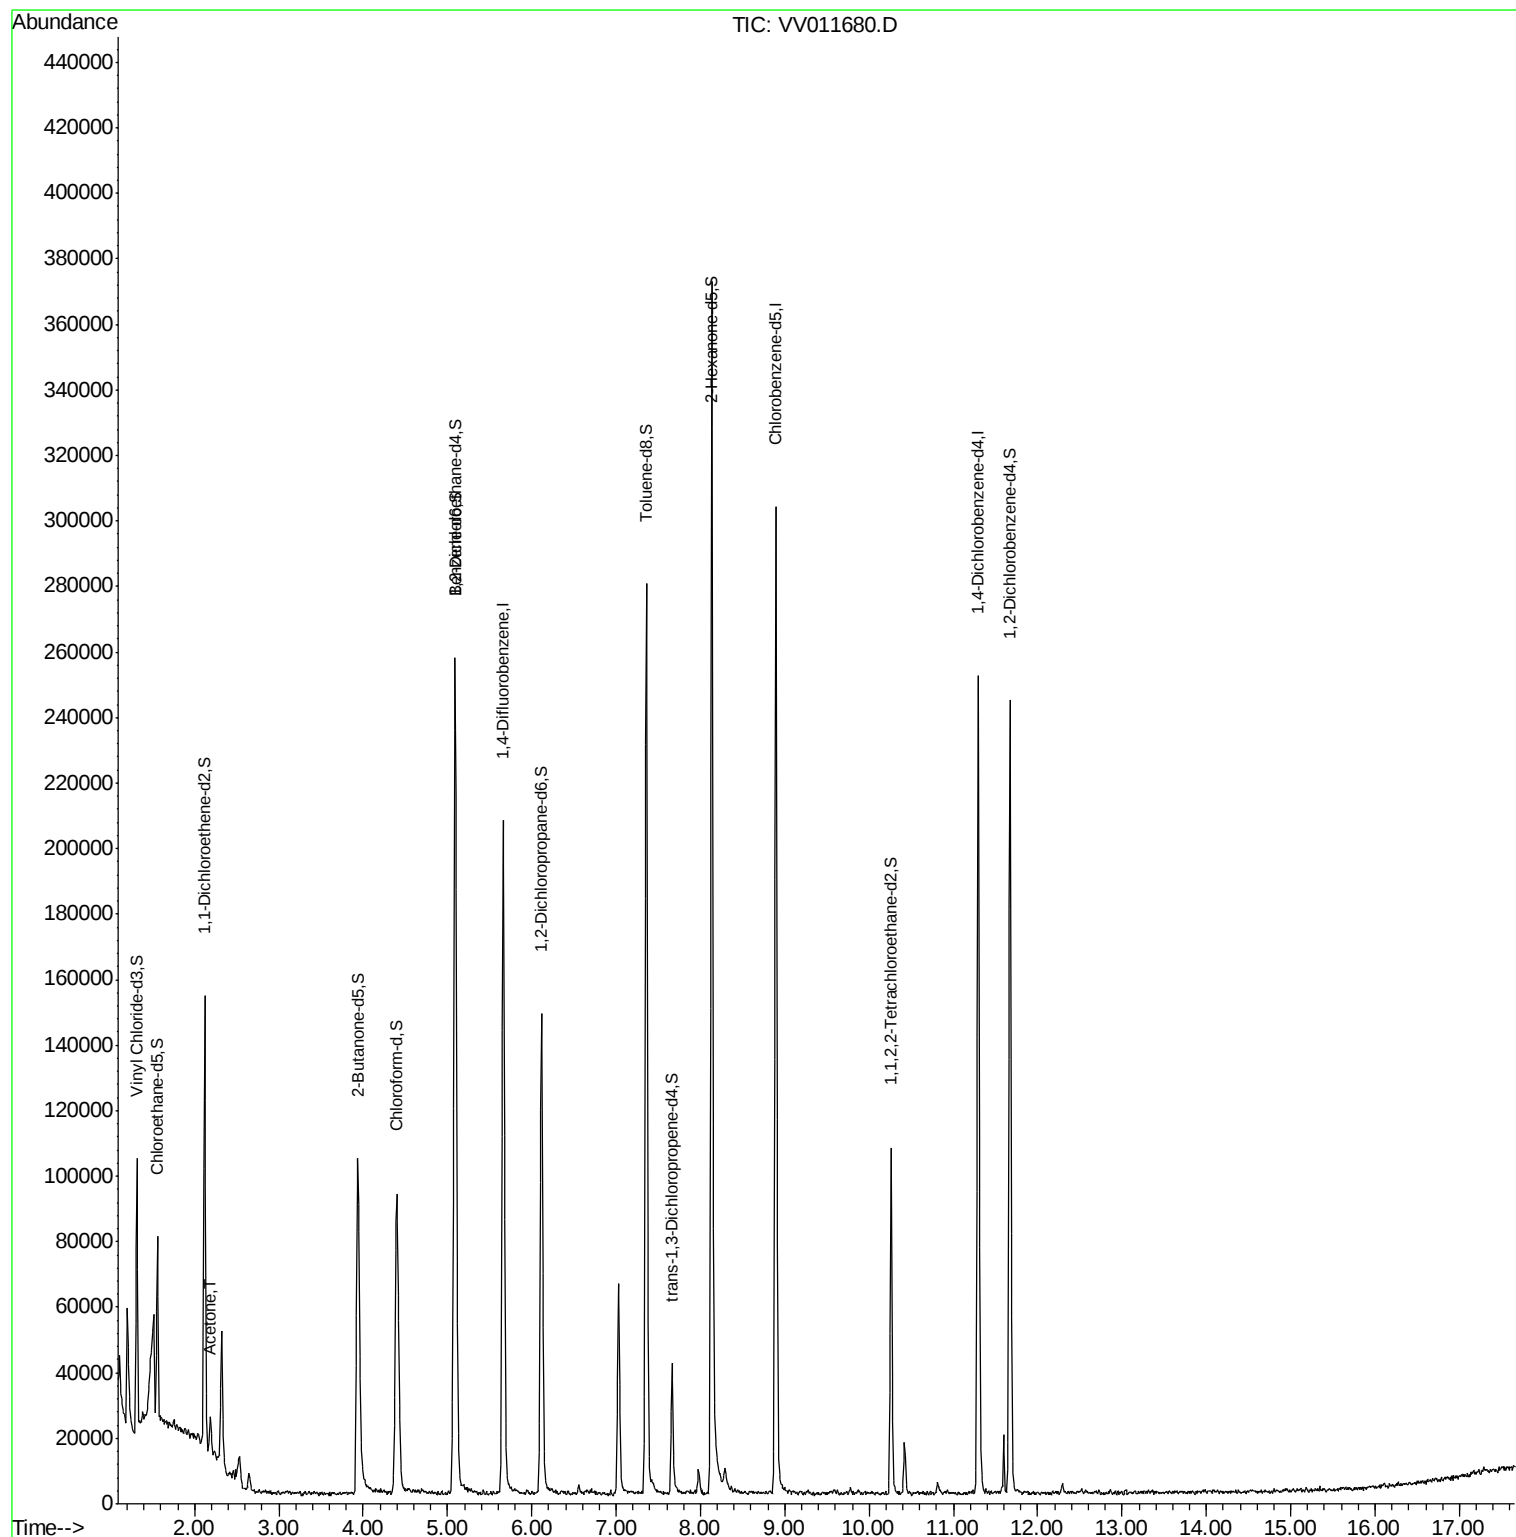

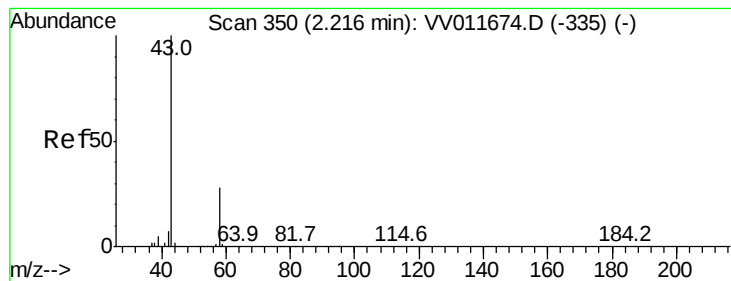

#13

Acetone

Concen: 5.245 ug/L

RT: 2.19 min Scan# 342

Delta R.T. -0.03 min

Lab File: VV011680.D

Acq: 21 Jun 2019 13:13

Instrument :

MSVOA_V

ClientSampleId :

DB8E1

Tot Ion: 43 Resp: 10762

Ion Ratio Lower Upper

43 100

58 29.1 0.0 56.6

