

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
 Data File : VV011684.D
 Acq On : 21 Jun 2019 14:55
 Operator : SY/MD
 Sample : K3415-09DL 50X
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GALP6DL

Quant Time: Jun 24 04:23:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 24 03:42:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	162864	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	151883	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	62682	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	47645	4.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.20%
7) Chloroethane-d5	1.58	69	34999	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.12	63	72956	3.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.40%
20) 2-Butanone-d5	3.96	46	160040	56.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.40%
24) Chloroform-d	4.40	84	78549	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.60%
26) 1,2-Dichloroethane-d4	5.08	65	58497	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.80%
32) Benzene-d6	5.09	84	197077	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.00%
36) 1,2-Dichloropropane-d6	6.12	67	62887	4.82	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.40%
41) Toluene-d8	7.36	98	166712	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	19462	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.14	63	117820	55.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.14%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	46116	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	57614	4.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.40%


Target Compounds					Ovalue
31) Carbon tetrachloride	4.87	117	109798	6.642 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062219\
Data File : VV011684.D
Acq On : 21 Jun 2019 14:55
Operator : SY/MD
Sample : K3415-09DL 50X
Misc : 25ML/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GALP6DL

Quant Time: Jun 24 04:23:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 24 03:42:07 2019
Response via : Initial Calibration

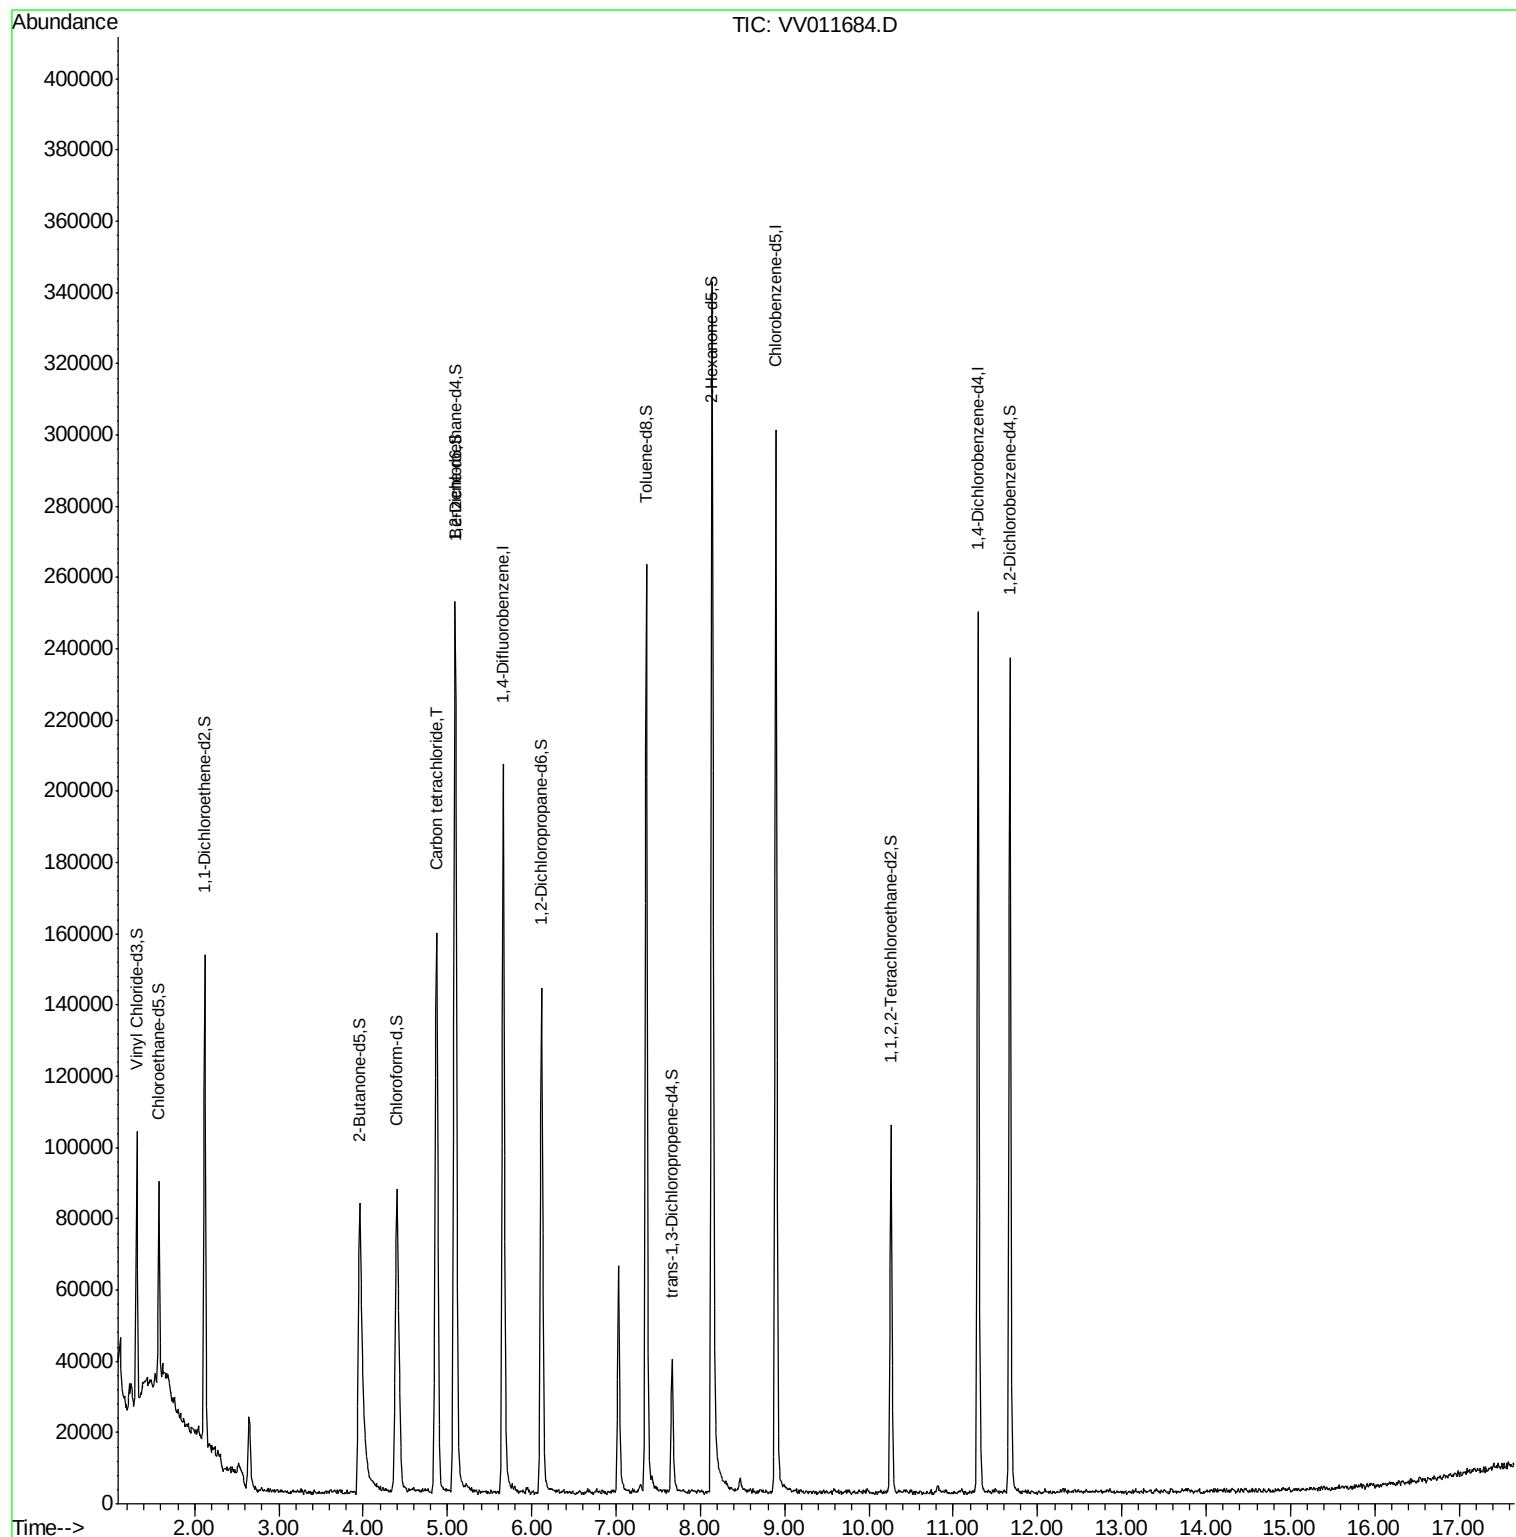

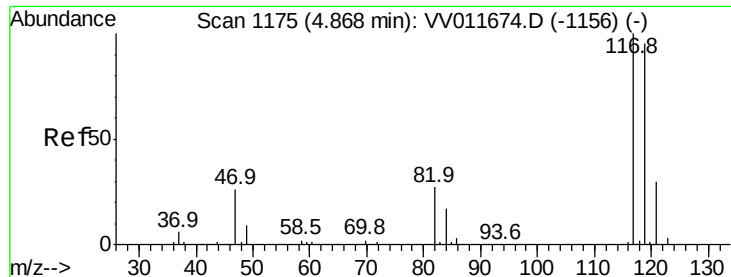

#31

Carbon tetrachloride

Concen: 6.642 ug/L

RT: 4.87 min Scan# 1176

Delta R.T. 0.00 min

Lab File: VV011684.D

Acq: 21 Jun 2019 14:55

Instrument :

MSVOA_V

ClientSampleId :

GALP6DL

Tot Ion:117 Resp: 109798

Ion Ratio Lower Upper

117 100

119 95.4 77.1 115.7

