

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
 Data File : VV011694.D
 Acq On : 21 Jun 2019 19:27
 Operator : SY/MD
 Sample : K3415-18
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GALQ3

Quant Time: Jun 24 05:26:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 24 03:42:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	153026	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	141740	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58858	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	44718	4.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.00%
7) Chloroethane-d5	1.57	69	32305	4.52	ug/L	-0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.12	63	69856	3.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.60%
20) 2-Butanone-d5	3.95	46	159942	59.78	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.56%
24) Chloroform-d	4.40	84	83342	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.00%
26) 1,2-Dichloroethane-d4	5.08	65	59136	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.20%
32) Benzene-d6	5.10	84	195497	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	6.12	67	63167	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.36	98	167183	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
43) trans-1,3-Dichloropropene-	7.67	79	18131	4.26	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.20%
46) 2-Hexanone-d5	8.14	63	115165	57.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	115.36%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	44916	5.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	56956	5.13	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	22270	11.523 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
Data File : VV011694.D
Acq On : 21 Jun 2019 19:27
Operator : SY/MD
Sample : K3415-18
Misc : 25ML/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GALQ3

Quant Time: Jun 24 05:26:16 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 24 03:42:07 2019
Response via : Initial Calibration

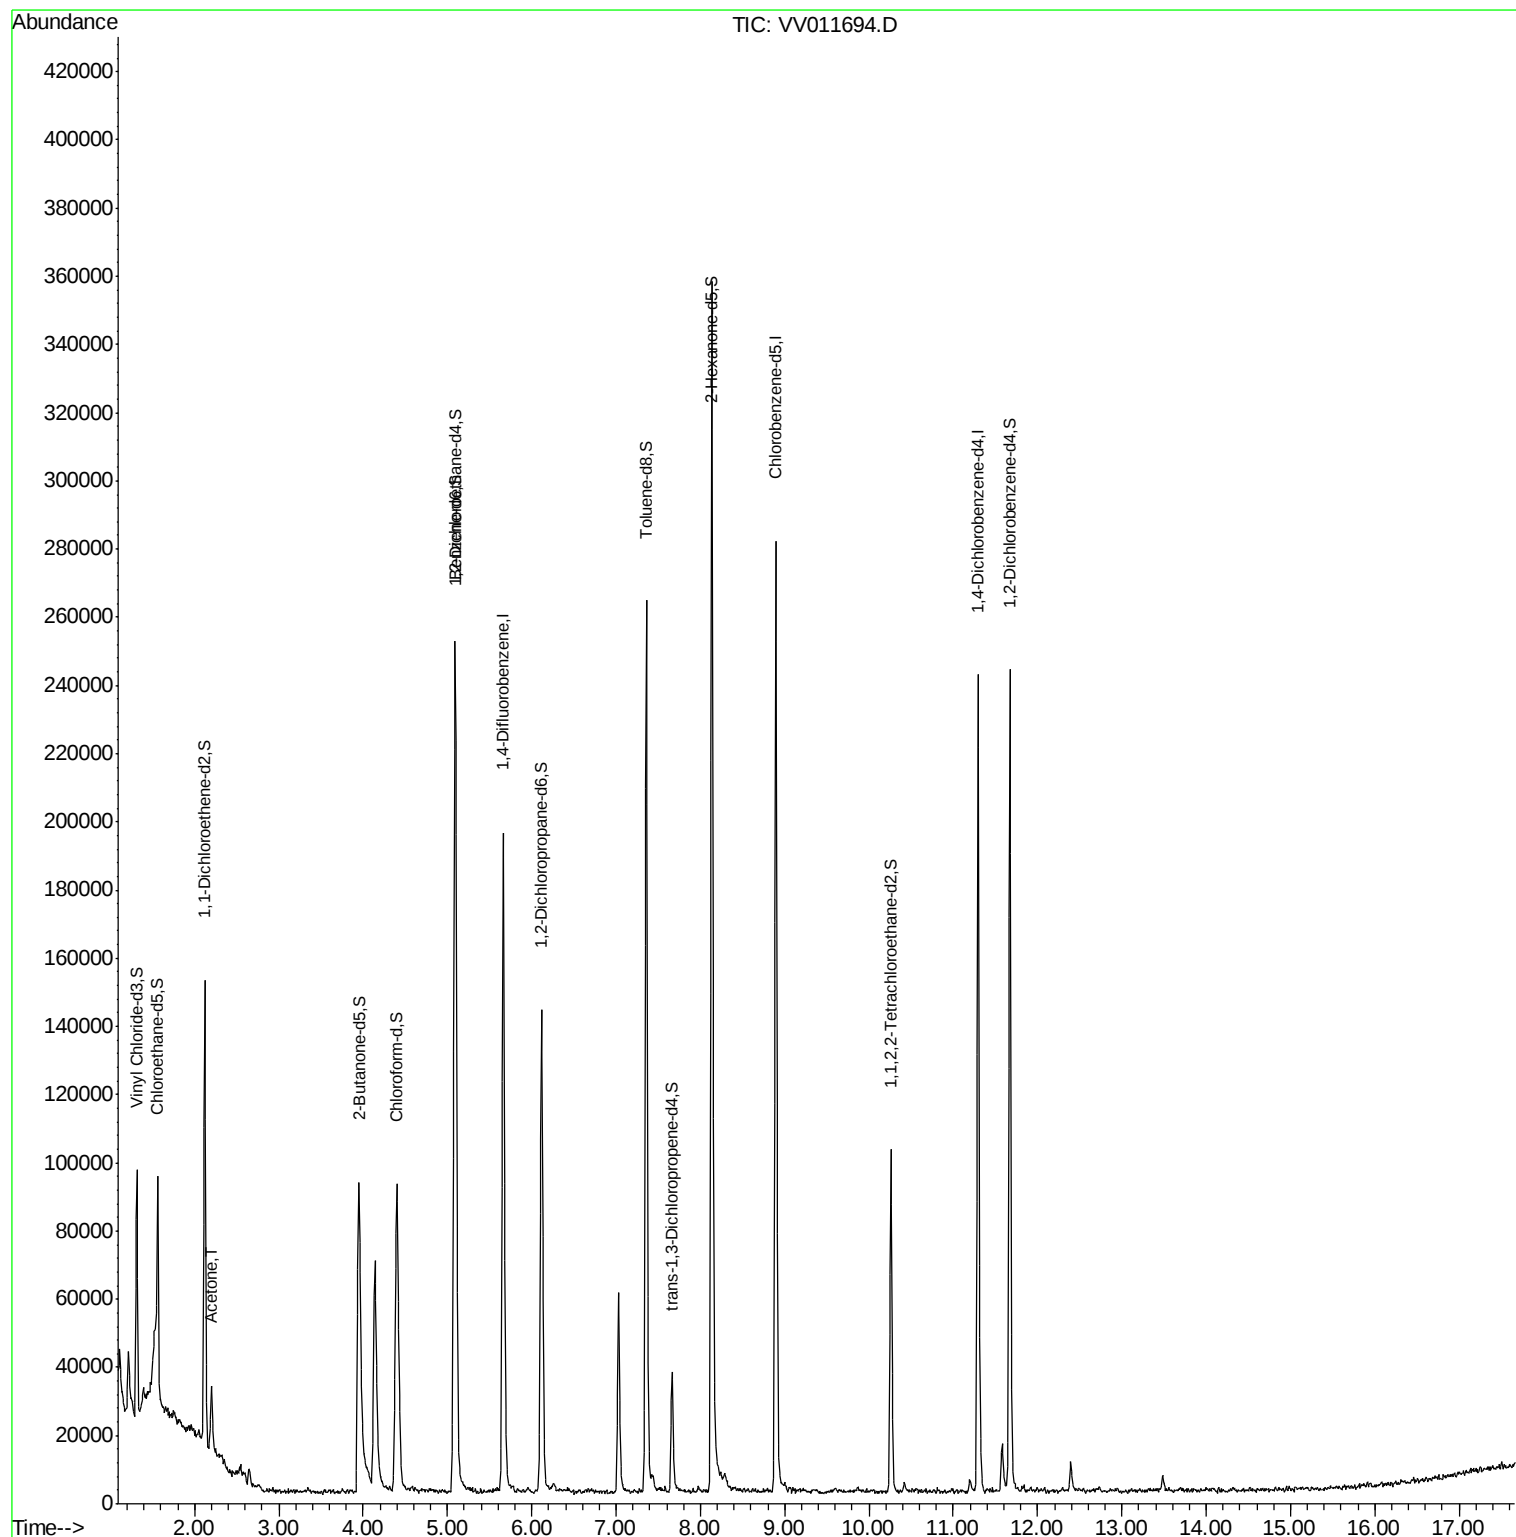

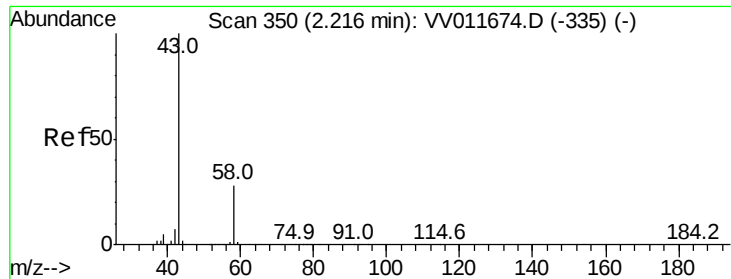

#13
Acetone
Concen: 11.523 ug/L
RT: 2.20 min Scan# 345
Delta R.T. -0.02 min
Lab File: VV011694.D
Acq: 21 Jun 2019 19:27

Instrument :
MSVOA_V
ClientSampleId :
GALQ3

Tot Ion: 43 Resp: 22270
Ion Ratio Lower Upper
43 100
58 26.2 0.0 56.6

