

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
 Data File : VV011695.D
 Acq On : 21 Jun 2019 19:52
 Operator : SY/MD
 Sample : K3415-19
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GALQ4

Quant Time: Jun 24 05:30:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 24 03:42:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	159213	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	150993	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	60255	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46130	4.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.20%
7) Chloroethane-d5	1.57	69	33208	4.47	ug/L	-0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.12	63	71568	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	3.95	46	158484	56.93	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.86%
24) Chloroform-d	4.40	84	86056	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
26) 1,2-Dichloroethane-d4	5.08	65	58912	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.09	84	194572	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
36) 1,2-Dichloropropane-d6	6.12	67	62082	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.36	98	165937	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	18239	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.13	63	113791	53.50	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.00%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	44842	4.97	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	59572	5.24	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	23185	11.530 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062219\
Data File : VV011695.D
Acq On : 21 Jun 2019 19:52
Operator : SY/MD
Sample : K3415-19
Misc : 25ML/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GALQ4

Quant Time: Jun 24 05:30:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 24 03:42:07 2019
Response via : Initial Calibration

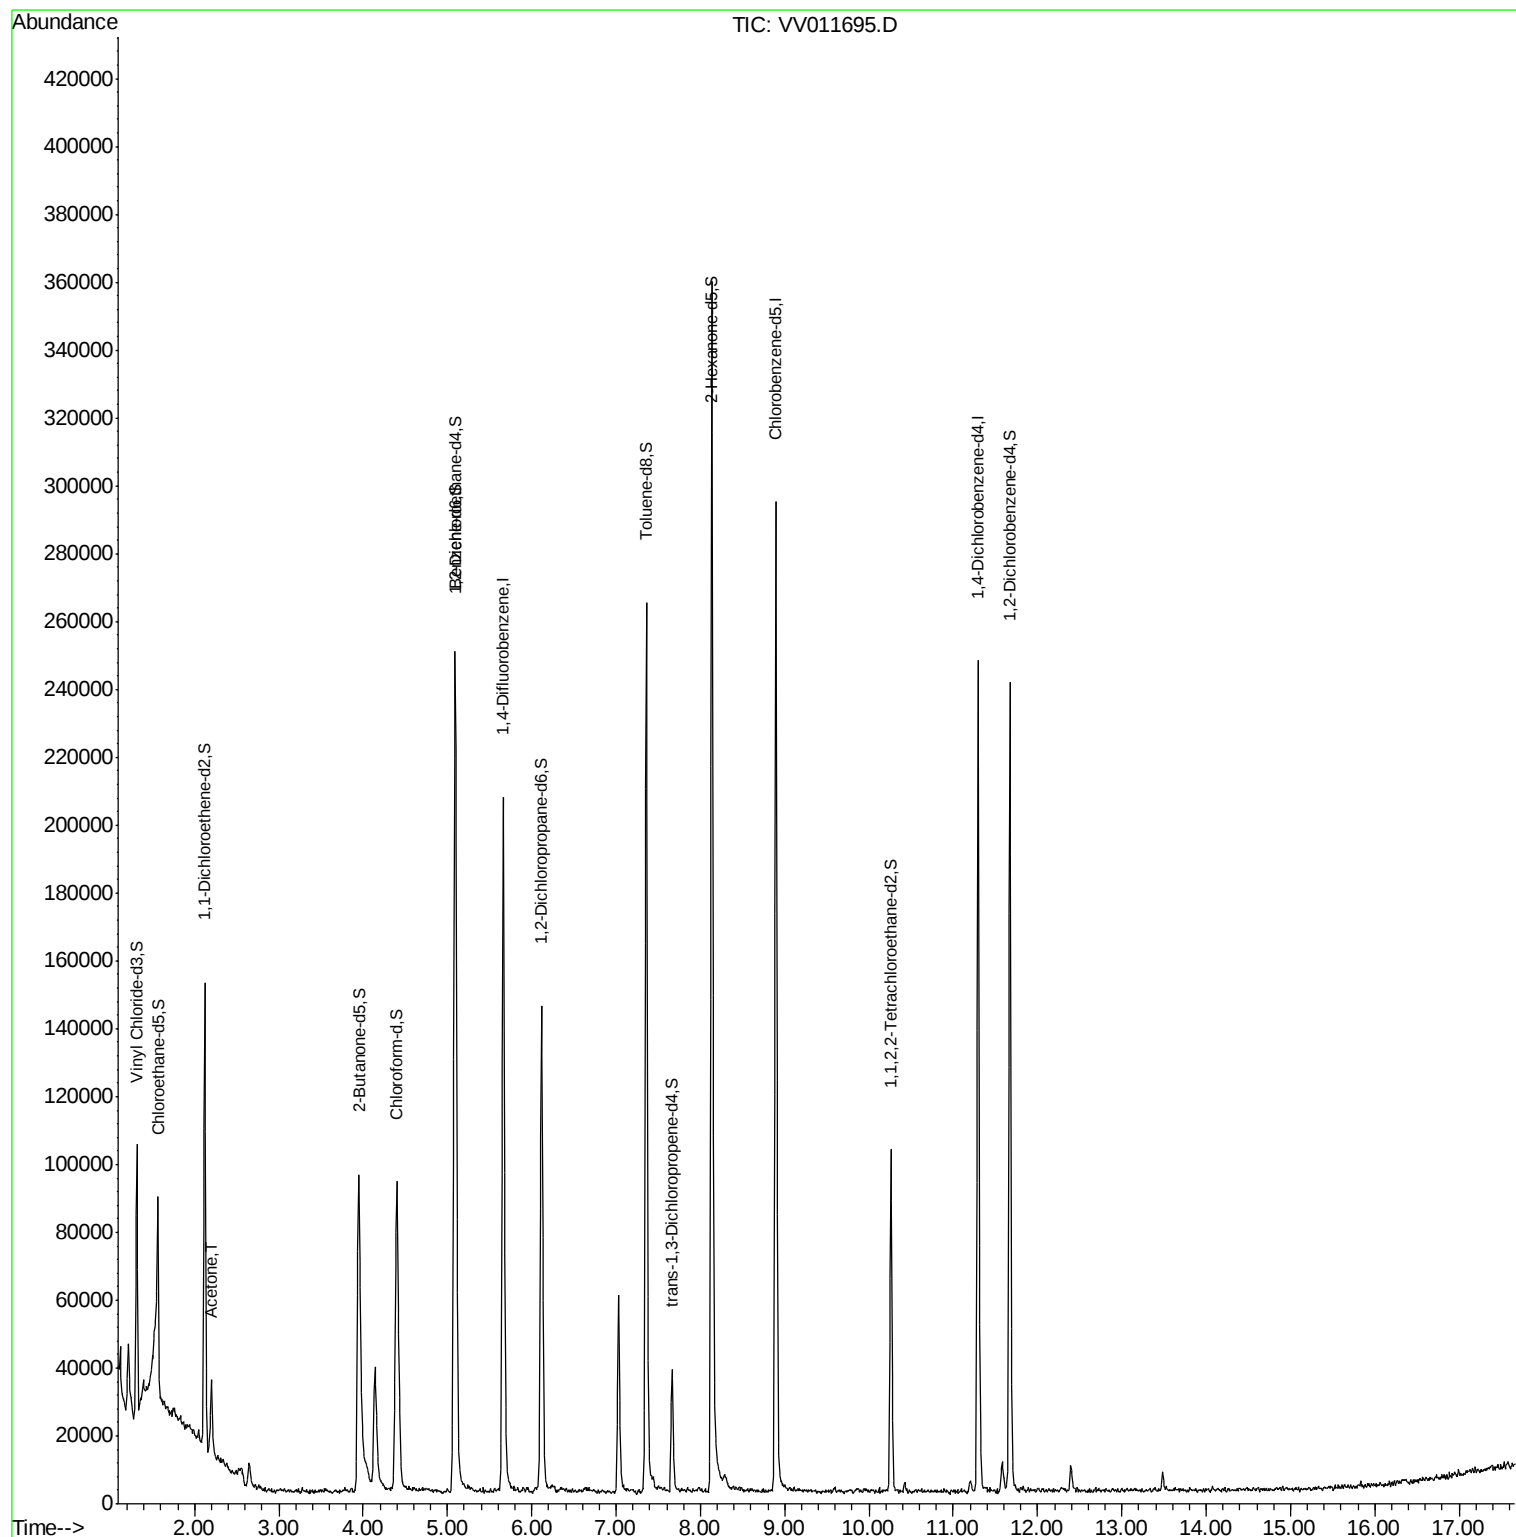

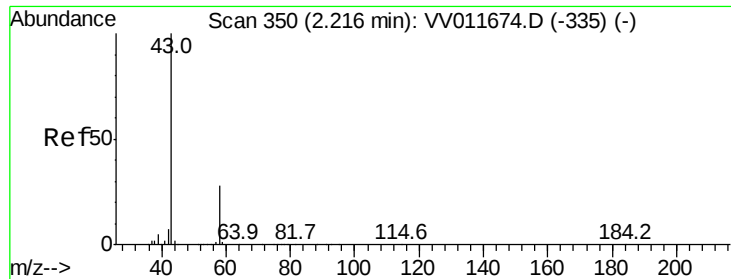

#13

Acetone

Concen: 11.530 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.02 min

Lab File: VV011695.D

Acq: 21 Jun 2019 19:52

Instrument :

MSVOA_V

ClientSampleId :


GALQ4

Tot Ion: 43 Resp: 23185

Ion Ratio Lower Upper

43 100

58 30.3 0.0 56.6

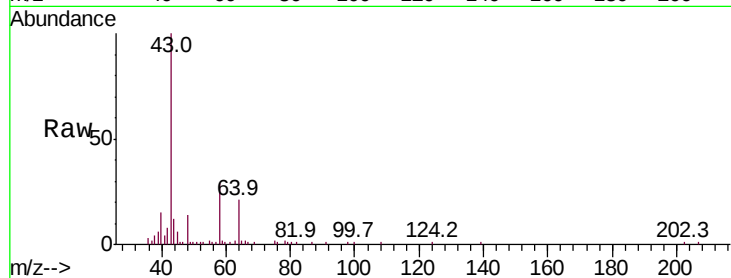

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

