

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
 Data File : VV011702.D
 Acq On : 21 Jun 2019 23:38
 Operator : SY/MD
 Sample : K3462-04
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCN2

Quant Time: Jun 24 06:07:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Jun 24 05:42:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	153977	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	141663	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	57553	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42840	4.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.80%
7) Chloroethane-d5	1.57	69	31902	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.12	63	67988	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	3.95	46	149790	55.64	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.28%
24) Chloroform-d	4.40	84	73162	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.40%
26) 1,2-Dichloroethane-d4	5.08	65	55836	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.09	84	187702	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.12	67	59895	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	7.36	98	155678	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.67	79	17231	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	8.13	63	108425	54.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.66%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	43203	5.10	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	53849	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%


Target Compounds					Ovalue
13) Acetone	2.20	43	4853	2.496 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
Data File : VV011702.D
Acq On : 21 Jun 2019 23:38
Operator : SY/MD
Sample : K3462-04
Misc : 25ML/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCN2

Quant Time: Jun 24 06:07:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Jun 24 05:42:24 2019
Response via : Initial Calibration

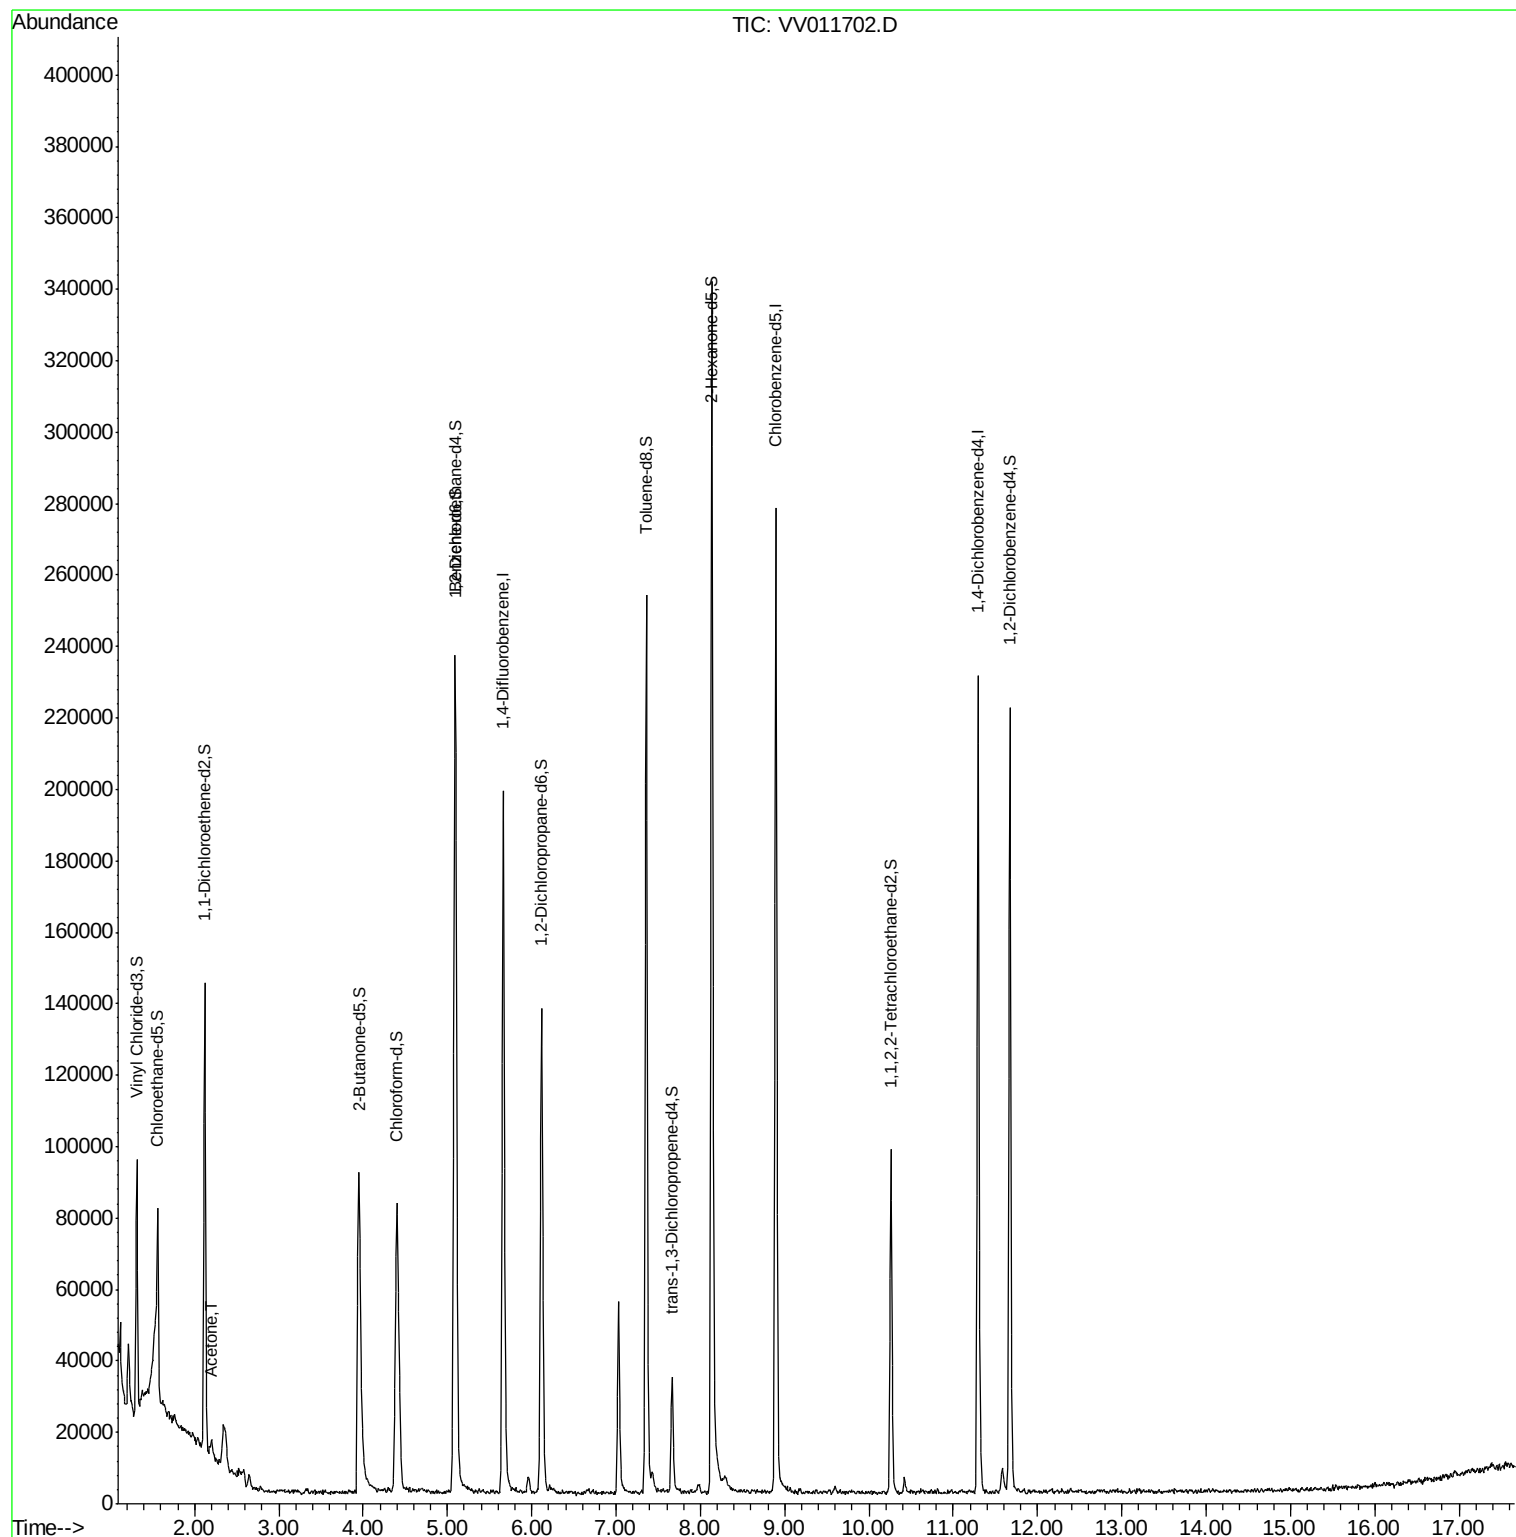

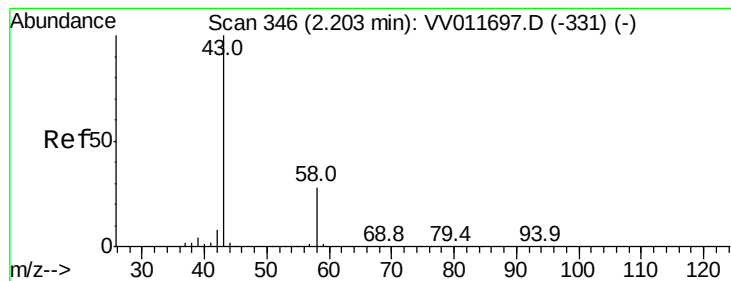

#13

Acetone

Concen: 2.496 ug/L

RT: 2.20 min Scan# 345

Delta R.T. -0.00 min

Lab File: VV011702.D

Acq: 21 Jun 2019 23:38

Instrument :
MSVOA_V
ClientSampleId :
BFCN2

Tot Ion: 43 Resp: 4853

Ion Ratio Lower Upper

43 100

58 36.3 0.0 56.6

