


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062219\
Data File : VV011673.D
Acq On : 21 Jun 2019 09:19
Operator : SY/MD
Sample : BFB54
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB54

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR062119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Jun 24 05:42:24 2019

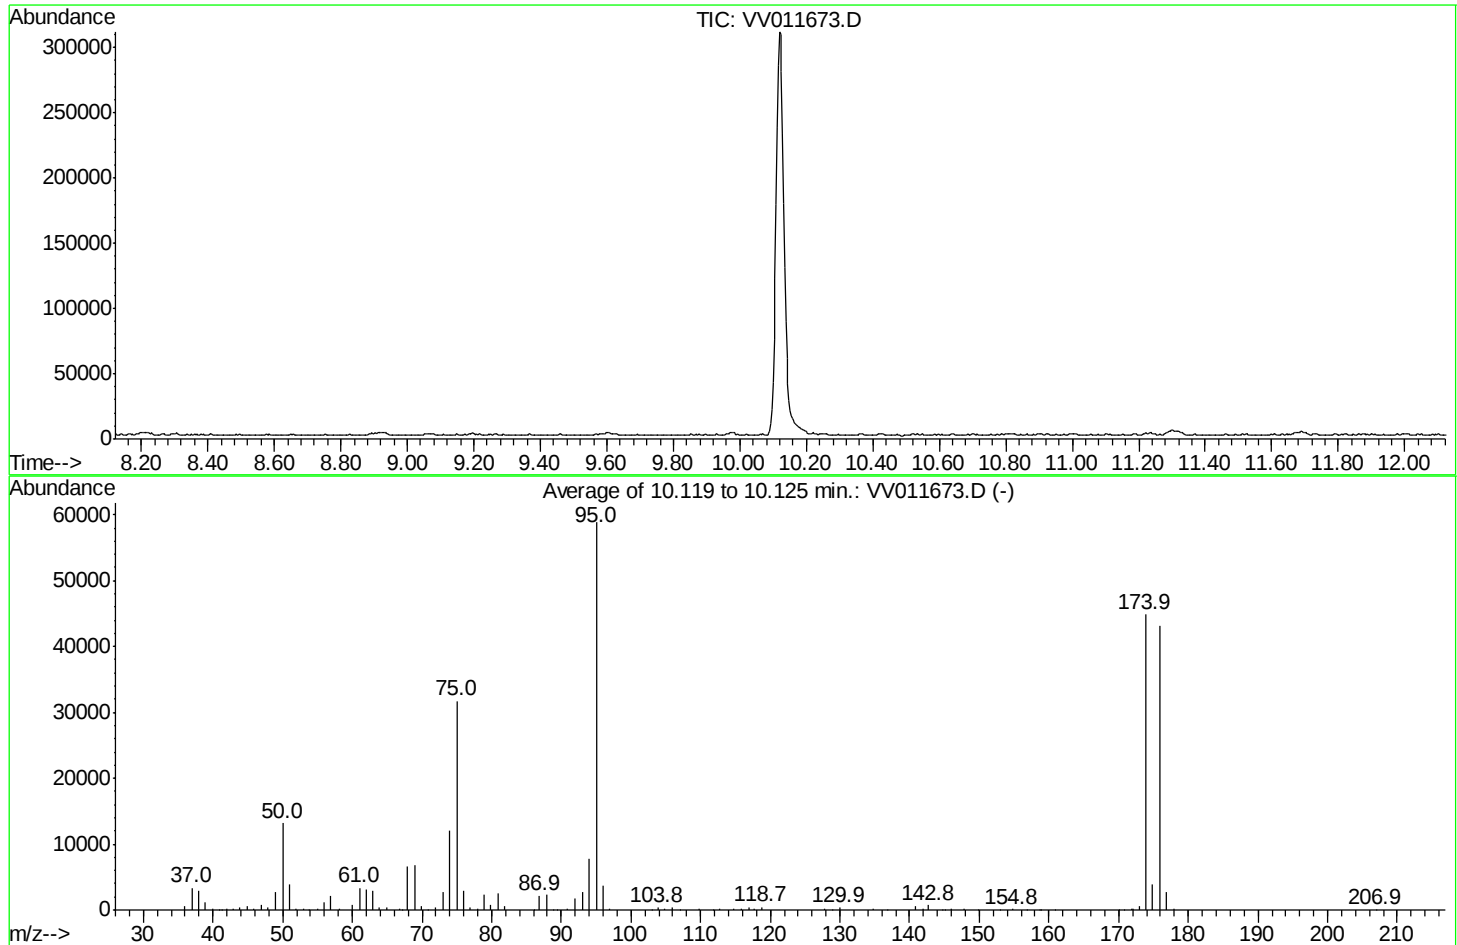

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	13190	PASS
75	95	30	80	53.9	31709	PASS
95	95	100	100	100.0	58853	PASS
96	95	5	9	6.4	3779	PASS
173	174	0.00	2	1.4	640	PASS
174	95	50	120	76.2	44834	PASS
175	174	5	9	8.6	3839	PASS
176	174	95	101	96.1	43074	PASS
177	176	5	9	6.2	2656	PASS

Scan 2795 (10.077 min): VV011673.D
BFB54

m/z	Abundance
36.00	179.0
37.80	119.0
39.90	1750.0
40.80	133.0
43.80	408.0
44.90	117.0
50.90	109.0
60.40	101.0
115.70	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	719.0
36.90	3587.0
38.00	3150.0
38.90	1176.0
39.90	2090.0
40.90	124.0
41.30	122.0
42.00	126.0
42.90	136.0
44.00	793.0
44.90	652.0
45.80	154.0
47.00	946.0
47.80	451.0
49.00	2974.0
50.00	13926.0
51.00	4177.0
51.90	315.0
53.00	127.0
55.00	226.0
56.00	1193.0
57.00	2099.0
58.10	101.0
59.90	775.0
61.00	3398.0
61.90	3258.0
63.00	2867.0
64.00	404.0
64.80	361.0
66.90	211.0
67.90	6964.0
69.00	7197.0
69.90	535.0
71.90	459.0
73.00	2782.0
74.00	12731.0
75.00	33312.0
76.00	3129.0
76.80	457.0
77.80	286.0
78.90	2399.0
79.90	856.0
80.90	2532.0
81.90	608.0
86.90	2339.0
87.90	2532.0
89.40	117.0
90.90	265.0
91.90	1874.0
93.00	2783.0
94.00	8366.0
95.00	60744.0
96.00	4071.0
97.00	153.0
103.90	372.0
104.90	178.0
105.90	326.0
109.80	176.0
111.80	131.0
112.70	135.0
114.80	138.0
115.90	275.0
116.90	388.0
117.70	267.0
118.70	386.0
127.80	178.0
128.80	105.0
129.90	347.0
134.80	261.0
136.80	136.0
140.90	688.0
141.80	108.0
142.80	714.0
144.70	132.0
145.90	115.0
147.90	168.0
153.00	110.0
154.80	171.0
156.80	124.0
158.70	105.0
171.90	411.0
173.00	691.0
173.90	45928.0
174.90	3952.0
175.90	43848.0
176.90	2570.0
177.90	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	679.0
37.00	3527.0
38.00	3083.0
38.90	1124.0
39.90	1937.0
40.90	137.0
42.00	112.0
42.90	123.0
44.00	865.0
44.90	664.0
45.80	152.0
47.00	894.0
47.80	469.0
49.00	2875.0
50.00	13538.0
51.00	4138.0
51.90	284.0
53.00	113.0
53.80	103.0
55.00	209.0
56.00	1113.0
56.90	2311.0
58.10	115.0
59.90	733.0
61.00	3448.0
62.00	3240.0
63.00	2991.0
63.90	374.0
64.90	316.0
66.80	172.0
67.90	6843.0
69.00	7057.0
70.00	559.0
70.90	104.0
71.90	505.0
73.00	2670.0
74.00	12531.0
75.00	32632.0
76.00	3040.0
76.80	503.0
77.90	249.0
78.80	2371.0
79.90	807.0
80.90	2556.0
81.90	596.0
86.00	107.0
86.90	2210.0
87.90	2535.0
90.80	280.0
91.90	1716.0
93.00	2688.0
94.00	8053.0
95.00	60792.0
96.00	3852.0
97.00	158.0
103.90	314.0
104.90	190.0
105.90	323.0
107.00	105.0
109.80	147.0
111.70	101.0
112.70	193.0
114.80	170.0
115.90	296.0
116.90	374.0
117.80	289.0
118.70	412.0
127.80	201.0
129.90	315.0
134.80	234.0
136.80	115.0
140.90	680.0
141.90	110.0
142.80	696.0
145.10	125.0
145.90	108.0
147.90	170.0
149.70	118.0
154.70	167.0
156.80	109.0
158.90	106.0
160.90	117.0
170.80	124.0
172.10	404.0
173.00	653.0
173.90	46272.0
174.90	4013.0
175.90	44488.0
176.90	2739.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54

m/z	Abundance
36.00	649.0
37.00	3097.0
38.00	2833.0
38.90	1079.0
39.90	1862.0
40.90	156.0
42.10	118.0
43.00	117.0
44.00	875.0
44.90	631.0
45.90	138.0
46.90	733.0
47.90	458.0
49.00	2582.0
50.00	12108.0
51.00	3715.0
52.00	291.0
52.80	101.0
53.70	112.0
55.00	195.0
56.00	964.0
56.90	2150.0
58.20	118.0
59.90	621.0
61.00	3152.0
62.00	2890.0
63.00	2804.0
63.80	339.0
65.00	285.0
66.70	133.0
67.10	150.0
67.90	6174.0
69.00	6316.0
70.00	505.0
71.90	477.0
73.00	2516.0
74.00	11187.0
75.00	29184.0
76.00	2813.0
76.80	470.0
78.00	291.0
78.80	2157.0
79.90	702.0
80.90	2342.0
81.90	481.0
86.00	170.0
86.90	1952.0
87.90	2209.0
88.80	109.0
90.70	235.0
91.90	1531.0
93.00	2450.0
94.00	6903.0
95.00	55024.0
96.00	3415.0
97.00	129.0
102.90	107.0
103.80	304.0
104.80	174.0
105.90	319.0
112.70	194.0
114.80	150.0
115.80	261.0
116.90	340.0
117.80	269.0
118.70	398.0
127.80	192.0
130.00	237.0
134.80	162.0
140.90	641.0
141.80	126.0
142.70	703.0
145.10	122.0
145.90	107.0
147.80	145.0
149.80	113.0
154.70	175.0
158.90	121.0
160.90	135.0
170.10	108.0
170.70	160.0
172.00	378.0
173.00	577.0
173.90	42304.0
174.90	3553.0
175.90	40888.0
176.90	2661.0
177.90	156.0
206.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB54