

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062220\
 Data File : VV017013.D
 Acq On : 22 Jun 2020 11:37
 Operator : SY/MD
 Sample : VV0622WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	80	rVB	173527	175925	12.54%	1.682%
2	1.579	146	152	163	rVB	116731	129493	9.23%	1.238%
3	2.122	310	321	345	rBV	291215	451979	32.22%	4.323%
4	2.367	396	397	399	rBV2	1605	695	0.05%	0.007%
5	2.518	438	444	445	rBV4	2856	2089	0.15%	0.020%
6	2.582	462	464	466	rBV3	1156	581	0.04%	0.006%
7	2.958	578	581	582	rBV4	1336	713	0.05%	0.007%
8	3.055	607	611	612	rBV4	1343	854	0.06%	0.008%
9	3.126	629	633	637	rBV6	1299	1553	0.11%	0.015%
10	3.283	677	682	685	rVB6	1690	1301	0.09%	0.012%
11	3.306	685	689	692	rBV3	1037	931	0.07%	0.009%
12	3.338	696	699	702	rVV5	1255	810	0.06%	0.008%
13	3.364	702	707	710	rVB5	1180	899	0.06%	0.009%
14	3.383	710	713	715	rBV3	1319	771	0.05%	0.007%
15	3.550	762	765	766	rBV2	1497	1028	0.07%	0.010%
16	3.592	776	778	781	rBV4	1569	855	0.06%	0.008%
17	3.743	821	825	826	rBV3	918	641	0.05%	0.006%
18	3.868	863	864	866	rBV	1023	538	0.04%	0.005%
19	3.910	867	877	913	rVV	96587	289660	20.65%	2.770%
20	4.376	1006	1022	1048	rBV	230716	572148	40.79%	5.472%
21	4.527	1066	1069	1071	rBV4	1228	845	0.06%	0.008%
22	4.855	1167	1171	1172	rBV3	1437	900	0.06%	0.009%
23	5.071	1222	1238	1266	rVV2	547133	1402728	100.00%	13.415%
24	5.425	1346	1348	1350	rBV3	1311	849	0.06%	0.008%
25	5.527	1377	1380	1383	rBV4	1981	1006	0.07%	0.010%
26	5.592	1396	1400	1401	rBV3	1069	737	0.05%	0.007%
27	5.643	1403	1416	1435	rBV	407960	810379	57.77%	7.750%
28	5.929	1491	1505	1517	rBV4	32988	72476	5.17%	0.693%
29	6.093	1543	1556	1580	rBV2	312824	636162	45.35%	6.084%
30	6.531	1688	1692	1693	rBV4	1774	1373	0.10%	0.013%
31	6.775	1765	1768	1771	rBV4	1694	1541	0.11%	0.015%
32	6.862	1792	1795	1801	rVB7	1760	1839	0.13%	0.018%
33	6.887	1801	1803	1805	rBV3	976	591	0.04%	0.006%
34	6.929	1814	1816	1820	rVB4	1251	806	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062220\
 Data File : VV017013.D
 Acq On : 22 Jun 2020 11:37
 Operator : SY/MD
 Sample : VV0622WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	7.006	1830	1840	1857	rBV	181454	326090	23.25%	3.119%
36	7.338	1932	1943	1962	rBV	647242	1113068	79.35%	10.645%
37	7.595	2021	2023	2028	rBV6	1412	1093	0.08%	0.010%
38	7.643	2028	2038	2055	rBV	129565	226129	16.12%	2.163%
39	7.810	2085	2090	2093	rBV6	1531	1484	0.11%	0.014%
40	8.109	2173	2183	2211	rBV2	294271	583461	41.59%	5.580%
41	8.421	2278	2280	2282	rBV3	1695	834	0.06%	0.008%
42	8.595	2331	2334	2337	rBV5	1262	987	0.07%	0.009%
43	8.649	2348	2351	2352	rBV2	1093	641	0.05%	0.006%
44	8.707	2366	2369	2372	rBV5	1298	1006	0.07%	0.010%
45	8.875	2407	2421	2444	rBV	612192	989544	70.54%	9.464%
46	9.026	2466	2468	2469	rBV3	1457	621	0.04%	0.006%
47	9.161	2502	2510	2511	rBV8	3426	3392	0.24%	0.032%
48	9.350	2567	2569	2573	rVB4	1897	1100	0.08%	0.011%
49	9.424	2589	2592	2595	rBV4	955	632	0.05%	0.006%
50	9.453	2599	2601	2604	rBV4	893	584	0.04%	0.006%
51	9.637	2656	2658	2663	rVB4	1504	867	0.06%	0.008%
52	9.675	2663	2670	2671	rBV5	1344	1423	0.10%	0.014%
53	9.749	2689	2693	2696	rBV4	924	926	0.07%	0.009%
54	9.801	2705	2709	2710	rBV3	1691	1117	0.08%	0.011%
55	9.862	2723	2728	2733	rVB8	1308	1355	0.10%	0.013%
56	9.887	2734	2736	2739	rVB3	1179	628	0.04%	0.006%
57	9.910	2739	2743	2744	rBV3	1194	783	0.06%	0.007%
58	10.103	2800	2803	2805	rBV3	1330	933	0.07%	0.009%
59	10.135	2811	2813	2816	rBV4	1324	687	0.05%	0.007%
60	10.190	2827	2830	2832	rBV2	1412	893	0.06%	0.009%
61	10.238	2834	2845	2862	rVV	373225	588005	41.92%	5.623%
62	10.338	2874	2876	2879	rBV2	1103	527	0.04%	0.005%
63	10.469	2914	2917	2919	rBV2	872	565	0.04%	0.005%
64	10.662	2974	2977	2986	rVB9	2250	3139	0.22%	0.030%
65	10.707	2986	2991	2992	rBV3	1478	1348	0.10%	0.013%
66	10.759	3005	3007	3010	rVB4	1024	516	0.04%	0.005%
67	10.891	3045	3048	3050	rBV4	1518	1022	0.07%	0.010%
68	10.923	3055	3058	3059	rBV3	1006	545	0.04%	0.005%
69	11.270	3155	3166	3186	rBV	609734	937538	66.84%	8.966%
70	11.527	3244	3246	3250	rBV4	1022	668	0.05%	0.006%
71	11.575	3259	3261	3262	rBV2	1226	574	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062220\
 Data File : VV017013.D
 Acq On : 22 Jun 2020 11:37
 Operator : SY/MD
 Sample : VV0622WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	11.646	3269	3283	3300	rBV	688902	1063599	75.82%	10.172%
73	11.817	3333	3336	3338	rBV4	793	585	0.04%	0.006%
74	11.919	3364	3368	3371	rBV4	1038	992	0.07%	0.009%
75	11.981	3385	3387	3391	rBV4	1081	589	0.04%	0.006%
76	12.209	3455	3458	3464	rVB7	1406	1512	0.11%	0.014%
77	12.450	3530	3533	3534	rBV3	1465	765	0.05%	0.007%
78	12.569	3567	3570	3575	rBV6	1270	1322	0.09%	0.013%
79	12.598	3575	3579	3580	rBV4	2325	931	0.07%	0.009%
80	12.620	3583	3586	3590	rBV4	1758	1125	0.08%	0.011%
81	12.656	3593	3597	3598	rBV4	1979	1297	0.09%	0.012%
82	12.858	3658	3660	3664	rBV4	1117	1041	0.07%	0.010%
83	12.968	3691	3694	3696	rBV3	1112	684	0.05%	0.007%
84	13.009	3703	3707	3712	rBV6	1621	1954	0.14%	0.019%
85	13.042	3715	3717	3720	rVV3	1002	609	0.04%	0.006%
86	13.157	3747	3753	3755	rBV6	1416	1365	0.10%	0.013%
87	13.222	3772	3773	3776	rBV3	1242	577	0.04%	0.006%
88	13.353	3812	3814	3819	rBV2	1776	1132	0.08%	0.011%
89	13.530	3863	3869	3875	rBV9	3825	5638	0.40%	0.054%
90	13.601	3889	3891	3893	rBV3	1258	684	0.05%	0.007%
91	13.656	3904	3908	3912	rVB6	881	832	0.06%	0.008%
92	13.939	3992	3996	3998	rBV4	1203	976	0.07%	0.009%
93	13.977	4006	4008	4012	rBV4	982	577	0.04%	0.006%
94	14.009	4016	4018	4022	rBV3	1366	860	0.06%	0.008%
95	14.302	4106	4109	4110	rBV2	1034	562	0.04%	0.005%
96	14.395	4135	4138	4140	rBV3	1937	1307	0.09%	0.012%
97	14.627	4207	4210	4214	rBV4	1097	1003	0.07%	0.010%
98	14.672	4221	4224	4227	rBV4	1487	1274	0.09%	0.012%
99	15.009	4327	4329	4331	rBV3	1134	585	0.04%	0.006%
100	15.083	4350	4352	4358	rBV7	1862	1416	0.10%	0.014%


Sum of corrected areas: 10456214

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062220\
Data File : VV017013.D
Acq On : 22 Jun 2020 11:37
Operator : SY/MD
Sample : VV0622WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK92

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

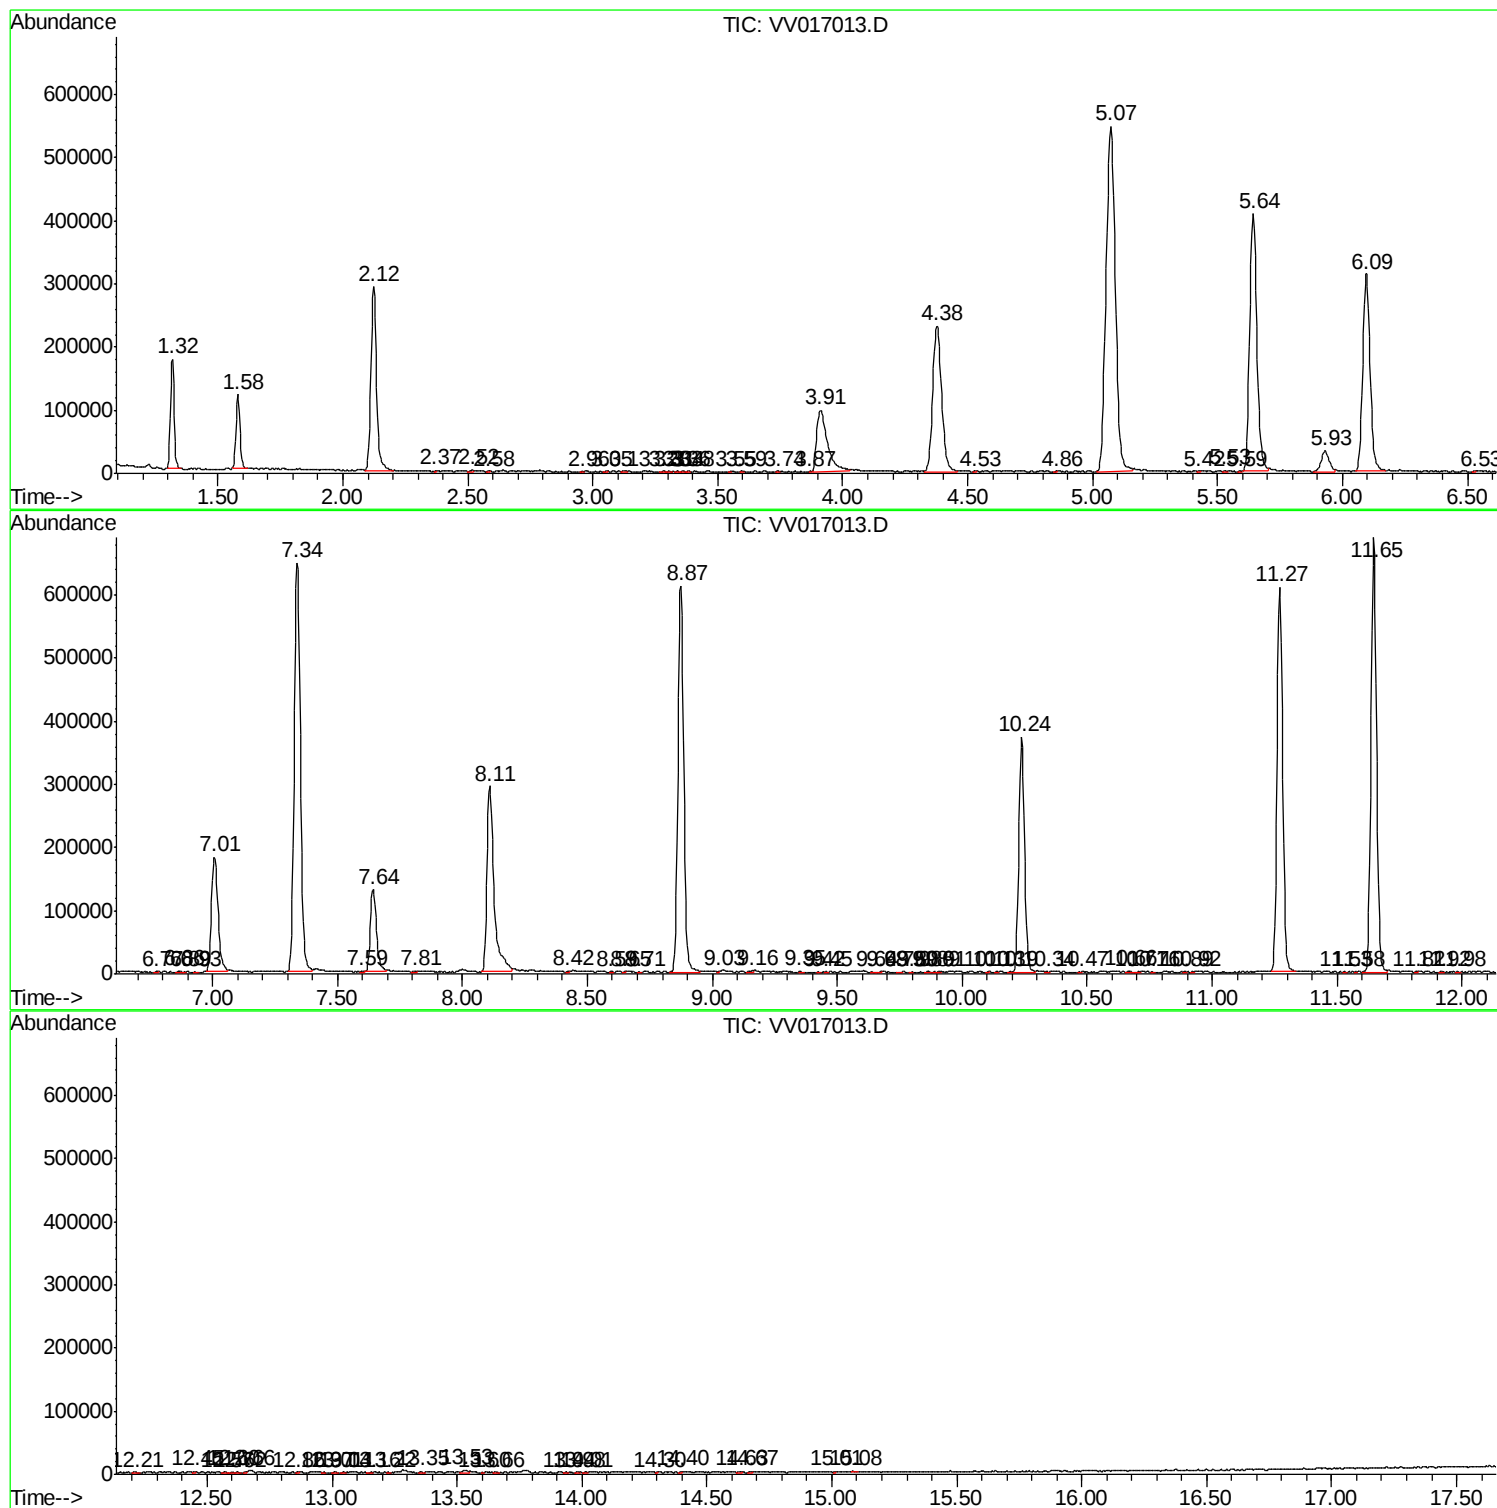

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062220\
Data File : VV017013.D
Acq On : 22 Jun 2020 11:37
Operator : SY/MD
Sample : VV0622WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK92

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV062220\
Data File : VV017013.D
Acq On : 22 Jun 2020 11:37
Operator : SY/MD
Sample : VV0622WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK92

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc