

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062220\
 Data File : VV017014.D
 Acq On : 22 Jun 2020 12:06
 Operator : SY/MD
 Sample : L3074-02DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M04DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB2	193648	202563	14.57%	1.523%
2	1.579	145	152	161	rBV	123621	133423	9.59%	1.003%
3	2.123	311	321	341	rVB	289121	438995	31.57%	3.301%
4	2.383	400	402	403	rBV2	1189	523	0.04%	0.004%
5	2.521	436	445	446	rBV6	4255	4691	0.34%	0.035%
6	2.586	463	465	467	rBV2	1126	529	0.04%	0.004%
7	2.634	476	480	481	rBV4	1001	771	0.06%	0.006%
8	2.672	490	492	493	rBV2	1517	626	0.05%	0.005%
9	2.782	517	526	527	rBV9	4014	5463	0.39%	0.041%
10	2.942	574	576	582	rBV4	1346	1362	0.10%	0.010%
11	3.010	594	597	599	rBV3	2066	1396	0.10%	0.010%
12	3.074	615	617	620	rVB2	1306	691	0.05%	0.005%
13	3.097	620	624	625	rBV2	1388	847	0.06%	0.006%
14	3.126	631	633	635	rBV3	1234	569	0.04%	0.004%
15	3.155	640	642	647	rVB5	2347	1636	0.12%	0.012%
16	3.354	697	704	705	rBV5	1411	1435	0.10%	0.011%
17	3.479	741	743	747	rBV4	856	635	0.05%	0.005%
18	3.553	761	766	768	rBV5	1175	906	0.07%	0.007%
19	3.631	786	790	792	rBV5	1235	650	0.05%	0.005%
20	3.933	865	884	912	rBV3	433409	1240172	89.18%	9.325%
21	4.373	1007	1021	1048	rVB	229811	564058	40.56%	4.241%
22	4.659	1109	1110	1113	rBV3	1295	692	0.05%	0.005%
23	4.737	1132	1134	1137	rVB4	1429	706	0.05%	0.005%
24	4.753	1137	1139	1141	rBV3	1077	494	0.04%	0.004%
25	4.910	1185	1188	1189	rBV3	1225	675	0.05%	0.005%
26	4.946	1197	1199	1202	rBV3	1365	959	0.07%	0.007%
27	5.000	1214	1216	1217	rBV2	1014	499	0.04%	0.004%
28	5.071	1220	1238	1259	rVV2	544269	1390615	100.00%	10.456%
29	5.338	1319	1321	1325	rVB5	1718	1154	0.08%	0.009%
30	5.409	1341	1343	1345	rBV3	948	499	0.04%	0.004%
31	5.640	1402	1415	1439	rBV	418656	833564	59.94%	6.268%
32	5.875	1485	1488	1491	rBV4	1539	842	0.06%	0.006%
33	5.936	1493	1507	1526	rBV4	255260	525815	37.81%	3.954%
34	6.093	1544	1556	1578	rVB	305805	616288	44.32%	4.634%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062220\
 Data File : VV017014.D
 Acq On : 22 Jun 2020 12:06
 Operator : SY/MD
 Sample : L3074-02DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M04DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.473	1669	1674	1676	rBV3	1099	919	0.07%	0.007%
36	6.553	1696	1699	1702	rBV4	1688	961	0.07%	0.007%
37	6.650	1727	1729	1731	rBV3	1869	806	0.06%	0.006%
38	6.737	1753	1756	1758	rBV3	1457	731	0.05%	0.005%
39	6.778	1767	1769	1775	rVB6	1632	1104	0.08%	0.008%
40	6.807	1775	1778	1780	rBV3	1219	753	0.05%	0.006%
41	6.839	1785	1788	1791	rBV3	1569	1047	0.08%	0.008%
42	6.904	1805	1808	1810	rVB4	1158	668	0.05%	0.005%
43	7.007	1829	1840	1860	rBV	179890	322814	23.21%	2.427%
44	7.267	1920	1921	1926	rVB3	1873	1116	0.08%	0.008%
45	7.338	1930	1943	1960	rBV	646338	1121548	80.65%	8.433%
46	7.640	2026	2037	2056	rBV	128507	228595	16.44%	1.719%
47	7.788	2081	2083	2084	rBV2	1526	572	0.04%	0.004%
48	7.897	2111	2117	2120	rBV6	1881	1845	0.13%	0.014%
49	7.997	2134	2148	2171	rBV	800198	1358328	97.68%	10.213%
50	8.106	2172	2182	2221	rVB2	297750	586393	42.17%	4.409%
51	8.376	2264	2266	2274	rVB8	1794	1775	0.13%	0.013%
52	8.592	2330	2333	2336	rVB4	1832	1032	0.07%	0.008%
53	8.614	2336	2340	2344	rBV7	1554	1620	0.12%	0.012%
54	8.656	2351	2353	2357	rVB5	1388	863	0.06%	0.006%
55	8.695	2362	2365	2367	rBV4	1508	942	0.07%	0.007%
56	8.797	2394	2397	2399	rBV4	1930	1455	0.10%	0.011%
57	8.871	2406	2420	2437	rBV	622519	1014299	72.94%	7.627%
58	9.100	2489	2491	2494	rBV3	1961	1080	0.08%	0.008%
59	9.154	2503	2508	2510	rBV6	2157	2033	0.15%	0.015%
60	9.302	2549	2554	2556	rBV5	1613	1119	0.08%	0.008%
61	9.608	2647	2649	2652	rVB5	1242	595	0.04%	0.004%
62	9.772	2698	2700	2707	rBV7	1235	1612	0.12%	0.012%
63	9.878	2730	2733	2738	rVB8	1311	1109	0.08%	0.008%
64	9.907	2738	2742	2745	rBV6	1271	1060	0.08%	0.008%
65	9.997	2767	2770	2772	rBV3	1134	638	0.05%	0.005%
66	10.032	2779	2781	2785	rVB2	1357	728	0.05%	0.005%
67	10.058	2785	2789	2791	rBV5	1467	1215	0.09%	0.009%
68	10.084	2794	2797	2800	rVB4	1053	603	0.04%	0.005%
69	10.100	2800	2802	2806	rBV4	1094	710	0.05%	0.005%
70	10.132	2808	2812	2816	rBV6	1849	1526	0.11%	0.011%
71	10.190	2828	2830	2832	rBV3	1734	995	0.07%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062220\
 Data File : VV017014.D
 Acq On : 22 Jun 2020 12:06
 Operator : SY/MD
 Sample : L3074-02DL 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9M04DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	10.238	2833	2845	2863	rVV	362977	576430	41.45%	4.334%
73	10.412	2897	2899	2901	rBV3	943	595	0.04%	0.004%
74	10.701	2984	2989	2991	rBV5	1352	1503	0.11%	0.011%
75	10.781	3012	3014	3015	rBV2	1107	560	0.04%	0.004%
76	10.977	3069	3075	3077	rBV6	1288	1197	0.09%	0.009%
77	11.109	3114	3116	3118	rBV3	1003	602	0.04%	0.005%
78	11.167	3131	3134	3136	rBV3	2076	1325	0.10%	0.010%
79	11.270	3155	3166	3186	rBV	643593	980915	70.54%	7.376%
80	11.421	3210	3213	3219	rBV7	2068	1734	0.12%	0.013%
81	11.540	3245	3250	3251	rBV4	2070	1303	0.09%	0.010%
82	11.563	3255	3257	3261	rBV3	1706	1333	0.10%	0.010%
83	11.646	3270	3283	3301	rBV	693263	1074382	77.26%	8.078%
84	11.887	3356	3358	3363	rVB4	1479	934	0.07%	0.007%
85	12.158	3440	3442	3445	rBV2	1422	781	0.06%	0.006%
86	12.276	3476	3479	3481	rVV5	1542	726	0.05%	0.005%
87	12.366	3503	3507	3509	rBV4	1515	1035	0.07%	0.008%
88	12.460	3534	3536	3541	rVV4	1522	897	0.06%	0.007%
89	12.592	3574	3577	3578	rBV3	967	593	0.04%	0.004%
90	12.756	3625	3628	3632	rBV5	1497	1481	0.11%	0.011%
91	12.903	3670	3674	3676	rBV3	1659	1230	0.09%	0.009%
92	13.283	3789	3792	3795	rBV3	2946	2028	0.15%	0.015%
93	13.447	3839	3843	3845	rBV3	2000	1834	0.13%	0.014%
94	13.595	3886	3889	3891	rBV3	1064	644	0.05%	0.005%
95	13.694	3918	3920	3922	rVB3	1579	565	0.04%	0.004%
96	13.916	3986	3989	3993	rBV5	1713	1139	0.08%	0.009%
97	13.955	3999	4001	4003	rBV3	2018	1038	0.07%	0.008%
98	14.604	4201	4203	4205	rBV4	990	500	0.04%	0.004%
99	14.685	4226	4228	4231	rBV4	1278	711	0.05%	0.005%
100	14.981	4317	4320	4324	rBV4	1741	1412	0.10%	0.011%


Sum of corrected areas: 13299379

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062220\
Data File : VV017014.D
Acq On : 22 Jun 2020 12:06
Operator : SY/MD
Sample : L3074-02DL 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
F9M04DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

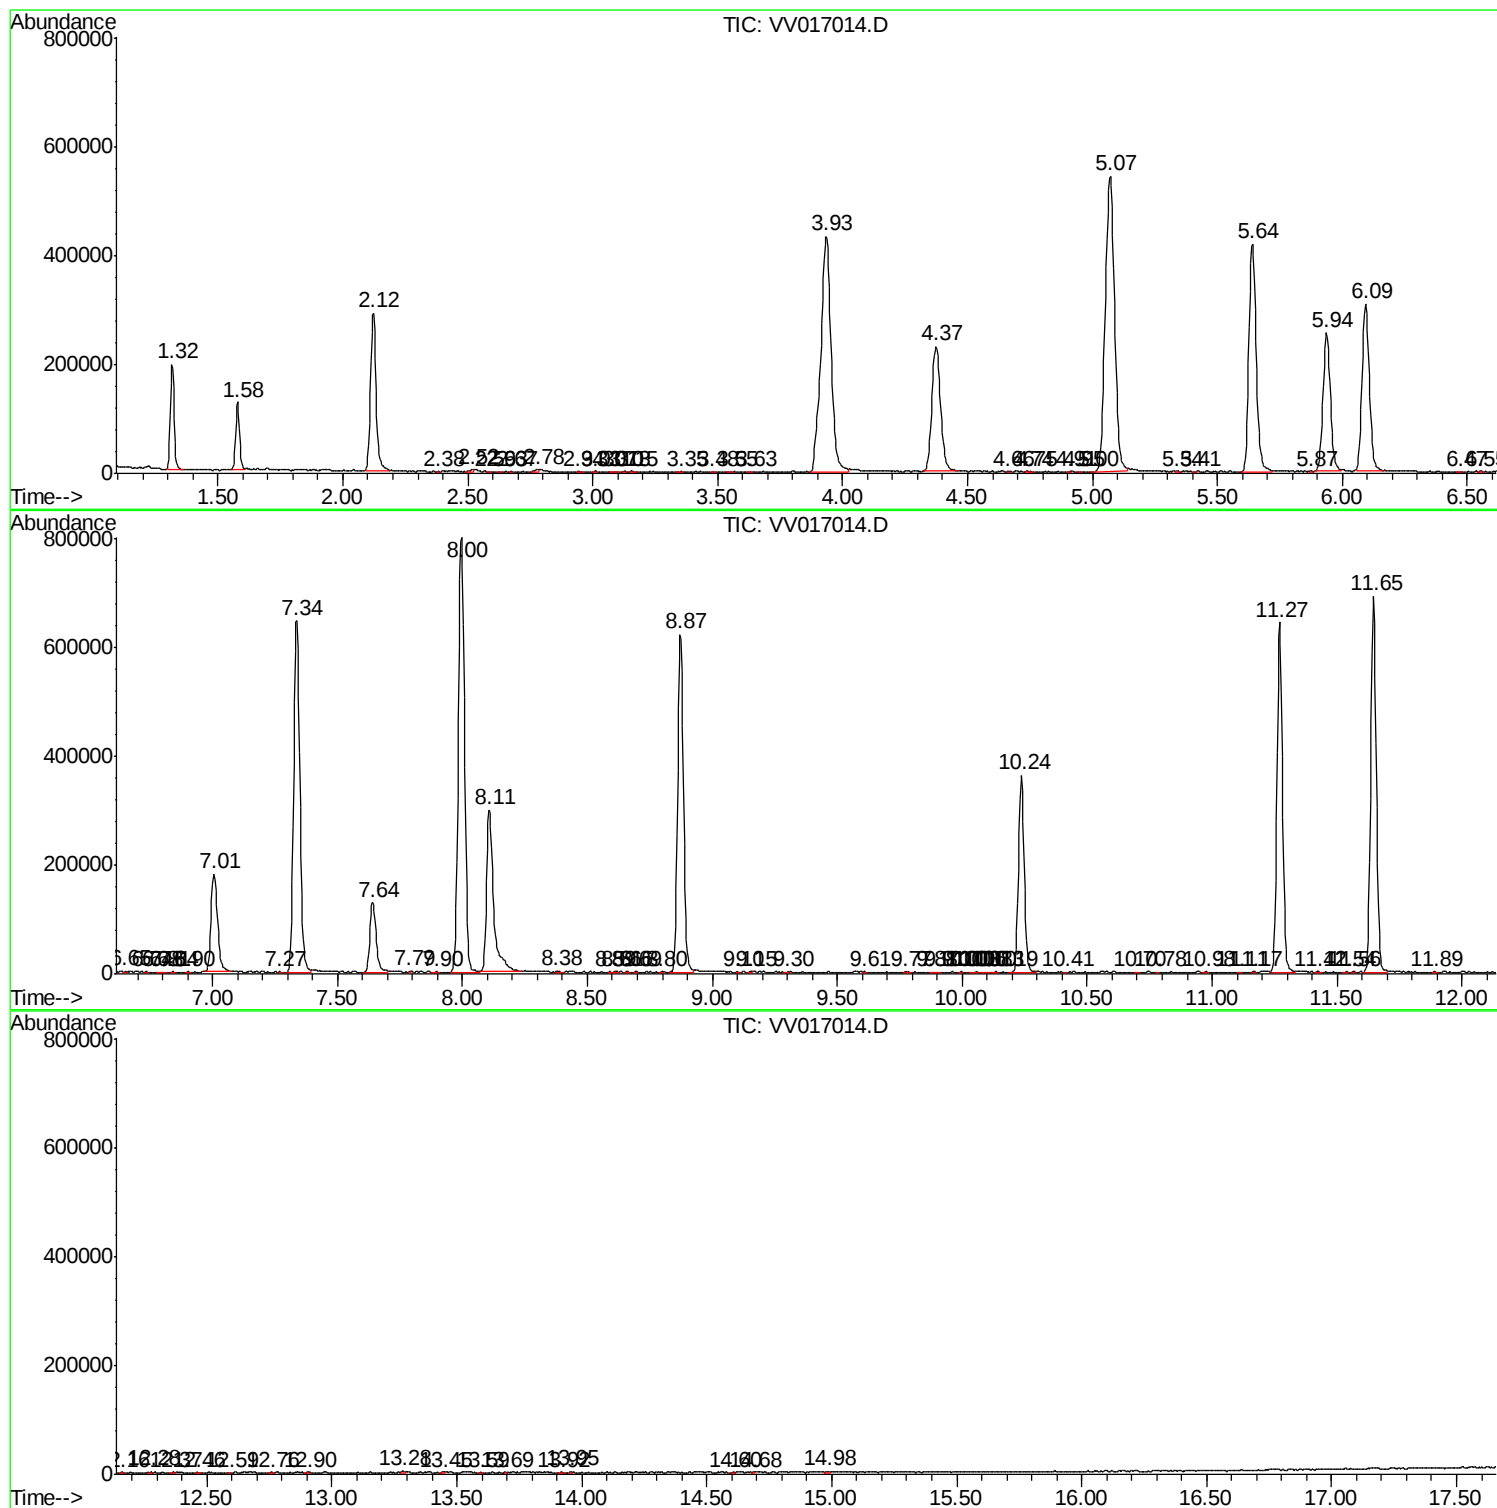

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV062220\
Data File : VV017014.D
Acq On : 22 Jun 2020 12:06
Operator : SY/MD
Sample : L3074-02DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M04DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062220\
Data File : VV017014.D
Acq On : 22 Jun 2020 12:06
Operator : SY/MD
Sample : L3074-02DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9M04DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc