


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062220\
 Data File : VV017011.D
 Acq On : 22 Jun 2020 09:33
 Operator : SY/MD
 Sample : BFB93
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB93

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 23 10:40:00 2020

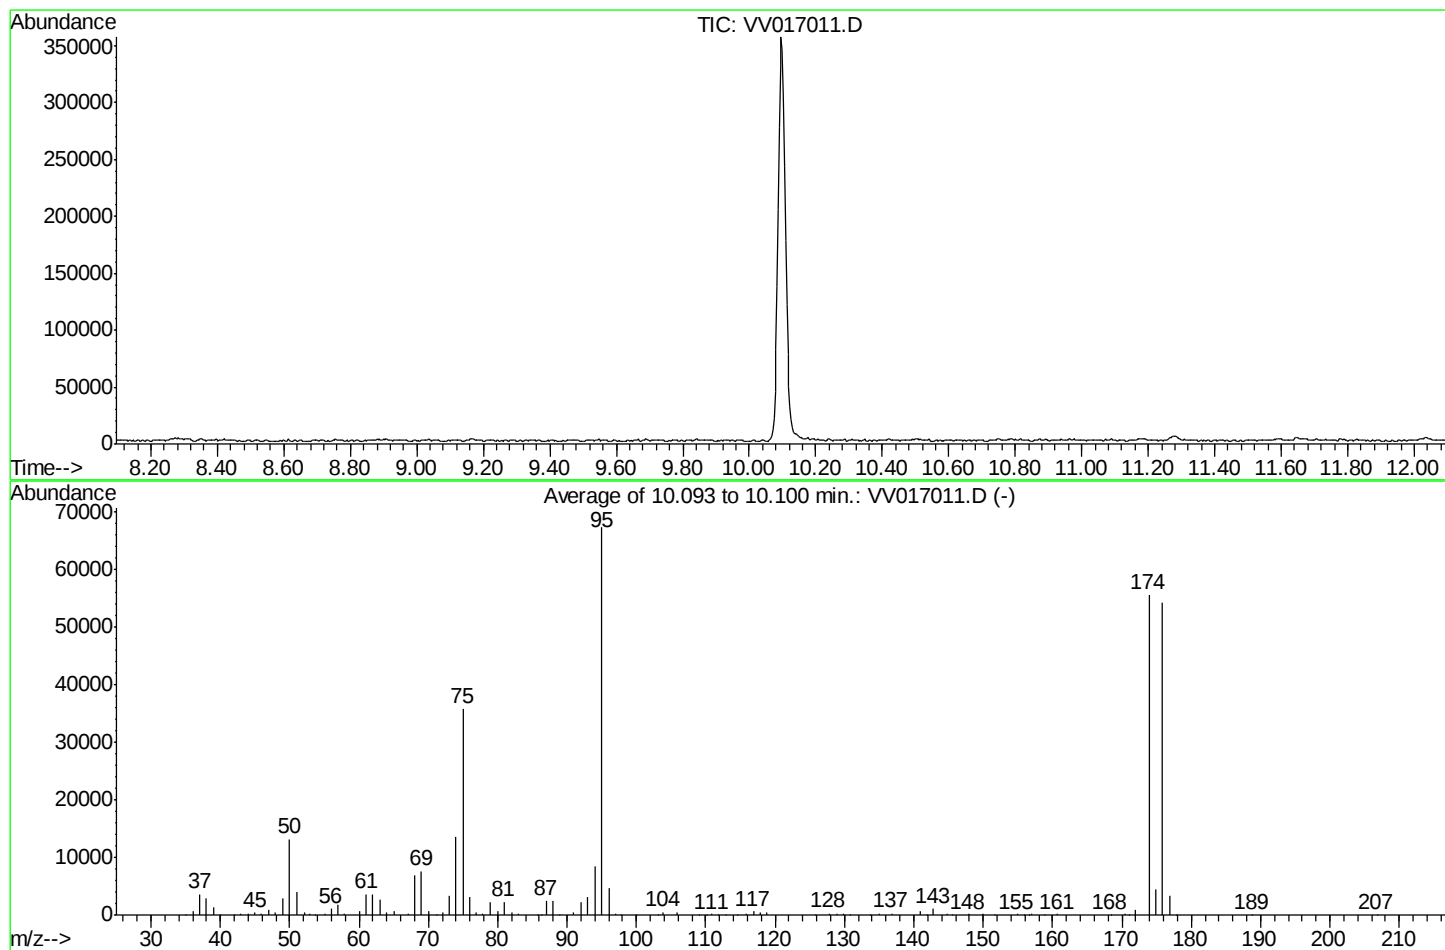

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	13232	PASS
75	95	30	80	53.3	35914	PASS
95	95	100	100	100.0	67357	PASS
96	95	5	9	6.9	4680	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.6	55669	PASS
175	174	5	9	7.9	4378	PASS
176	174	95	101	97.5	54301	PASS
177	176	5	9	6.3	3425	PASS

m/z	Abundance
35.00	129.0
36.00	715.0
37.00	3523.0
38.00	3090.0
39.00	1411.0
39.90	278.0
42.10	104.0
42.90	176.0
44.00	755.0
45.00	543.0
45.80	138.0
46.30	196.0
47.00	927.0
47.90	469.0
49.00	3130.0
50.00	13181.0
51.00	3825.0
52.00	324.0
52.90	246.0
55.20	258.0
56.00	959.0
57.00	1680.0
57.90	132.0
58.00	132.0
60.00	665.0
61.00	3443.0
62.00	3467.0
63.00	2785.0
64.00	409.0
65.00	716.0
67.00	295.0
68.00	6761.0
69.00	7646.0
70.00	554.0
71.10	116.0
72.00	353.0
73.00	2995.0
74.00	13337.0
75.00	35040.0
76.00	3340.0
76.90	374.0
77.70	317.0
78.90	2297.0
80.00	584.0
80.90	2243.0
82.00	616.0
83.10	113.0
86.20	249.0
87.00	2520.0
87.90	2412.0
90.90	364.0
92.00	2217.0
93.00	2816.0
94.00	8350.0
95.00	65408.0
96.00	4540.0
97.00	170.0
103.00	124.0
103.90	470.0
105.80	306.0
110.10	141.0
110.90	118.0
111.70	136.0
113.00	106.0
115.90	297.0
116.90	558.0
117.90	403.0
118.90	461.0
127.80	267.0
128.80	166.0
129.80	239.0
130.80	134.0
133.70	115.0
134.90	193.0
136.80	230.0
141.00	913.0
141.90	107.0
142.90	885.0
144.90	204.0
147.90	141.0
150.00	166.0
151.70	123.0
154.90	192.0
157.00	230.0
160.70	120.0
170.50	108.0
171.00	158.0
171.90	777.0
173.90	53024.0
174.90	4102.0
175.90	50208.0
177.00	3236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

177.90

182.0

Instrument :

MSVOA_V

ClientSampleId :

BFB93

m/z	Abundance
36.00	714.0
37.00	3755.0
38.00	3118.0
39.00	1553.0
39.90	362.0
42.00	108.0
42.90	157.0
44.00	734.0
45.00	506.0
45.80	127.0
47.00	994.0
47.90	527.0
49.00	3013.0
50.00	13649.0
51.00	4380.0
52.10	378.0
53.00	229.0
53.70	120.0
55.20	299.0
56.00	1063.0
57.00	1938.0
57.80	143.0
60.00	787.0
61.00	3753.0
62.00	3699.0
63.00	2875.0
64.00	458.0
65.00	748.0
67.00	335.0
68.00	7135.0
69.00	7816.0
70.00	587.0
71.10	108.0
72.00	421.0
73.00	3449.0
74.00	14189.0
75.00	37200.0
76.00	3191.0
76.90	408.0
77.80	297.0
78.90	2416.0
80.00	745.0
80.90	2361.0
82.00	525.0
83.00	128.0
87.00	2622.0
87.90	2511.0
90.90	358.0
92.00	2409.0
93.00	3117.0
94.00	8695.0
95.00	69536.0
96.00	4888.0
97.00	172.0
97.70	126.0
100.00	117.0
103.90	500.0
105.80	390.0
109.10	136.0
110.00	106.0
110.90	157.0
111.80	119.0
112.90	121.0
114.60	114.0
115.90	301.0
116.90	651.0
117.80	359.0
118.80	428.0
125.80	115.0
127.70	296.0
128.80	225.0
129.80	288.0
130.80	139.0
135.00	231.0
136.90	237.0
141.00	789.0
142.80	1086.0
144.80	223.0
145.60	145.0
148.00	147.0
150.00	153.0
151.70	127.0
154.90	175.0
157.00	169.0
160.70	116.0
168.40	120.0
170.60	126.0
170.90	140.0
171.90	886.0
173.90	57712.0
174.90	4499.0
175.90	56432.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

177.00

177.90

3593.0

144.0

Instrument :

MSVOA_V

ClientSampleId :

BFB93

m/z	Abundance
36.00	670.0
37.00	3564.0
38.00	2810.0
39.00	1527.0
40.00	478.0
41.60	114.0
42.10	107.0
42.80	130.0
44.00	778.0
45.00	497.0
45.80	117.0
47.00	1042.0
47.90	514.0
49.00	2694.0
50.00	12868.0
51.00	4246.0
52.10	400.0
53.00	211.0
53.60	144.0
55.10	292.0
56.00	1184.0
57.00	2076.0
57.80	155.0
60.00	779.0
61.00	3654.0
62.00	3566.0
63.00	2688.0
64.00	417.0
65.00	685.0
67.00	318.0
68.00	6951.0
69.00	7377.0
70.00	611.0
71.10	110.0
72.00	407.0
73.00	3431.0
74.00	13237.0
75.00	35504.0
76.00	2846.0
77.00	396.0
77.90	300.0
78.90	2238.0
80.00	813.0
80.90	2382.0
81.90	487.0
82.90	148.0
85.80	104.0
87.00	2540.0
87.90	2219.0
88.80	152.0
90.80	319.0
92.00	2296.0
93.00	3131.0
94.00	8388.0
95.00	67128.0
96.00	4613.0
97.00	195.0
103.80	457.0
105.90	432.0
109.00	133.0
110.90	189.0
112.80	128.0
114.60	124.0
115.90	280.0
116.90	664.0
117.80	305.0
118.80	414.0
127.70	331.0
128.90	217.0
129.80	313.0
135.00	225.0
136.90	228.0
140.90	643.0
142.80	1082.0
144.80	195.0
145.60	193.0
147.80	154.0
150.00	116.0
154.90	189.0
155.80	117.0
156.70	112.0
158.90	107.0
160.70	148.0
168.30	139.0
170.60	144.0
171.90	881.0
173.90	56272.0
174.90	4533.0
175.90	56264.0
177.00	3446.0
188.80	107.0
206.80	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93

m/z	Abundance
36.00	134.0
36.70	131.0
37.40	106.0
39.00	170.0
39.90	361.0
41.10	137.0
41.60	114.0
43.90	609.0
44.90	106.0
46.30	110.0
51.20	117.0
58.00	112.0
74.10	108.0
82.10	118.0
132.40	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB93