
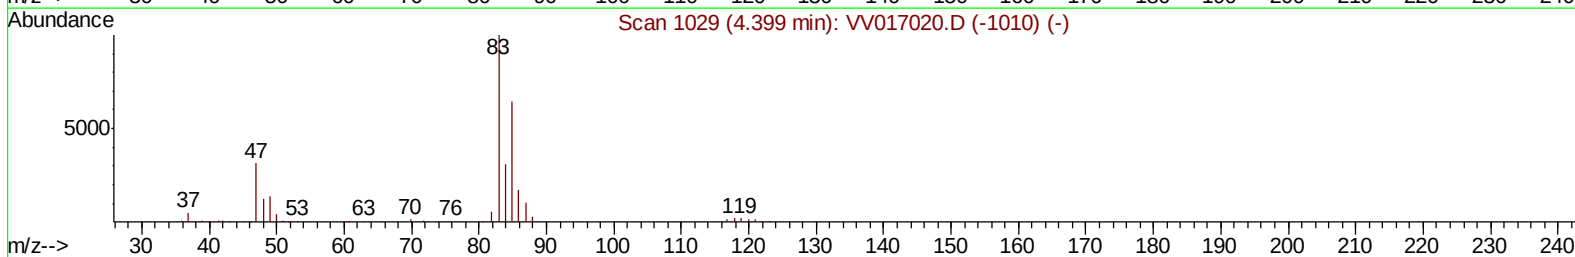
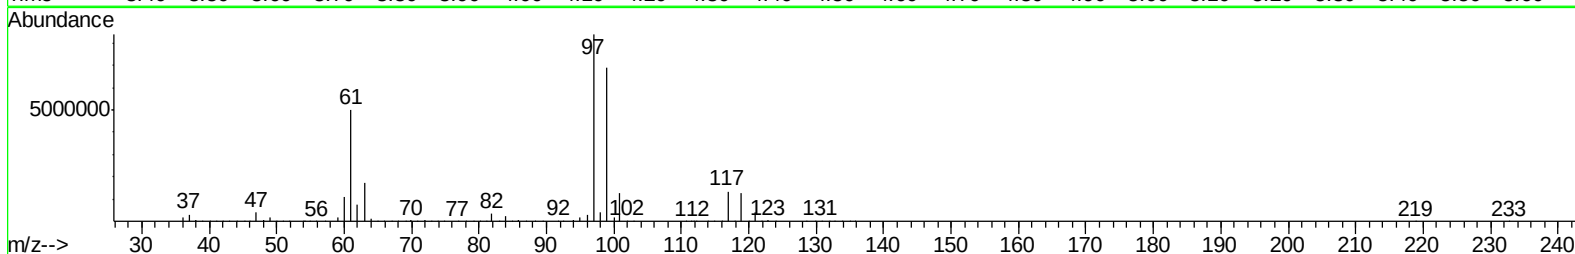


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062320\
Data File : VV017022.D
Acq On : 22 Jun 2020 17:22
Operator : SY/MD
Sample : L3067-01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Jun 23 04:55:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 23 04:53:49 2020
Response via : Initial Calibration

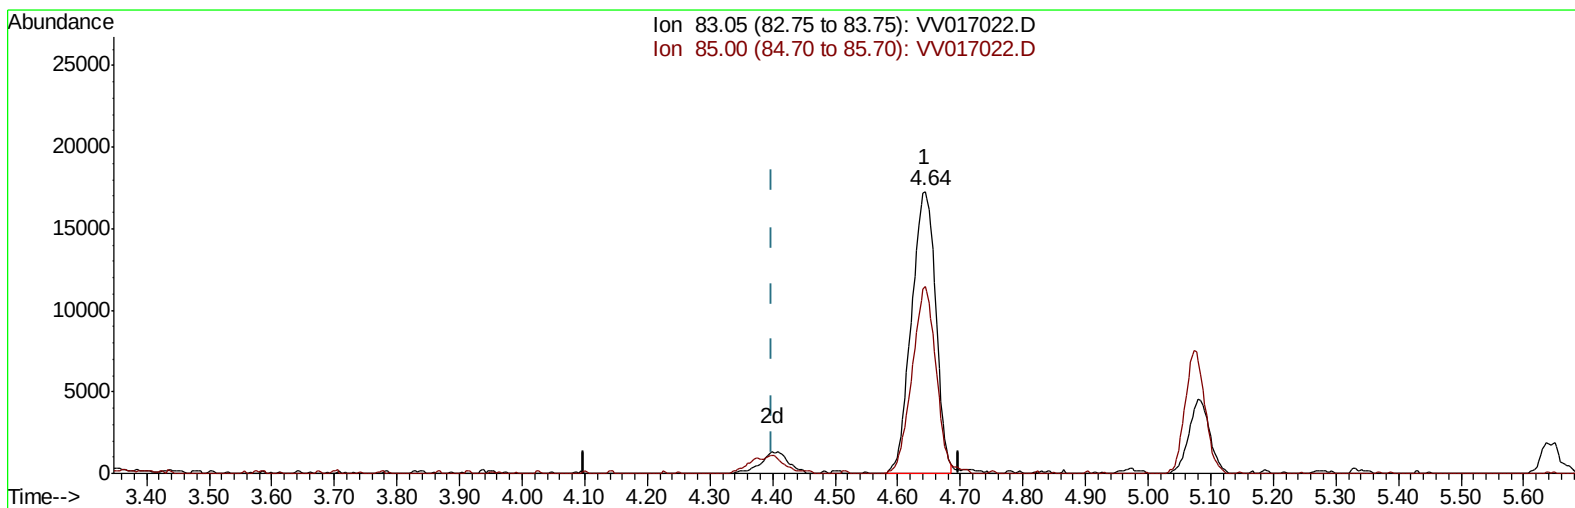

TIC: VV017022.D

(25) Chloroform (T)

4.643min (+0.244) 1.89ug/L

response 46637

Ion	Exp%	Act%
83.05	100	100
85.00	63.20	66.31
0.00	0.00	0.00
0.00	0.00	0.00