
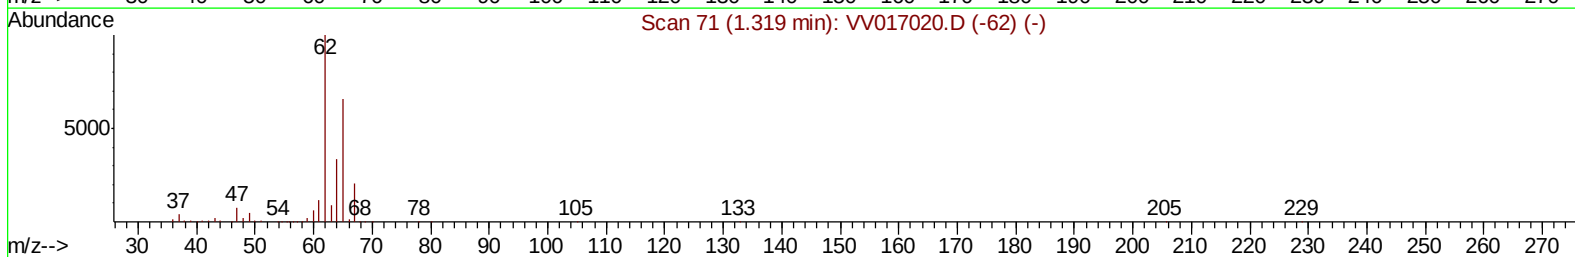
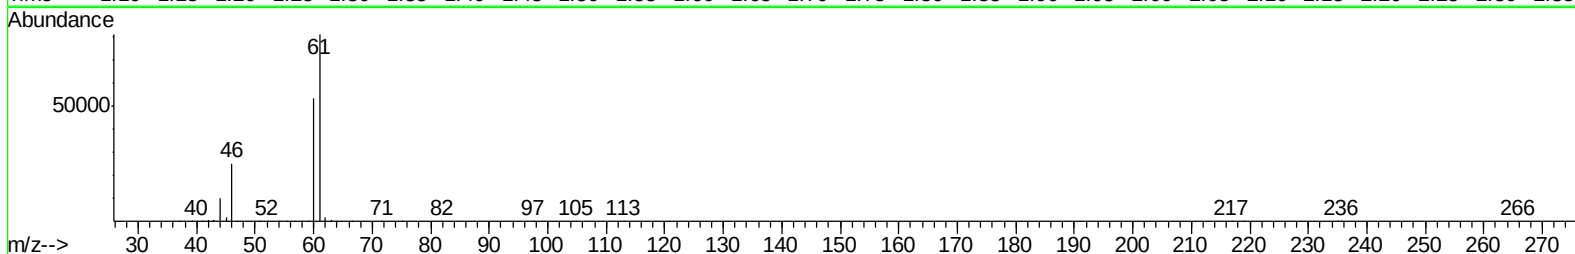


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062320\
Data File : VV017041.D
Acq On : 23 Jun 2020 00:57
Operator : SY/MD
Sample : L3067-20
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Jun 23 05:01:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 23 04:53:49 2020
Response via : Initial Calibration

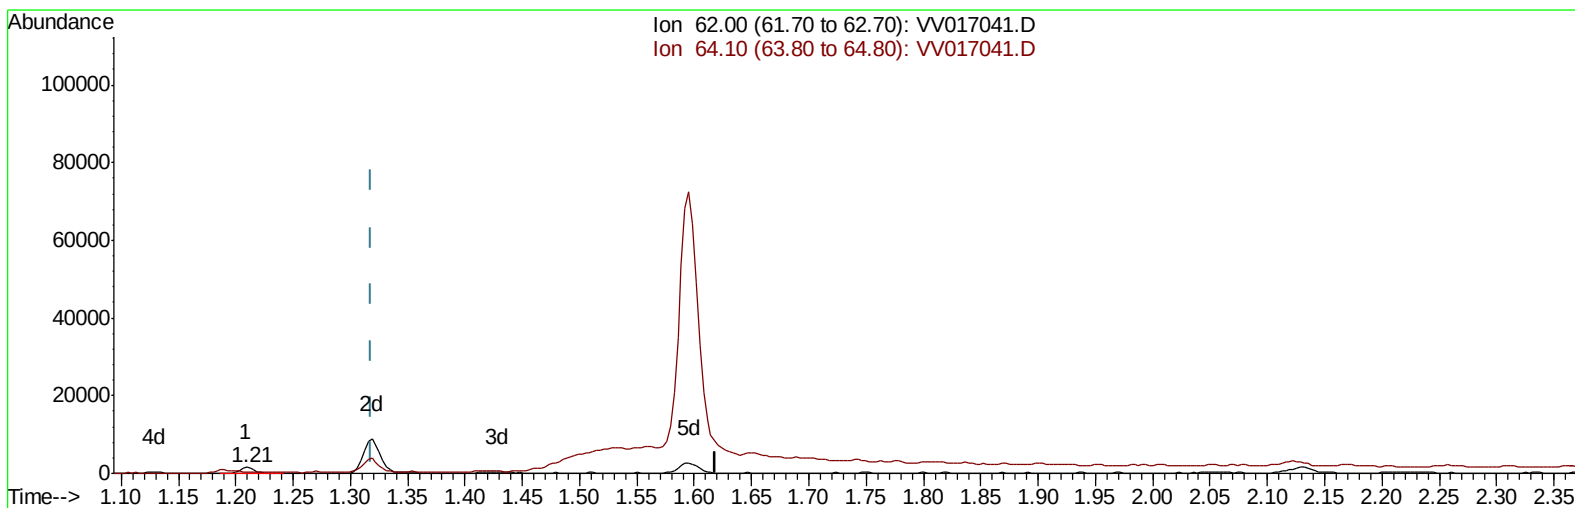

TIC: VV017041.D

(5) Vinyl chloride (T)

1.209min (-0.109) 0.13ug/L

response 1544

Ion	Exp%	Act%
62.00	100	100
64.10	32.10	24.89
0.00	0.00	0.00
0.00	0.00	0.00