

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062320\
 Data File : VV017021.D
 Acq On : 22 Jun 2020 16:59
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK50

Quant Time: Jun 23 05:05:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 23 04:53:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	194526	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	185504	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	90264	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	50305	4.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.20%
7) Chloroethane-d5	1.58	69	40101	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.40%
11) 1,1-Dichloroethene-d2	2.12	63	75417	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.94	46	148958	50.06	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.12%
24) Chloroform-d	4.38	84	118912	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.06	65	66740	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.80%
32) Benzene-d6	5.07	84	235133	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.09	67	68304	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	7.34	98	212978	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
45) trans-1,3-Dichloropropene-	7.64	79	27395	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
48) 2-Hexanone-d5	8.11	63	89806	39.28	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.56%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	43476	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	83647	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%


Target Compounds					Ovalue
25) Chloroform	4.40	83	4716	0.194 ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062320\
Data File : VV017021.D
Acq On : 22 Jun 2020 16:59
Operator : SY/MD
Sample : VV0623WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK50

Quant Time: Jun 23 05:05:37 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 23 04:53:49 2020
Response via : Initial Calibration

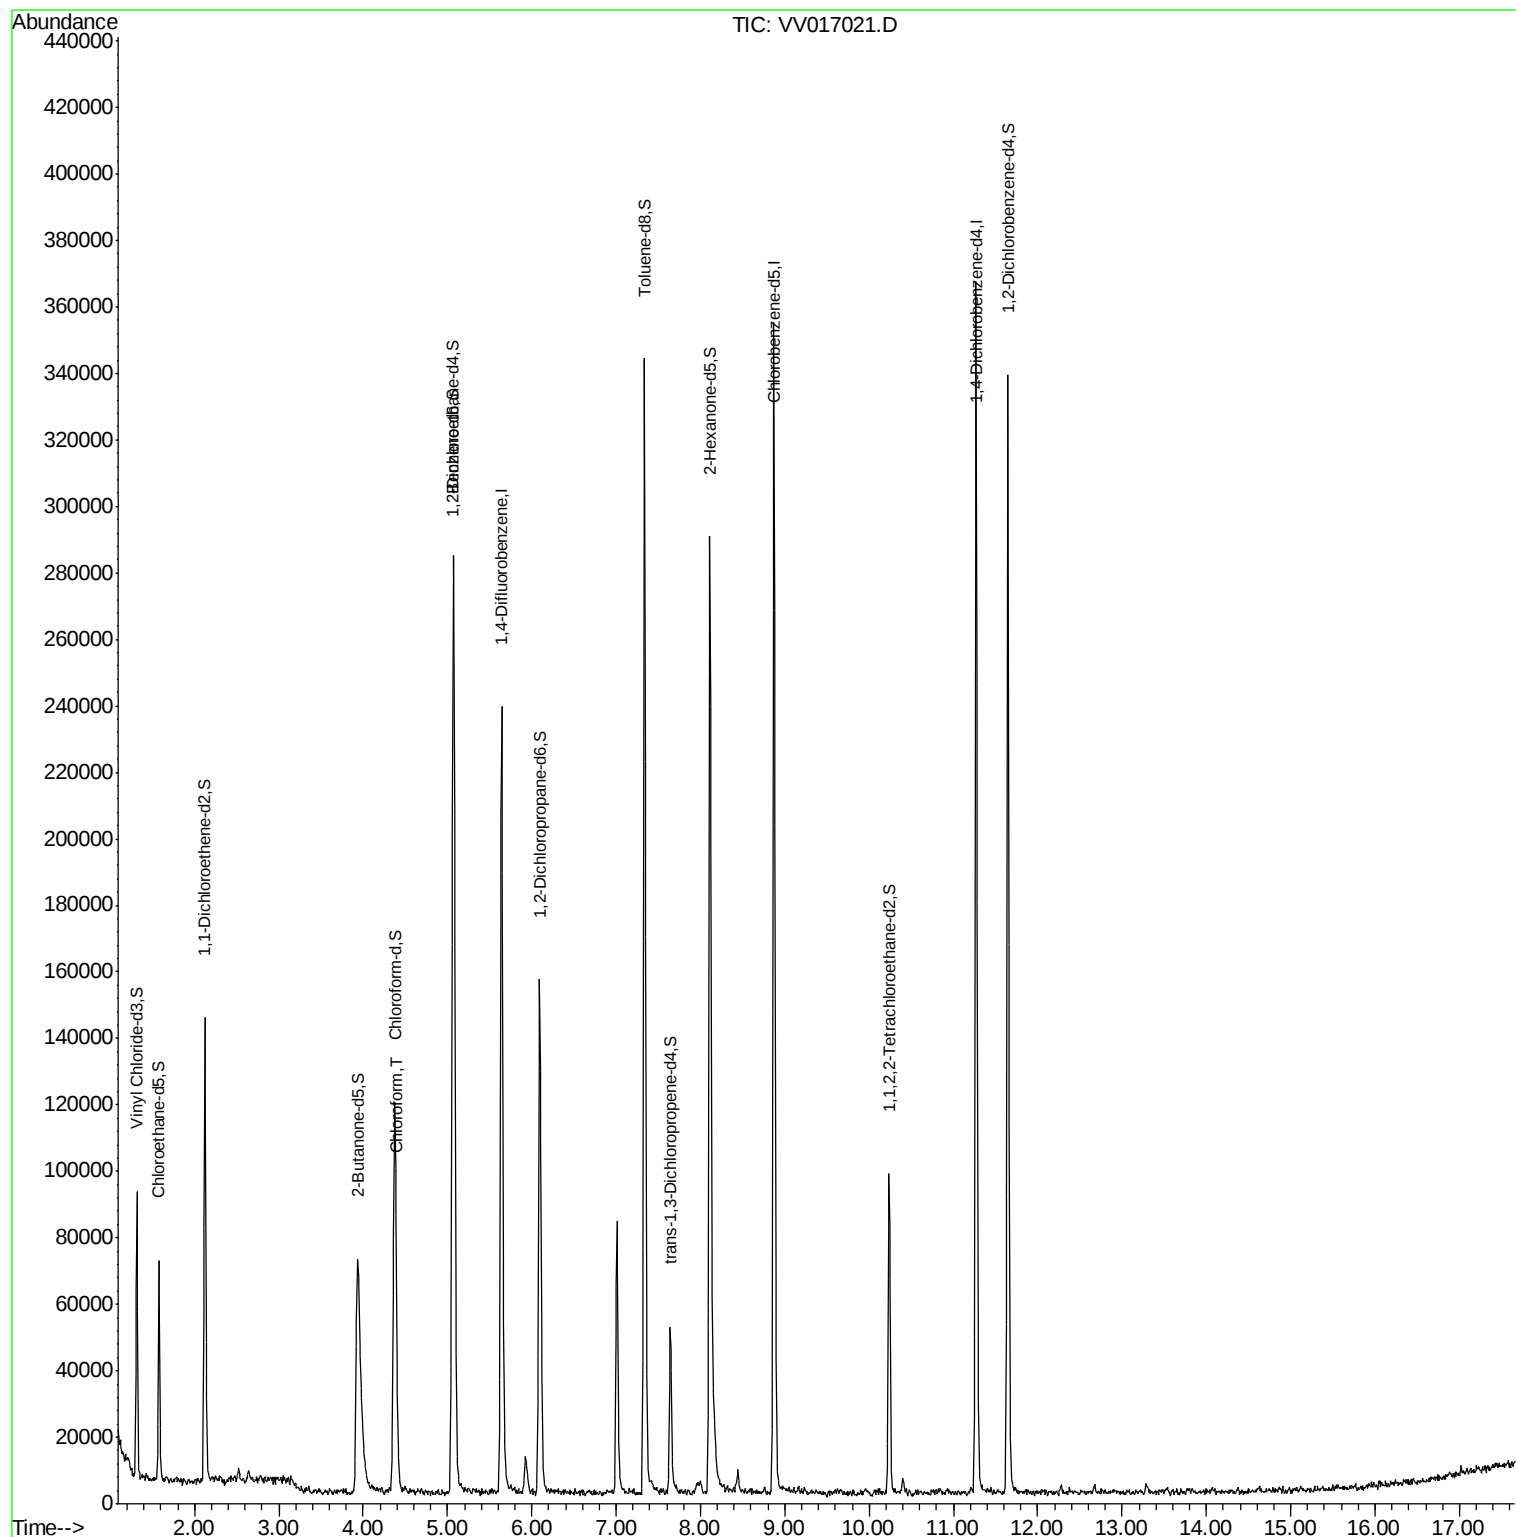

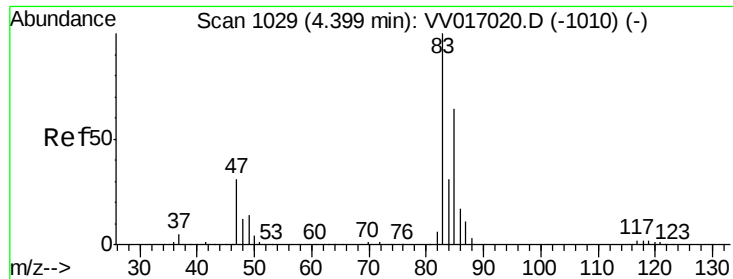

#25
 Chloroform
 Concen: 0.194 ug/L
 RT: 4.40 min Scan# 1029
 Delta R.T. -0.00 min
 Lab File: VV017021.D
 Acq: 22 Jun 2020 16:59

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK50

Tot Ion: 83 Resp: 4716
 Ion Ratio Lower Upper
 83 100
 85 73.0 44.2 82.2

