

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062320\
 Data File : VV017034.D
 Acq On : 22 Jun 2020 22:09
 Operator : SY/MD
 Sample : L3067-15
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXH2

Quant Time: Jun 23 06:30:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 23 04:53:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	184682	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	181009	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	11.27	152	92705	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47059	4.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.80%
7) Chloroethane-d5	1.58	69	37392	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.80%
11) 1,1-Dichloroethene-d2	2.13	63	212590	10.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	201.60%#
20) 2-Butanone-d5	3.92	46	140272	49.65	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.30%
24) Chloroform-d	4.38	84	111067	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
26) 1,2-Dichloroethane-d4	5.06	65	59882	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.07	84	216093	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
36) 1,2-Dichloropropane-d6	6.09	67	63566	4.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.40%
41) Toluene-d8	7.34	98	202852	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
45) trans-1,3-Dichloropropene-	7.65	79	25302	4.32	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.40%
48) 2-Hexanone-d5	8.11	63	96094	43.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.14%
59) 1,1,2,2-Tetrachloroethane-	10.24	84	47113	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
65) 1,2-Dichlorobenzene-d4	11.65	152	81761	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%

Target Compounds

					Ovalue
5) Vinyl chloride	1.32	62	63765	5.262	ug/L 98
8) Chloroethane	1.60	64	71797	10.720	ug/L 94
12) 1,1-Dichloroethene	2.14	96	249514	28.151	ug/L # 68
18) trans-1,2-Dichloroethene	2.78	96	5613	0.598	ug/L 84
19) 1,1-Dichloroethane	3.21	63	5514214	261.291	ug/L 98
22) cis-1,2-Dichloroethene	3.94	96	159521	12.420	ug/L # 100
27) 1,2-Dichloroethane	5.17	62	5465	0.382	ug/L 99
29) 1,1,1-Trichloroethane	4.64	97	12842799	592.212	ug/L 98
33) Benzene	5.13	78	105595	2.228	ug/L 100
34) Trichloroethene	5.95	95	5577	0.402	ug/L 93
42) Toluene	7.41	91	18008	0.327	ug/L 87
47) 1,1,2-Trichloroethane	7.87	97	2699	0.324	ug/L # 85
49) Tetrachloroethene	8.00	164	3762	0.337	ug/L 83
53) Chlorobenzene	8.90	112	40231	1.171	ug/L 95
54) Ethylbenzene	9.04	91	3656	0.062	ug/L 95
55) m,p-xylene	9.16	106	2152	0.093	ug/L 80
56) o-xylene	9.57	106	4720	0.219	ug/L 95

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062320\
Data File : VV017034.D
Acq On : 22 Jun 2020 22:09
Operator : SY/MD
Sample : L3067-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXH2

Quant Time: Jun 23 06:30:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 23 04:53:49 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
58) Isopropylbenzene	9.95	105	24756	0.418	ug/L	96
64) 1,4-Dichlorobenzene	11.29	146	4642	0.164	ug/L	96
66) 1,2-Dichlorobenzene	11.67	146	25445	1.005	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062320\
Data File : VV017034.D
Acq On : 22 Jun 2020 22:09
Operator : SY/MD
Sample : L3067-15
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXH2

Quant Time: Jun 23 06:30:03 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 23 04:53:49 2020
Response via : Initial Calibration

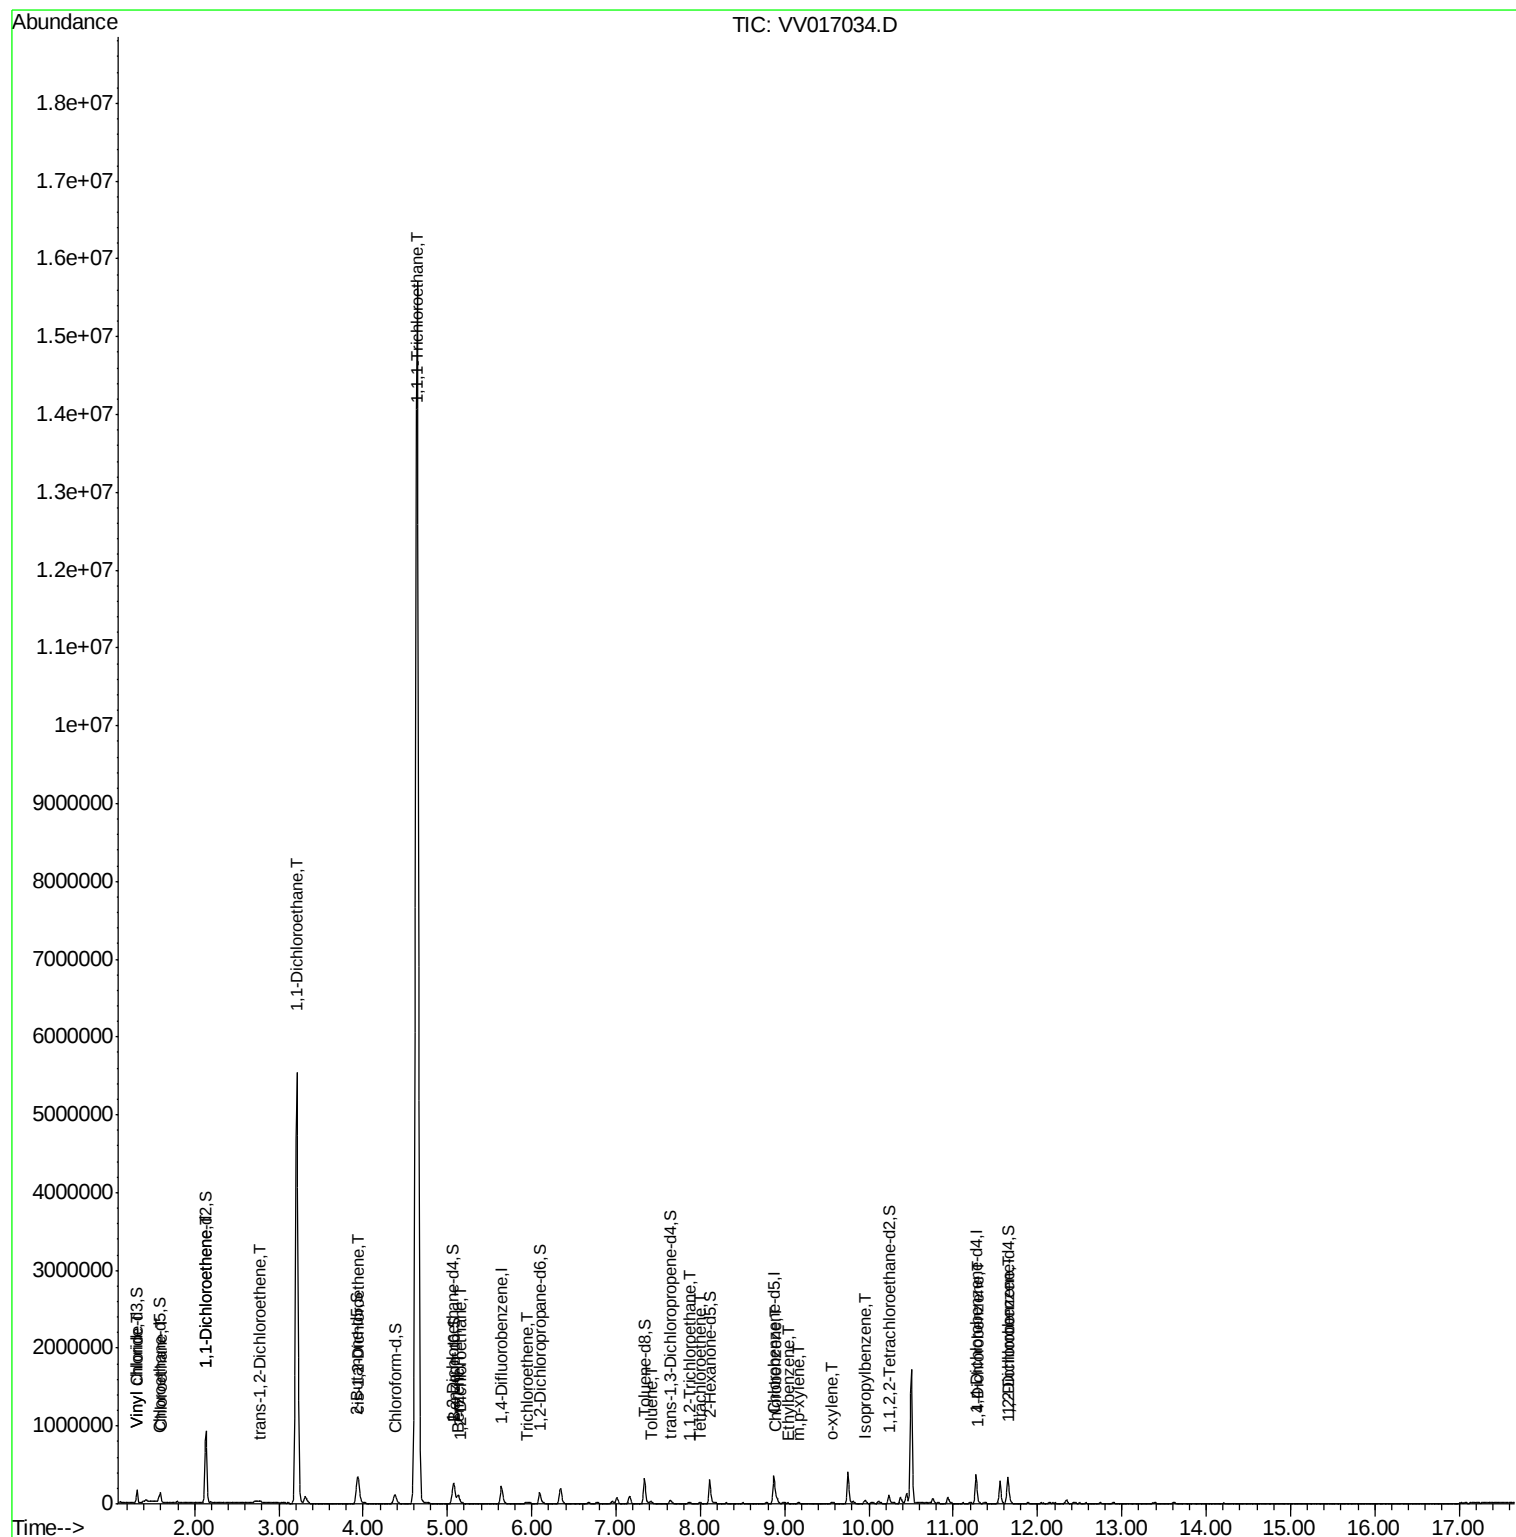



#5

Vinyl chloride

Concen: 5.262 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampled :


BFXH2

Tot Ion: 62 Resp: 63765




Ion Ratio Lower Upper

62 100

64 33.0 22.5 41.7

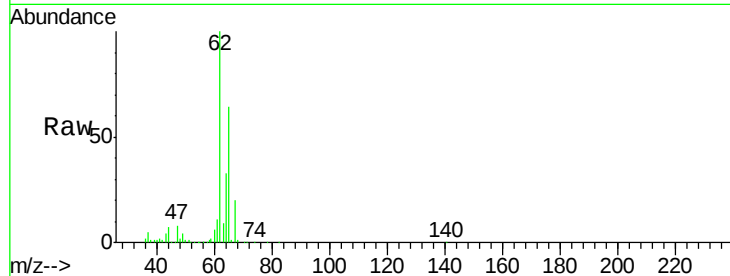

Abundance Ion 62.00 (61.70 to 62.70): VV017034.D (-62) (-)

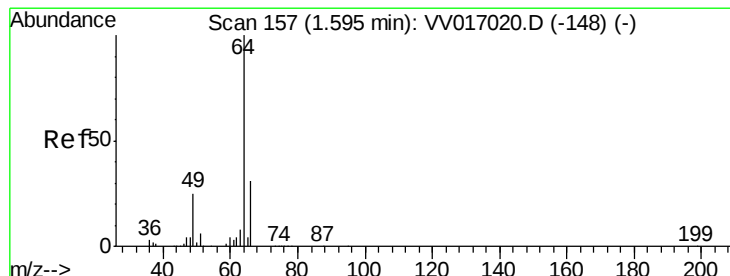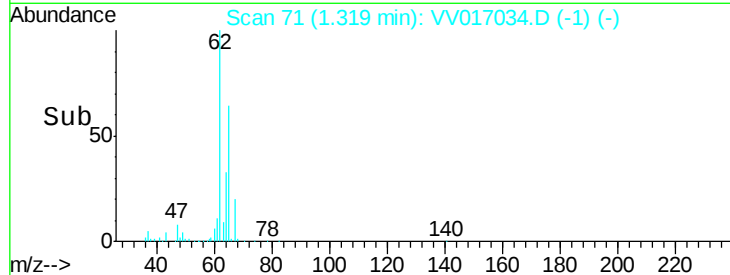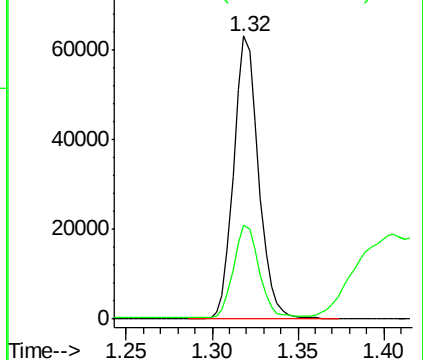

#8

Chloroethane

Concen: 10.720 ug/L

RT: 1.60 min Scan# 157

Delta R.T. -0.00 min

Lab File: VV017034.D


Acq: 22 Jun 2020 22:09

Tgt Ion: 64 Resp: 71797



Ion Ratio Lower Upper


64 100

66 29.3 22.8 42.4

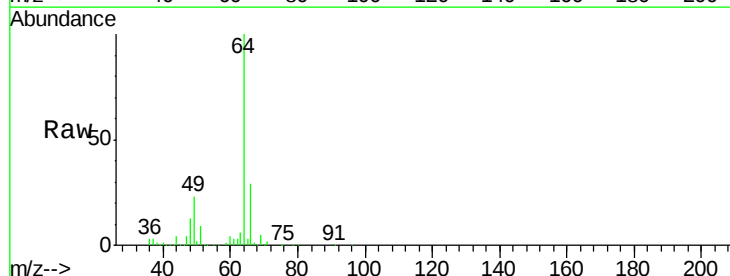

Abundance Ion 64.10 (63.80 to 64.80): VV017034.D (-64) (-)




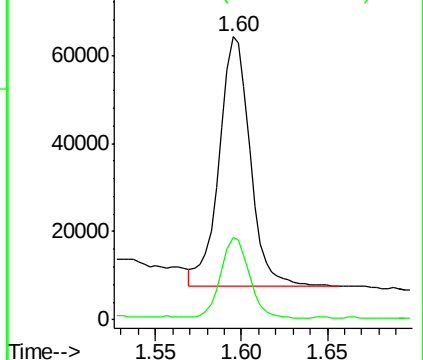




#12
 1,1-Dichloroethene
 Concen: 28.151 ug/L
 RT: 2.14 min Scan# 325
 Delta R.T. 0.00 min
 Lab File: VV017034.D
 Acq: 22 Jun 2020 22:09




Instrument :
 MSVOA_V
 ClientSampleId :
 BFXH2


Tot Ion: 96 Resp: 249514
 Ion Ratio Lower Upper
 96 100
 61 176.1 125.0 232.2
 63 71.1 109.8 203.8#

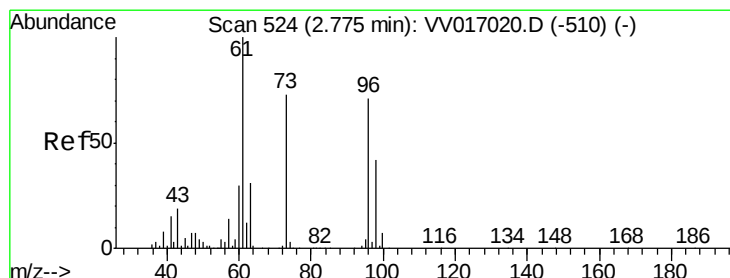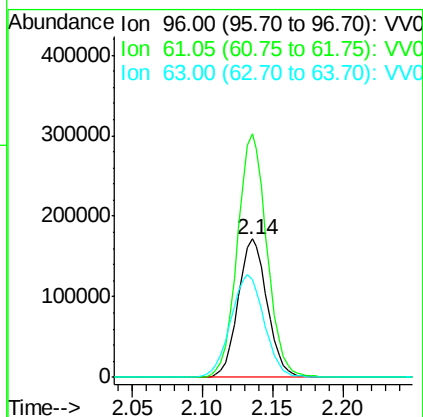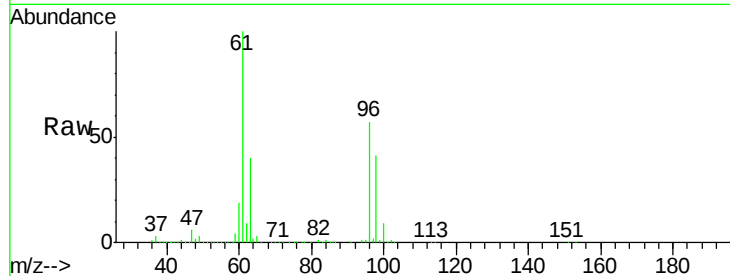

#18
 trans-1,2-Dichloroethene
 Concen: 0.598 ug/L
 RT: 2.78 min Scan# 525
 Delta R.T. 0.00 min
 Lab File: VV017034.D
 Acq: 22 Jun 2020 22:09

Tgt Ion: 96 Resp: 5613
 Ion Ratio Lower Upper
 96 100
 61 119.7 102.3 189.9
 98 67.4 44.7 82.9

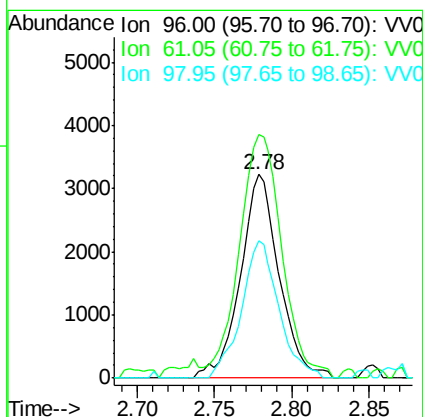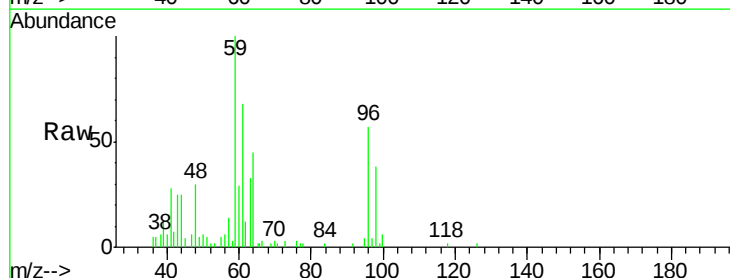

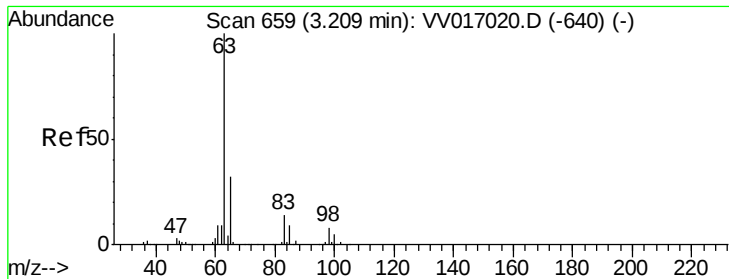

#19

1,1-Dichloroethane

Concen: 261.291 ug/L

RT: 3.21 min Scan# 660

Delta R.T. 0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampleId :

BFXH2


Tot Ion: 63 Resp: 5514214

Ion Ratio Lower Upper

63 100

65 32.6 21.8 40.4




83 14.2 9.7 17.9

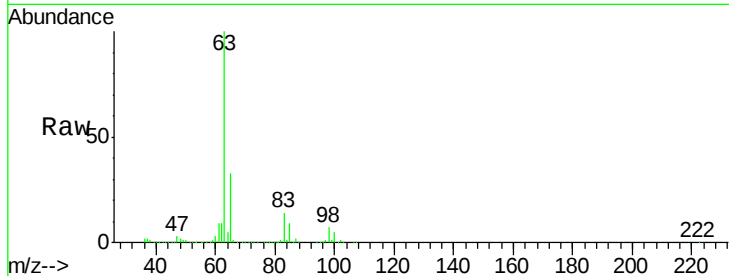

Abundance Ion 63.10 (62.80 to 63.80): VV0

Ion 65.10 (64.80 to 65.80): VV0

Ion 83.05 (82.75 to 83.75): VV0

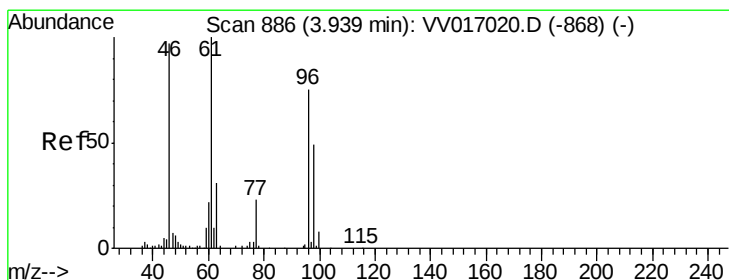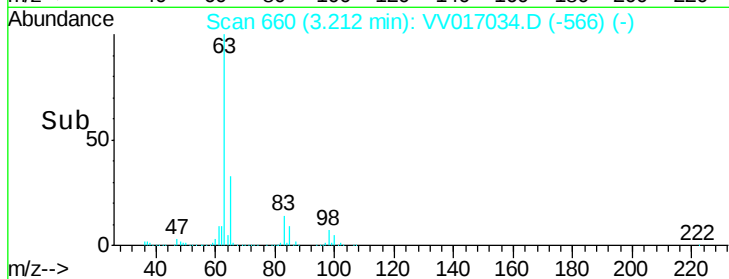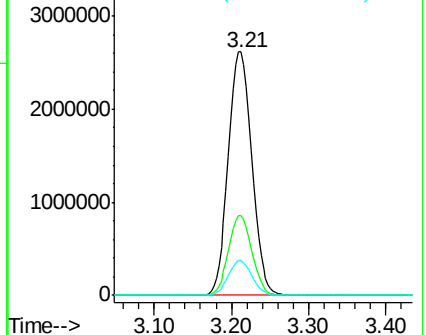

#22

cis-1,2-Dichloroethene

Concen: 12.420 ug/L

RT: 3.94 min Scan# 886

Delta R.T. -0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09


Tgt Ion: 96 Resp: 159521

Ion Ratio Lower Upper

96 100

61 130.3 91.0 169.0



68 0.4 0.0 0.0#

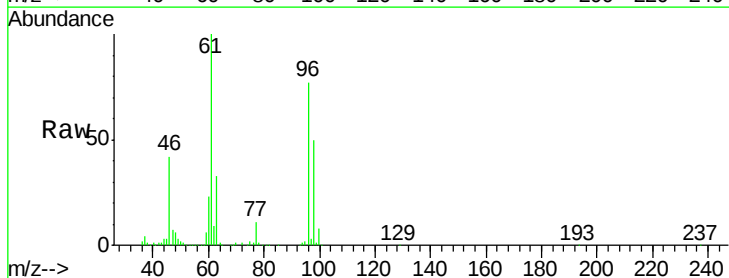


Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 68.15 (67.85 to 68.85): VV0

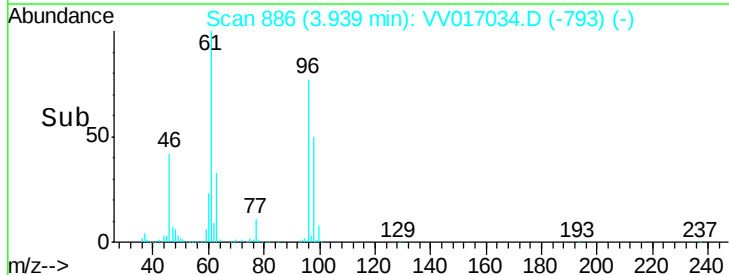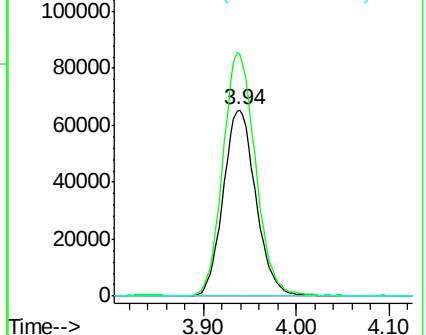



#27

1,2-Dichloroethane

Concen: 0.382 ug/L

RT: 5.17 min Scan# 1268

Delta R.T. 0.01 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampled :


BFXH2

Tot Ion: 62 Resp: 5465

Ion Ratio Lower Upper




62 100

98 8.1 6.7 10.1

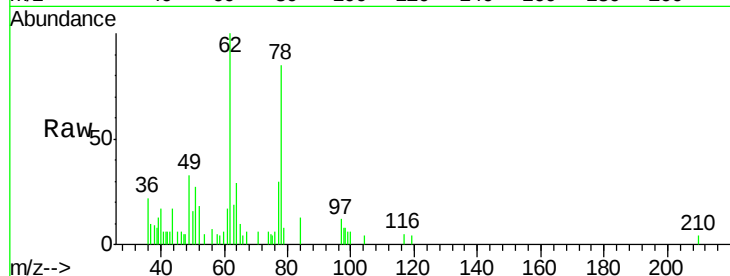

Abundance Ion 62.00 (61.70 to 62.70): VV0

Ion 98.05 (97.75 to 98.75): VV0

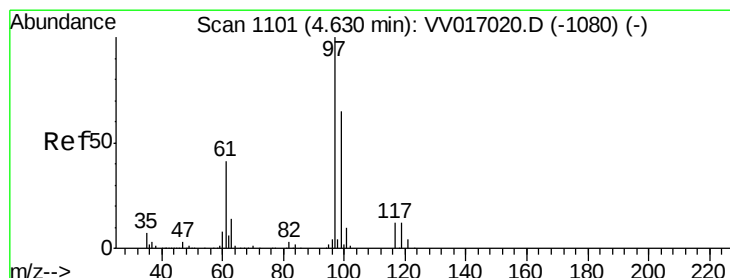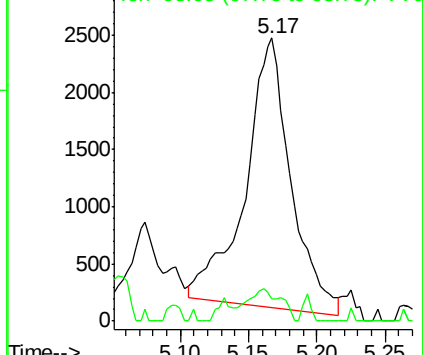

#29

1,1,1-Trichloroethane

Concen: 592.212 ug/L

RT: 4.64 min Scan# 1104

Delta R.T. 0.01 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09


Tgt Ion: 97 Resp:12842799

Ion Ratio Lower Upper

97 100

99 65.6 50.3 75.5



61 44.8 36.0 54.0

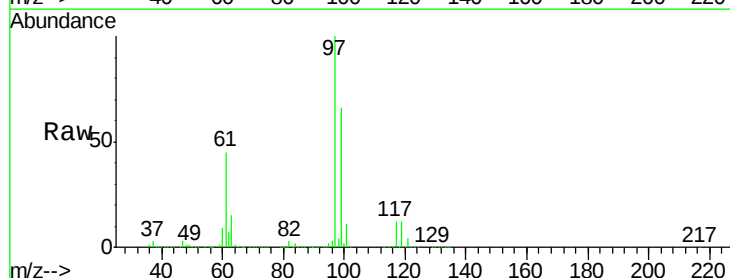


Abundance Ion 96.95 (96.65 to 97.65): VV0

Ion 99.05 (98.75 to 99.75): VV0

Ion 61.05 (60.75 to 61.75): VV0

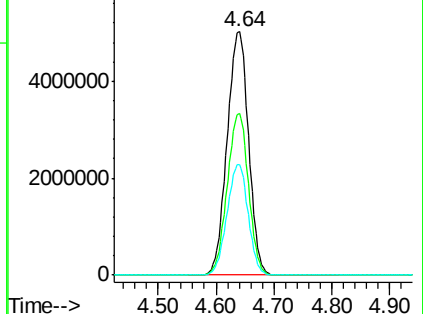

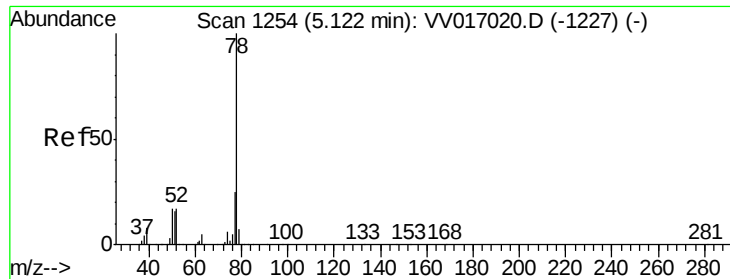

#33

Benzene

Concen: 2.228 ug/L

RT: 5.13 min Scan# 1255

Delta R.T. 0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09


Instrument :

MSVOA_V




ClientSampleId :

BFXH2

Tgt Ion: 78 Resp: 105595

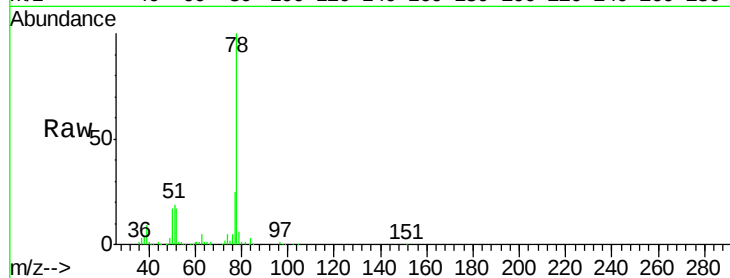

Abundance Ion 78.10 (77.80 to 78.80): VV0

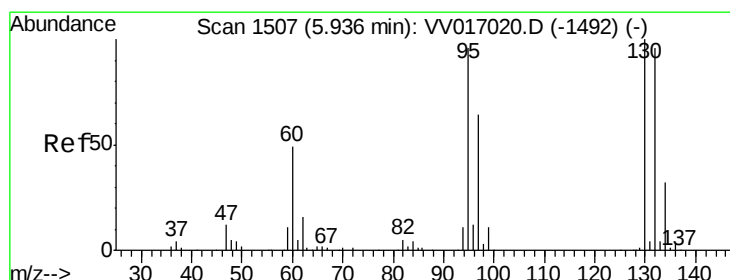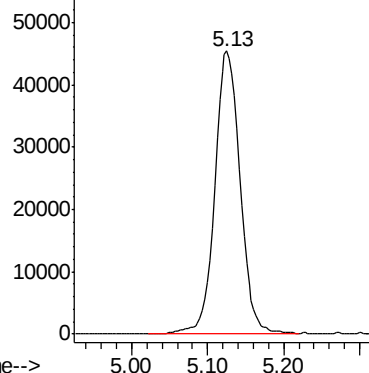

#34

Trichloroethene

Concen: 0.402 ug/L

RT: 5.95 min Scan# 1510

Delta R.T. 0.01 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Tgt Ion: 95 Resp: 5577




Ion	Ratio	Lower	Upper
95	100		
97	60.8	45.3	84.1
132	88.2	68.8	127.8
130	106.7	70.2	130.4


Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 96.95 (96.65 to 97.65): VV0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

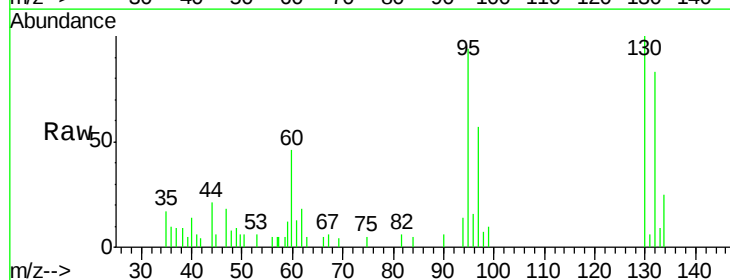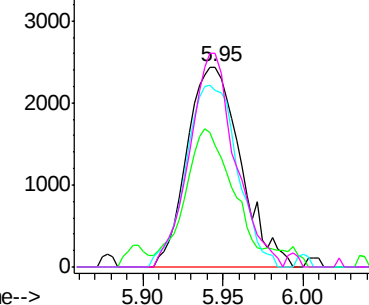

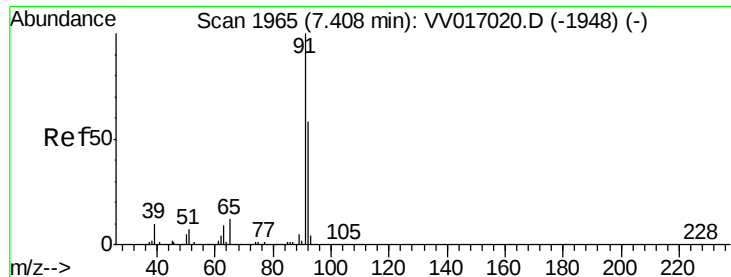

#42

Toluene

Concen: 0.327 ug/L

RT: 7.41 min Scan# 1966

Delta R.T. 0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampled :





BFXH2

Tot Ion: 91 Resp: 18008

Ion Ratio Lower Upper

91 100

92 66.6 39.9 74.1

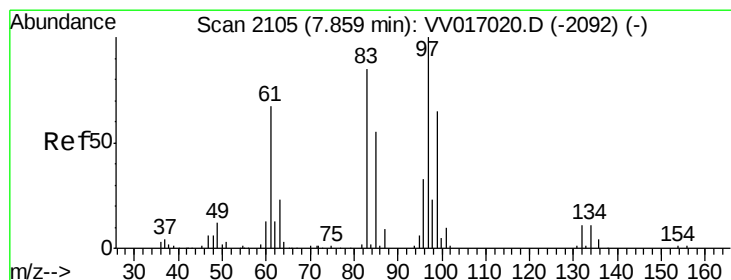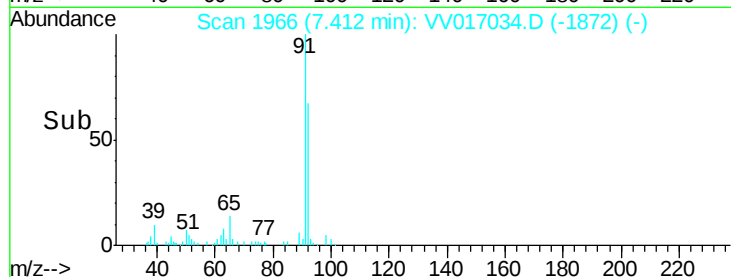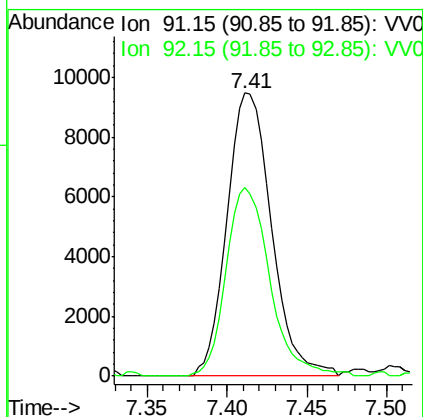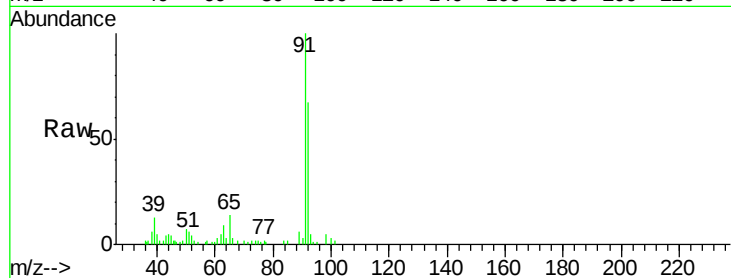

#47

1,1,2-Trichloroethane

Concen: 0.324 ug/L

RT: 7.87 min Scan# 2108

Delta R.T. 0.01 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Tgt Ion: 97 Resp: 2699




Ion Ratio Lower Upper


97 100

99 56.8 43.6 81.0

83 56.8 57.4 106.6#

85 59.8 38.8 72.0

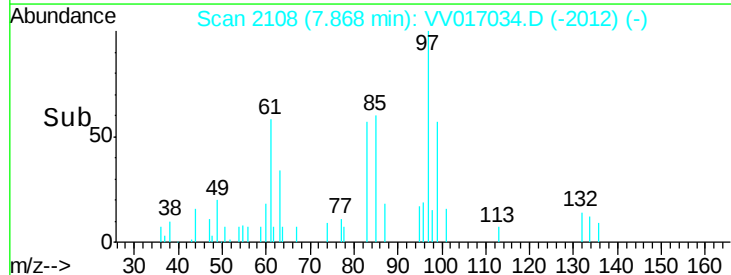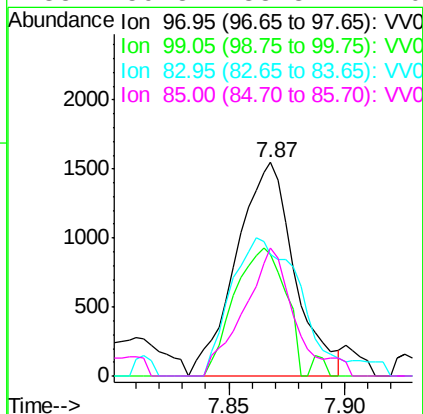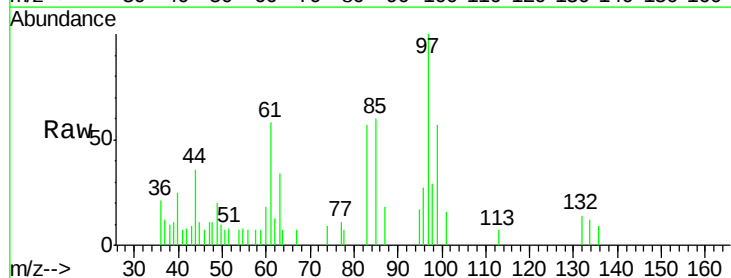

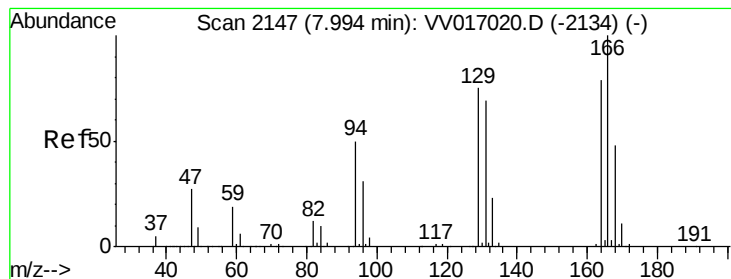

#49

Tetrachloroethene

Concen: 0.337 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. 0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampleId :

BFXH2

Tot Ion:164 Resp: 3762


Ion Ratio Lower Upper

164 100

129 81.7 65.2 121.0

131 84.3 64.1 119.1

166 96.5 90.2 167.4



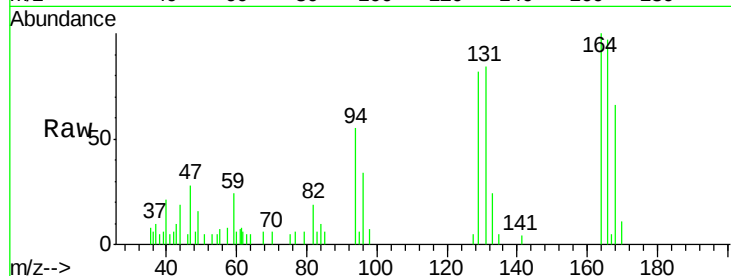


Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

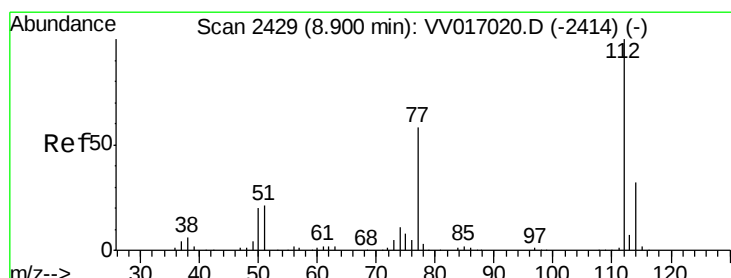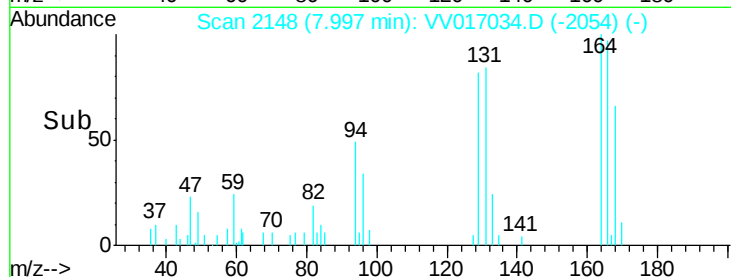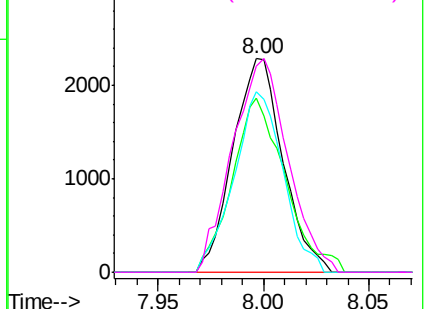

#53

Chlorobenzene

Concen: 1.171 ug/L

RT: 8.90 min Scan# 2430

Delta R.T. 0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09


Tgt Ion:112 Resp: 40231

Ion Ratio Lower Upper

112 100

114 34.6 22.0 41.0



77 61.4 46.0 69.0

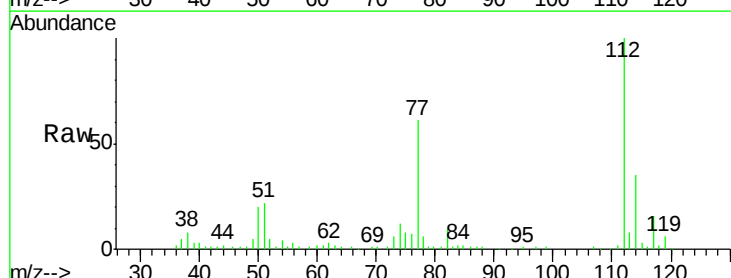


Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VV0

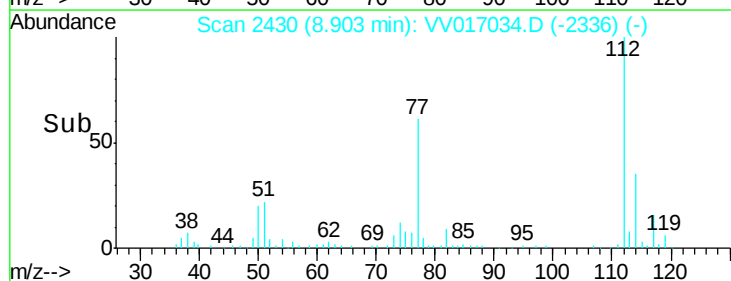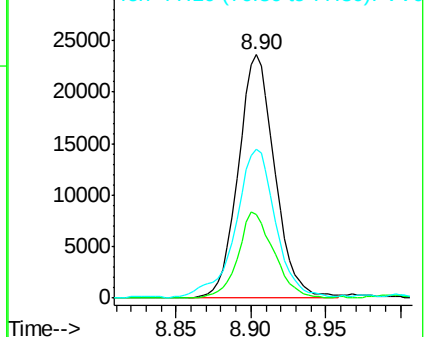

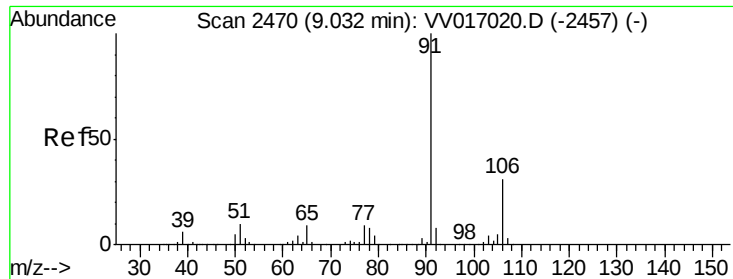

#54

Ethylbenzene

Concen: 0.062 ug/L

RT: 9.04 min Scan# 2473

Delta R.T. 0.01 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampleId :


BFXH2

Tot Ion: 91 Resp: 3656

Ion Ratio Lower Upper




91 100

106 27.2 21.1 39.1

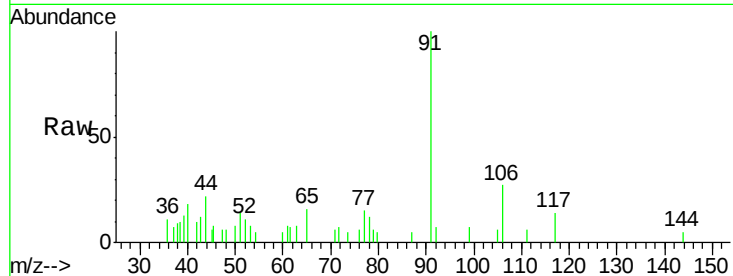

Abundance Ion 91.15 (90.85 to 91.85): VV0

Ion 106.15 (105.85 to 106.85): V

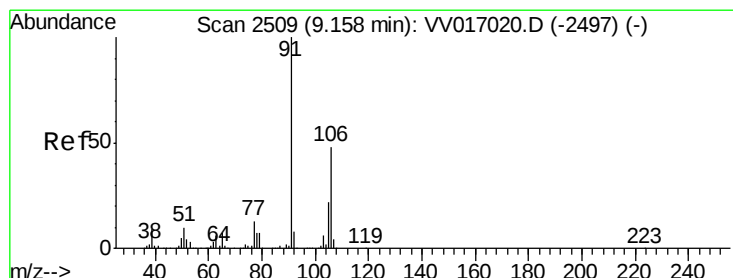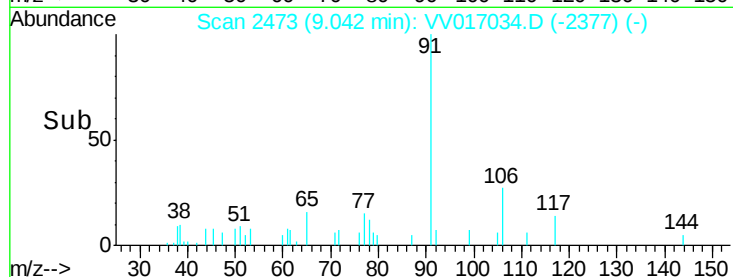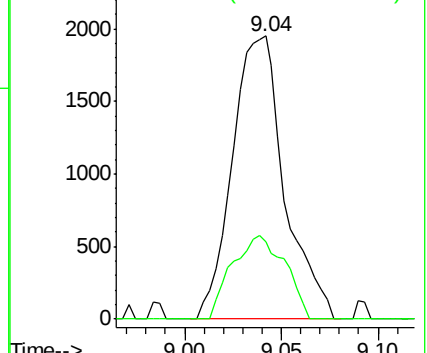

#55

m,p-xylene

Concen: 0.093 ug/L

RT: 9.16 min Scan# 2510

Delta R.T. 0.00 min

Lab File: VV017034.D


Acq: 22 Jun 2020 22:09

Tgt Ion: 106 Resp: 2152

Ion Ratio Lower Upper



106 100


91 173.0 142.7 264.9

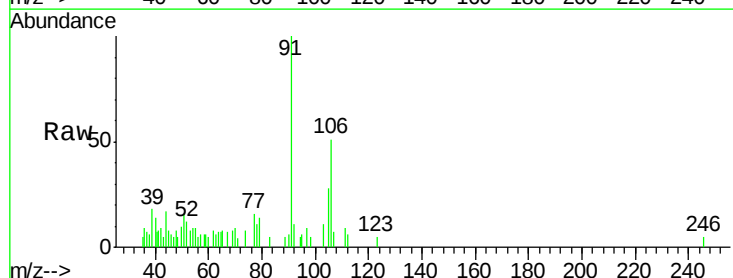

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VV0

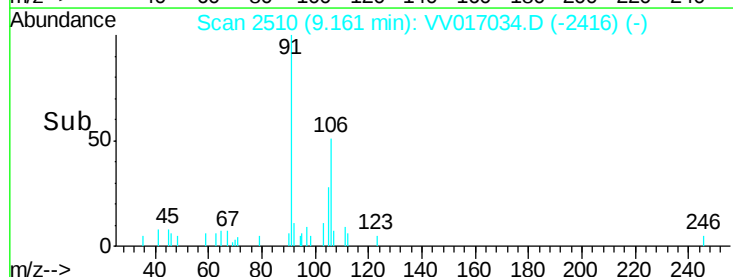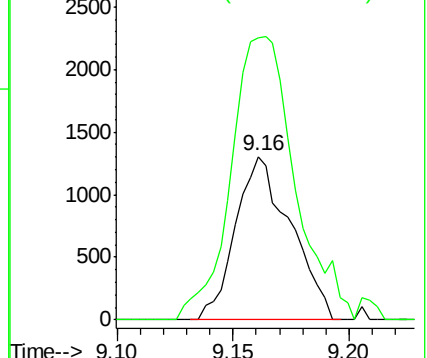


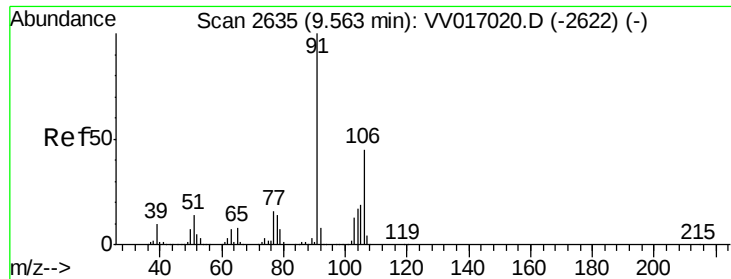




#56
o-xylene
Concen: 0.219 ug/L
RT: 9.57 min Scan# 2637
Delta R.T. 0.01 min
Lab File: VV017034.D
Acq: 22 Jun 2020 22:09

Instrument :
MSVOA_V
ClientSampleId :
BFXH2

Tot Ion:106 Resp: 4720
Ion Ratio Lower Upper
106 100
91 227.5 153.6 285.2

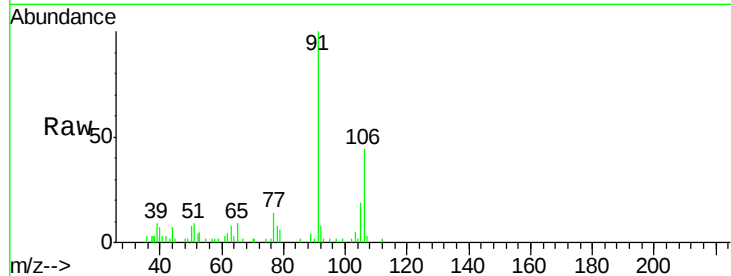


Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VV0

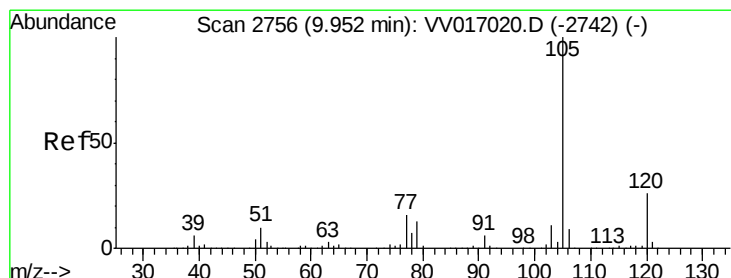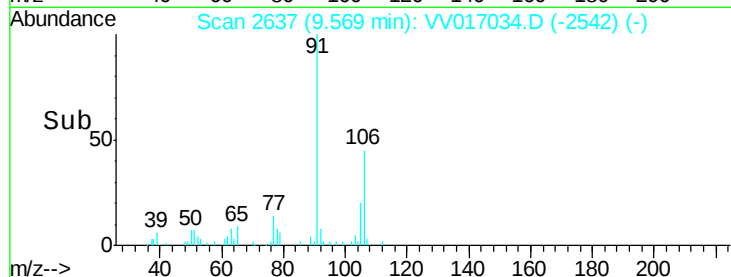
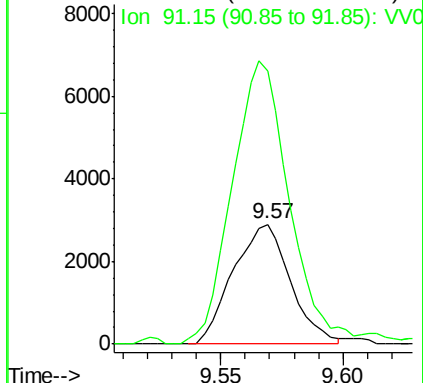



#58
Isopropylbenzene
Concen: 0.418 ug/L
RT: 9.95 min Scan# 2757
Delta R.T. 0.00 min
Lab File: VV017034.D
Acq: 22 Jun 2020 22:09

Tgt Ion:105 Resp: 24756
Ion Ratio Lower Upper
105 100
120 25.0 21.2 31.8
77 18.3 13.0 19.4

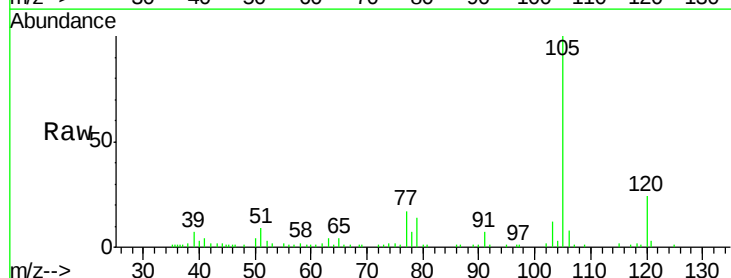

Abundance Ion 105.05 (104.75 to 105.75): V
Ion 120.10 (119.80 to 120.80): V
Ion 77.10 (76.80 to 77.80): VV0

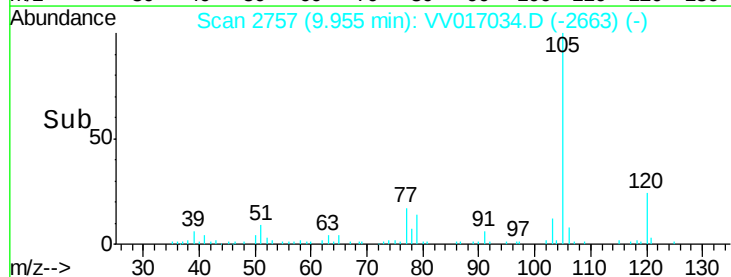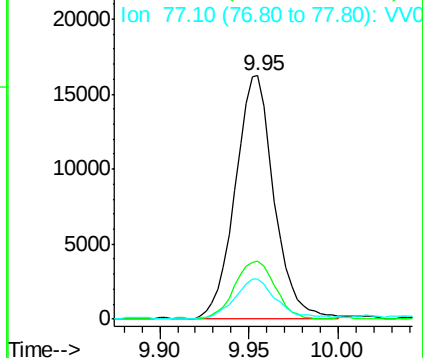

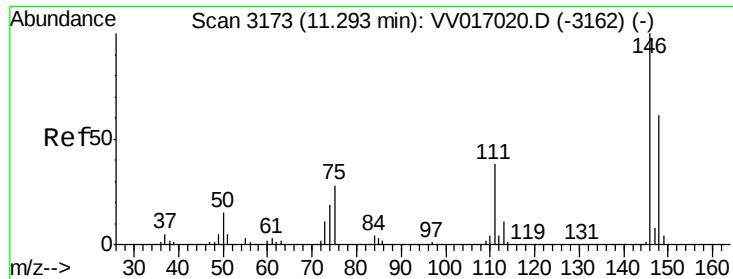

#64

1,4-Dichlorobenzene

Concen: 0.164 ug/L

RT: 11.29 min Scan# 3173

Delta R.T. -0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09

Instrument :

MSVOA_V

ClientSampled :

BFXH2


Tot Ion:146 Resp: 4642

Ion Ratio Lower Upper

146 100

111 37.6 27.4 50.8




148 59.6 44.3 82.3

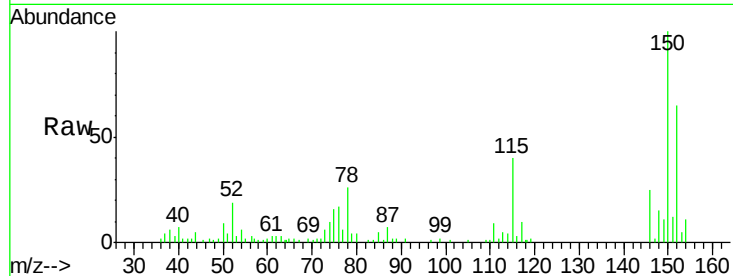

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

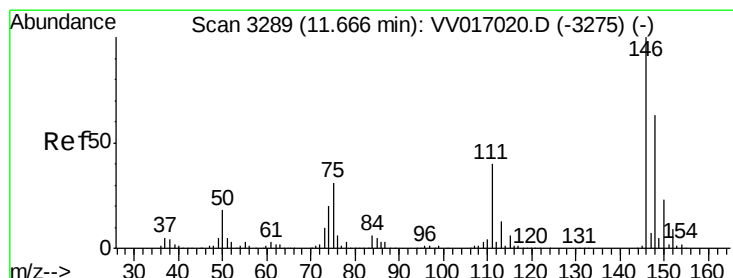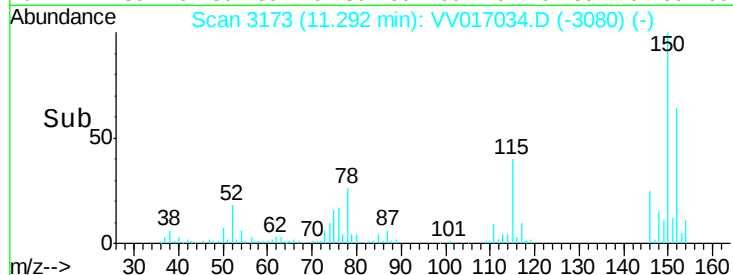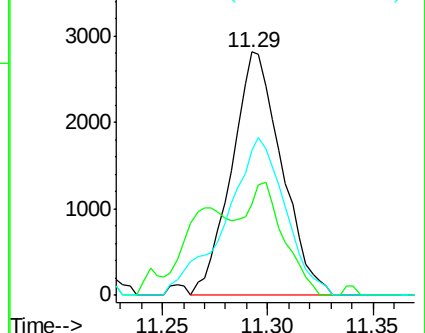

#66

1,2-Dichlorobenzene

Concen: 1.005 ug/L

RT: 11.67 min Scan# 3289

Delta R.T. -0.00 min

Lab File: VV017034.D

Acq: 22 Jun 2020 22:09


Tgt Ion:146 Resp: 25445

Ion Ratio Lower Upper

146 100

111 47.9 34.4 51.6

148 65.6 49.9 74.9

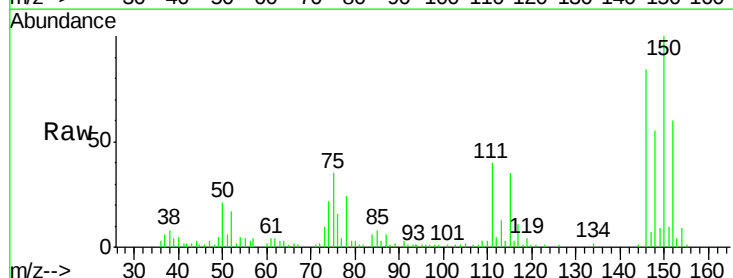

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

