

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV062320\
 Data File : VV017058.D
 Acq On : 23 Jun 2020 16:10
 Operator : SY/MD
 Sample : L3067-19DL2 1000X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXH6DL2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	61	70	83	rVB	73631	76414	13.08%	1.365%
2	1.579	144	152	162	rVB	61716	68369	11.70%	1.221%
3	2.122	311	321	333	rBV	127004	194300	33.26%	3.471%
4	2.521	439	445	463	rVB8	6489	13149	2.25%	0.235%
5	3.212	643	660	679	rVB2	41422	94683	16.21%	1.691%
6	3.936	867	885	919	rBV2	62168	262503	44.94%	4.689%
7	4.380	1006	1023	1044	rBV2	99797	260889	44.66%	4.660%
8	4.634	1083	1102	1122	rBV	174862	442365	75.73%	7.902%
9	5.074	1223	1239	1262	rBV2	239487	584123	100.00%	10.434%
10	5.640	1402	1415	1436	rBV	210602	431557	73.88%	7.709%
11	5.936	1495	1507	1514	rBV	6190	11618	1.99%	0.208%
12	6.096	1543	1557	1576	rBV	139485	284083	48.63%	5.074%
13	7.010	1830	1841	1857	rBV	69041	128207	21.95%	2.290%
14	7.338	1929	1943	1963	rBV	293060	505197	86.49%	9.024%
15	7.643	2027	2038	2054	rBV	42961	75588	12.94%	1.350%
16	8.112	2173	2184	2213	rBV2	253808	500445	85.67%	8.939%
17	8.440	2277	2286	2296	rBV2	10199	18695	3.20%	0.334%
18	8.871	2408	2420	2443	rBV	309967	521946	89.36%	9.323%
19	10.238	2833	2845	2861	rBV	90985	147346	25.23%	2.632%
20	11.270	3152	3166	3188	rBV	323875	508768	87.10%	9.088%
21	11.646	3270	3283	3301	rBV	290540	468010	80.12%	8.360%


Sum of corrected areas: 5598255

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV062320\
Data File : VV017058.D
Acq On : 23 Jun 2020 16:10
Operator : SY/MD
Sample : L3067-19DL2 1000X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXH6DL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

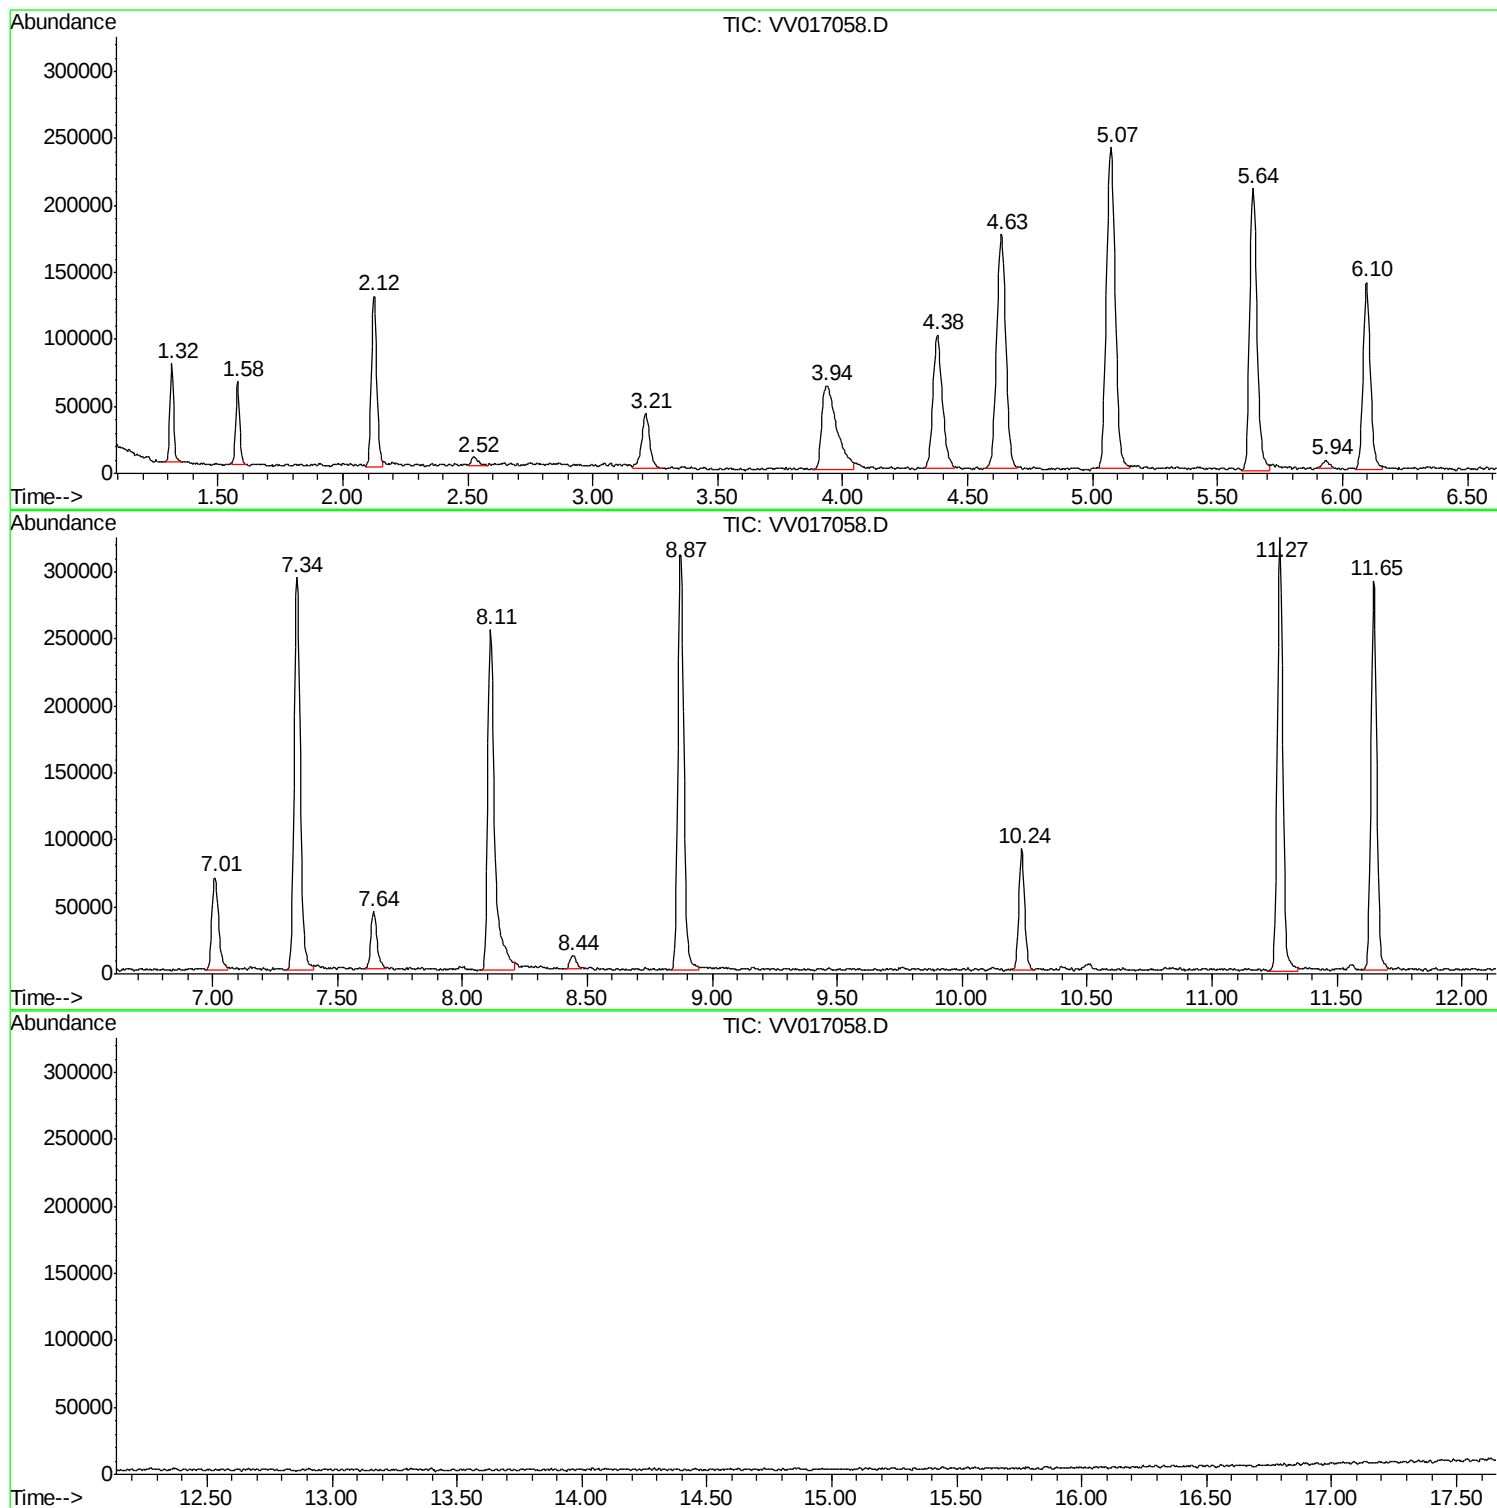

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062320\
Data File : VV017058.D
Acq On : 23 Jun 2020 16:10
Operator : SY/MD
Sample : L3067-19DL2 1000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXH6DL2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV062320\
Data File : VV017058.D
Acq On : 23 Jun 2020 16:10
Operator : SY/MD
Sample : L3067-19DL2 1000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXH6DL2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc