


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062320\
 Data File : VV017019.D
 Acq On : 22 Jun 2020 14:20
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 23 04:53:49 2020

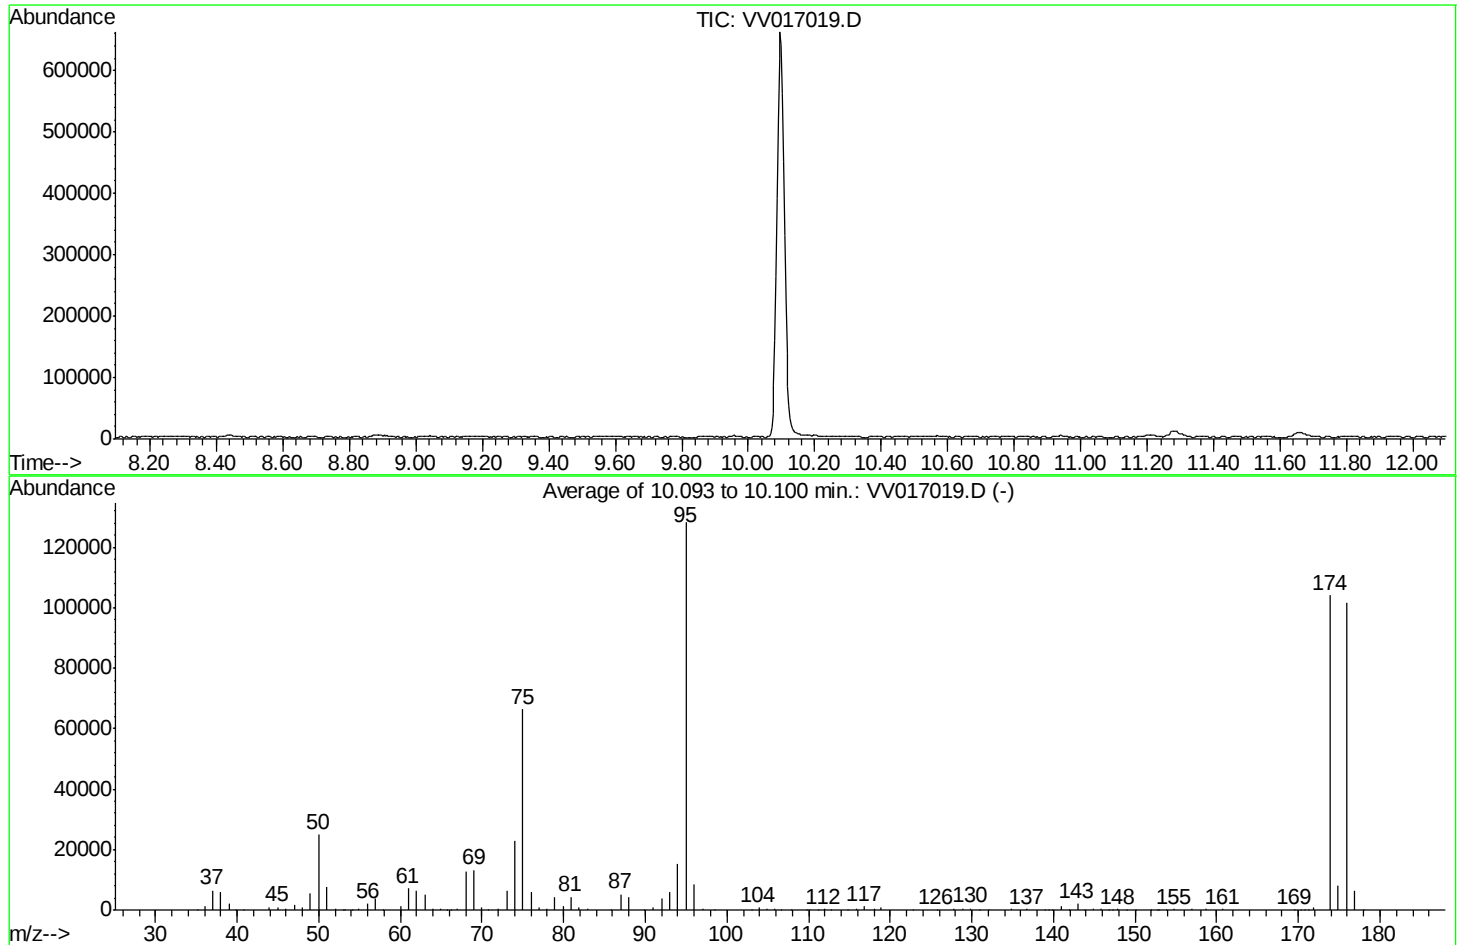

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	24864	PASS
75	95	30	80	51.8	66426	PASS
95	95	100	100	100.0	128250	PASS
96	95	5	9	6.6	8477	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.2	104165	PASS
175	174	5	9	7.8	8087	PASS
176	174	95	101	97.8	101848	PASS
177	176	5	9	6.4	6558	PASS

m/z	Abundance
35.10	142.0
36.00	1395.0
37.00	6393.0
38.00	5908.0
39.10	2153.0
40.00	380.0
40.90	194.0
42.90	136.0
43.90	1093.0
45.00	1023.0
45.90	334.0
47.00	1424.0
48.00	845.0
49.00	5477.0
50.00	24456.0
51.00	7545.0
52.00	539.0
52.90	126.0
53.20	145.0
54.10	109.0
54.90	513.0
56.00	2070.0
57.00	3983.0
57.80	159.0
60.00	1211.0
61.00	7080.0
62.00	6132.0
63.00	4799.0
64.00	568.0
64.90	639.0
66.30	195.0
67.00	544.0
68.00	12735.0
69.00	13196.0
70.00	1079.0
72.00	665.0
73.00	5959.0
74.00	22304.0
75.00	65360.0
76.00	6048.0
77.00	725.0
78.00	590.0
78.90	4050.0
79.90	1346.0
80.90	4293.0
81.90	1106.0
83.00	239.0
85.70	119.0
87.00	5076.0
87.90	4076.0
89.80	118.0
90.90	815.0
92.00	3842.0
93.00	5919.0
94.00	14961.0
95.00	123872.0
96.00	8509.0
97.00	245.0
103.90	693.0
105.00	268.0
106.00	488.0
106.70	174.0
107.80	129.0
109.80	126.0
111.10	129.0
111.90	229.0
112.80	198.0
114.80	188.0
115.90	536.0
116.80	928.0
118.00	577.0
118.80	697.0
122.70	118.0
127.80	585.0
128.90	240.0
129.90	655.0
131.00	219.0
134.90	285.0
136.80	306.0
138.90	110.0
140.90	1496.0
142.00	194.0
142.90	1820.0
143.80	116.0
144.80	375.0
145.80	265.0
147.20	101.0
147.80	361.0
149.00	103.0
150.00	215.0
151.90	116.0
152.70	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

153.80	119.0
154.80	371.0
157.00	290.0
158.80	234.0
160.70	231.0
169.50	103.0
170.20	129.0
171.90	992.0
173.90	98440.0
174.90	7702.0
175.90	95992.0
176.90	6114.0
178.00	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
35.20	148.0
36.00	1375.0
37.00	6799.0
38.00	6360.0
39.10	2151.0
40.00	398.0
40.90	184.0
42.80	126.0
43.90	1150.0
45.00	1053.0
45.90	334.0
47.00	1647.0
48.00	981.0
49.00	5660.0
50.00	25640.0
51.00	7969.0
52.00	561.0
53.20	152.0
54.10	119.0
54.90	511.0
56.00	2129.0
57.00	4094.0
57.90	173.0
60.00	1392.0
61.00	7281.0
62.00	6436.0
63.00	5055.0
64.10	618.0
65.00	612.0
66.30	186.0
67.00	570.0
68.00	13192.0
69.00	13816.0
70.00	1085.0
71.90	640.0
73.00	6342.0
74.00	23544.0
75.00	68712.0
76.00	6125.0
77.00	888.0
77.90	555.0
78.90	4298.0
79.90	1399.0
80.90	4404.0
81.90	1080.0
83.00	277.0
85.80	176.0
87.00	5339.0
88.00	4568.0
90.90	860.0
92.00	4175.0
93.00	6243.0
94.00	16068.0
95.00	132736.0
96.00	8623.0
97.00	232.0
103.90	706.0
104.90	264.0
105.90	553.0
106.60	207.0
107.80	137.0
109.70	112.0
111.20	175.0
111.90	281.0
112.80	236.0
114.70	193.0
115.90	539.0
116.80	1124.0
118.00	602.0
118.80	692.0
122.70	113.0
125.70	119.0
127.80	598.0
128.90	281.0
129.90	616.0
131.00	217.0
132.10	157.0
134.80	265.0
136.80	366.0
140.90	1556.0
141.90	184.0
142.90	2064.0
143.90	127.0
144.80	337.0
145.90	333.0
146.70	102.0
147.90	371.0
150.00	224.0
152.70	115.0
153.80	126.0
154.80	383.0
157.00	270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

158.80	242.0
160.80	244.0
169.60	117.0
171.20	244.0
171.90	1047.0
173.90	107952.0
174.90	8222.0
175.90	105536.0
176.90	6865.0
178.00	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
35.20	159.0
36.00	1121.0
37.00	6271.0
38.00	6306.0
39.00	2129.0
39.90	468.0
41.10	140.0
42.80	155.0
43.90	1127.0
45.00	1052.0
46.00	344.0
47.00	1648.0
48.00	1024.0
49.00	5311.0
50.00	24496.0
51.00	7740.0
52.00	490.0
53.00	161.0
54.10	108.0
54.90	434.0
56.00	1986.0
57.00	3715.0
58.00	181.0
60.00	1322.0
61.00	6838.0
62.00	6101.0
63.00	4810.0
64.00	578.0
65.00	560.0
65.70	168.0
66.20	153.0
67.00	487.0
68.00	12519.0
69.00	12825.0
70.00	947.0
70.70	118.0
72.00	621.0
73.00	6316.0
74.00	22576.0
75.00	65208.0
76.00	5671.0
77.00	888.0
77.90	462.0
78.90	4296.0
79.90	1306.0
80.90	4153.0
81.90	1016.0
83.00	270.0
85.80	268.0
87.00	4856.0
88.00	4671.0
90.90	718.0
92.00	3979.0
93.00	5923.0
94.00	15590.0
95.00	128144.0
96.00	8301.0
97.10	247.0
98.40	102.0
103.00	101.0
103.90	650.0
104.80	230.0
105.80	562.0
106.60	192.0
110.10	114.0
111.20	152.0
111.90	287.0
112.80	206.0
114.80	169.0
115.80	493.0
116.90	1231.0
118.00	557.0
118.80	671.0
125.70	135.0
127.80	564.0
128.80	301.0
129.90	576.0
131.00	185.0
132.10	153.0
134.70	265.0
136.80	357.0
139.40	128.0
139.90	133.0
140.90	1399.0
141.90	171.0
143.00	2075.0
143.90	139.0
144.90	271.0
145.90	325.0
146.70	105.0
148.00	389.0
150.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

152.00	113.0
152.90	107.0
153.80	100.0
154.80	349.0
156.90	218.0
158.70	241.0
160.80	238.0
170.80	229.0
171.20	223.0
171.90	1011.0
173.90	106104.0
174.90	8339.0
175.90	104016.0
176.90	6695.0
178.00	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.70	102.0
37.30	142.0
38.10	137.0
39.00	141.0
39.90	327.0
40.70	123.0
41.30	113.0
42.20	212.0
42.80	147.0
44.00	391.0
45.00	138.0
45.60	111.0
48.20	113.0
50.90	110.0
51.60	160.0
56.90	126.0
63.80	148.0
69.30	107.0
93.90	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40