


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV062320\
 Data File : VV017043.D
 Acq On : 23 Jun 2020 09:19
 Operator : SY/MD
 Sample : BFB41
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Jun 24 05:01:54 2020

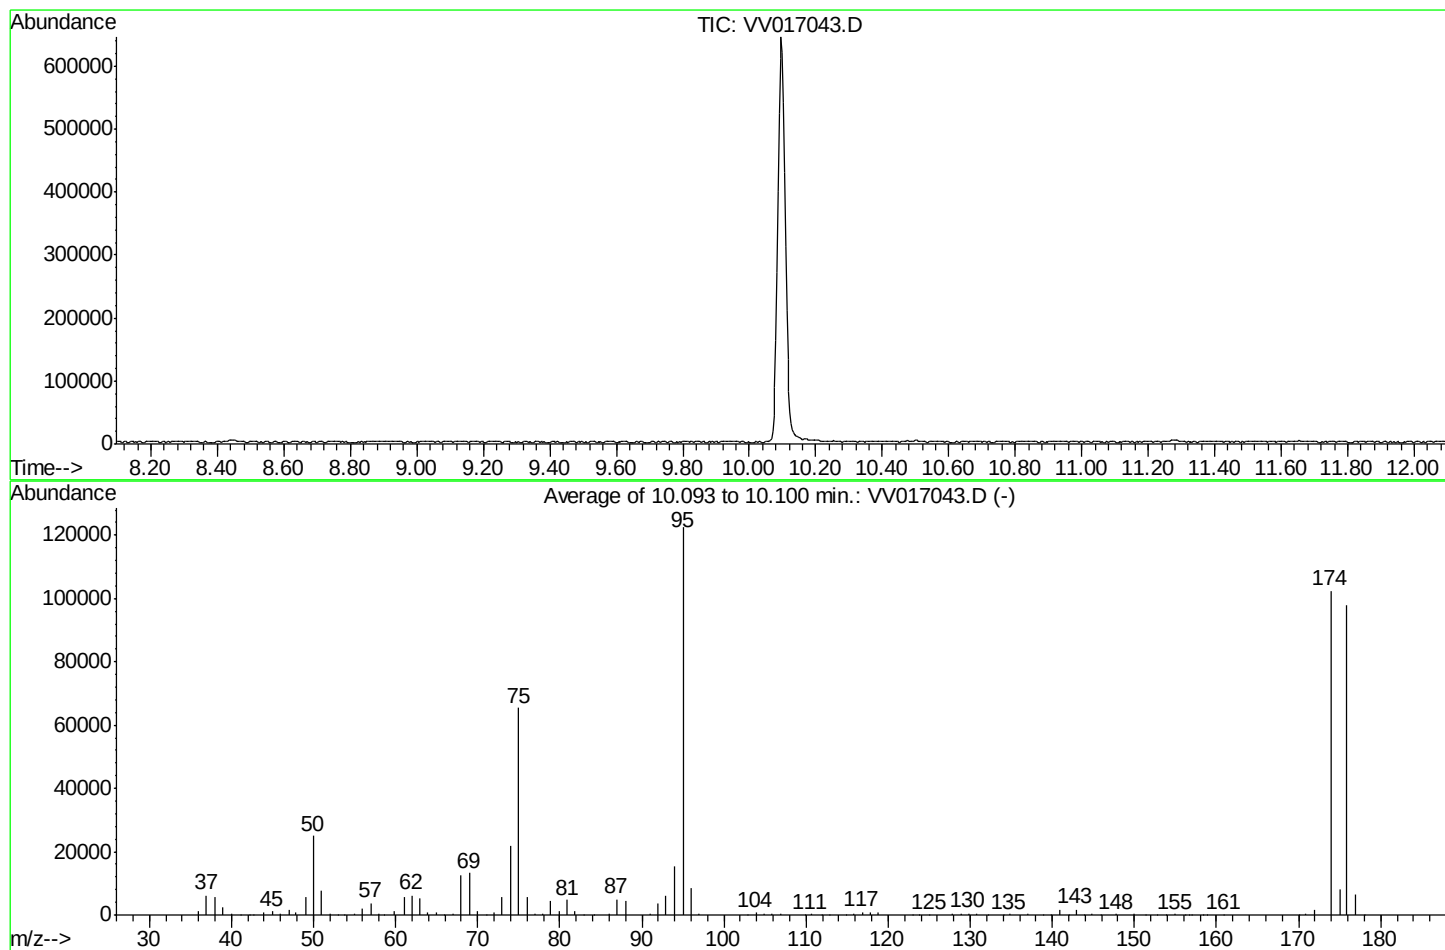

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	24936	PASS
75	95	30	80	53.4	65389	PASS
95	95	100	100	100.0	122506	PASS
96	95	5	9	6.9	8413	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.5	102346	PASS
175	174	5	9	8.0	8140	PASS
176	174	95	101	95.5	97762	PASS
177	176	5	9	6.7	6589	PASS

m/z	Abundance
36.00	1435.0
37.00	6450.0
38.00	5667.0
39.00	2511.0
40.00	592.0
41.10	149.0
42.20	187.0
42.90	144.0
44.00	1385.0
45.00	1247.0
46.00	278.0
47.00	1720.0
47.90	821.0
49.00	5743.0
50.00	24856.0
51.00	7491.0
52.00	459.0
52.90	218.0
53.80	155.0
54.90	445.0
56.00	1993.0
57.00	3530.0
57.90	265.0
58.60	110.0
59.90	1297.0
61.00	5856.0
62.00	6105.0
63.00	5286.0
63.90	722.0
65.00	973.0
65.90	137.0
67.00	481.0
68.00	12413.0
69.00	13689.0
70.00	1098.0
71.90	760.0
73.00	5347.0
74.00	21240.0
75.00	64504.0
76.00	5824.0
77.00	648.0
77.90	444.0
78.90	4186.0
79.90	1379.0
80.90	4711.0
81.90	1019.0
82.80	140.0
86.00	320.0
86.90	4942.0
88.00	4534.0
91.00	512.0
92.00	3482.0
93.00	5944.0
94.00	14876.0
95.00	119576.0
96.00	8764.0
97.00	328.0
102.90	155.0
103.90	720.0
104.90	227.0
105.90	664.0
106.90	189.0
109.90	204.0
110.60	248.0
111.80	125.0
112.90	175.0
114.80	126.0
115.80	605.0
116.90	933.0
117.90	610.0
118.80	737.0
123.70	146.0
125.10	107.0
127.90	382.0
128.90	297.0
129.80	586.0
130.80	187.0
134.80	390.0
137.00	267.0
138.90	104.0
139.80	130.0
140.90	1770.0
142.00	190.0
142.90	1757.0
144.80	494.0
146.00	130.0
147.70	293.0
150.00	225.0
152.70	148.0
153.80	157.0
154.90	348.0
156.70	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

158.30	110.0
158.90	177.0
160.80	210.0
170.00	148.0
170.80	317.0
171.90	1577.0
173.90	98152.0
175.00	7946.0
175.90	93128.0
176.90	6368.0
178.00	249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	1436.0
37.00	6499.0
38.00	5770.0
39.00	2476.0
40.00	555.0
41.20	153.0
42.20	171.0
42.90	123.0
44.00	1413.0
44.90	1205.0
46.00	230.0
47.00	1627.0
47.90	819.0
49.00	5853.0
50.00	25752.0
51.00	7815.0
52.10	447.0
52.90	217.0
54.90	401.0
56.00	2034.0
57.00	3811.0
57.90	297.0
59.90	1325.0
61.00	6030.0
62.00	6346.0
63.00	5581.0
63.90	672.0
65.00	941.0
65.90	150.0
67.00	514.0
68.00	13000.0
69.00	13564.0
70.00	1120.0
71.10	104.0
72.00	869.0
73.00	5883.0
74.00	22544.0
75.00	67424.0
76.00	6006.0
77.00	737.0
77.80	542.0
78.90	4508.0
79.90	1396.0
80.90	4944.0
81.90	1122.0
82.90	156.0
85.90	287.0
86.90	5040.0
88.00	4795.0
90.90	608.0
92.00	4023.0
92.90	6537.0
94.00	15685.0
95.00	126664.0
96.00	8614.0
97.00	273.0
102.90	137.0
103.90	697.0
105.00	188.0
105.90	656.0
106.80	228.0
109.80	191.0
110.70	243.0
111.80	141.0
112.90	198.0
114.80	177.0
115.80	592.0
116.90	988.0
117.90	694.0
118.80	695.0
122.90	102.0
123.70	112.0
125.00	114.0
127.80	406.0
128.90	333.0
129.80	609.0
130.80	234.0
132.20	120.0
134.80	369.0
137.00	313.0
138.90	120.0
139.80	196.0
140.90	1829.0
142.00	181.0
142.90	1814.0
143.80	111.0
144.80	514.0
145.90	146.0
147.80	291.0
150.00	232.0
151.30	115.0
152.70	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

153.80	162.0
155.00	372.0
156.20	127.0
157.00	199.0
158.90	142.0
160.90	177.0
170.80	258.0
172.00	1625.0
173.90	105624.0
175.00	8427.0
175.90	101088.0
176.90	6823.0
178.00	206.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.00	1226.0
37.00	5791.0
38.00	5568.0
39.00	2308.0
40.00	491.0
41.20	160.0
42.20	109.0
42.80	163.0
44.00	1294.0
44.90	1079.0
45.90	191.0
47.00	1509.0
47.90	860.0
49.00	5301.0
50.00	24200.0
51.00	7520.0
52.00	356.0
53.00	212.0
55.00	323.0
56.00	1849.0
57.00	3815.0
57.90	276.0
59.90	1217.0
61.00	5687.0
62.00	6188.0
63.00	5310.0
64.00	660.0
65.00	881.0
65.90	154.0
67.00	485.0
68.00	12372.0
69.00	12747.0
70.00	1000.0
72.00	935.0
73.00	5909.0
74.00	22024.0
75.00	64240.0
76.00	5555.0
77.00	800.0
77.80	563.0
78.90	4493.0
79.90	1353.0
80.90	4597.0
81.80	1157.0
83.00	154.0
84.10	111.0
85.90	221.0
86.90	4611.0
88.00	4601.0
90.90	612.0
92.00	3968.0
92.90	6243.0
94.00	15096.0
95.00	121280.0
96.00	7862.0
97.00	211.0
102.90	113.0
103.90	663.0
104.80	145.0
105.00	149.0
105.90	596.0
106.80	257.0
109.80	154.0
110.70	199.0
111.90	142.0
112.90	215.0
114.80	200.0
115.80	507.0
116.80	997.0
117.90	678.0
118.80	713.0
122.90	139.0
125.00	125.0
127.80	443.0
128.90	296.0
129.80	601.0
130.80	242.0
134.00	125.0
134.80	321.0
136.90	327.0
138.90	145.0
139.80	198.0
140.80	1665.0
142.00	178.0
142.90	1702.0
143.80	140.0
144.80	439.0
145.80	161.0
147.90	354.0
149.90	217.0
151.30	123.0
152.80	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

153.80	148.0
155.00	334.0
156.20	134.0
157.00	232.0
158.80	106.0
161.00	171.0
170.80	215.0
172.00	1486.0
173.90	103264.0
175.00	8048.0
175.90	99072.0
176.90	6576.0
178.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
35.80	151.0
36.20	175.0
36.90	148.0
37.50	133.0
38.00	124.0
38.70	114.0
39.90	316.0
41.00	102.0
41.60	132.0
42.70	123.0
44.00	390.0
45.40	122.0
47.10	121.0
48.00	154.0
49.40	104.0
51.60	113.0
52.50	130.0
53.40	192.0
61.60	144.0
66.40	101.0
68.10	112.0
69.20	158.0
73.20	108.0
76.20	135.0
77.00	121.0
78.30	115.0
105.70	125.0
107.10	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41