

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021552.D
 Acq On : 23 Jun 2021 12:04
 Operator : SY/MD
 Sample : VV0623MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021552.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	228240	232891	13.40%	1.740%
2	1.565	157	163	175	rVB	187021	210892	12.13%	1.576%
3	2.105	322	331	365	rVB	383080	584955	33.65%	4.372%
4	2.696	513	515	517	rBV	434	274	0.02%	0.002%
5	2.815	551	552	556	rVB2	430	168	0.01%	0.001%
6	2.944	589	592	593	rBV	432	223	0.01%	0.002%
7	2.976	600	602	603	rBV	437	137	0.01%	0.001%
8	3.027	616	618	619	rBV	325	161	0.01%	0.001%
9	3.105	639	642	643	rBV	298	177	0.01%	0.001%
10	3.182	664	666	667	rBV	343	131	0.01%	0.001%
11	3.227	678	680	682	rBV	357	158	0.01%	0.001%
12	3.240	682	684	687	rVB3	324	196	0.01%	0.001%
13	3.262	689	691	694	rBV2	275	163	0.01%	0.001%
14	3.304	702	704	706	rBV2	485	256	0.01%	0.002%
15	3.397	730	733	739	rBV5	680	718	0.04%	0.005%
16	3.449	747	749	750	rBV5	417	180	0.01%	0.001%
17	3.481	756	759	762	rBV3	515	254	0.01%	0.002%
18	3.503	764	766	771	rVB2	440	348	0.02%	0.003%
19	3.532	773	775	777	rBV3	261	182	0.01%	0.001%
20	3.571	786	787	794	rBV4	425	396	0.02%	0.003%
21	3.735	835	838	840	rBV	314	171	0.01%	0.001%
22	3.770	844	849	850	rBV2	234	177	0.01%	0.001%
23	3.889	875	886	941	rVV	126878	440353	25.33%	3.291%
24	4.346	1011	1028	1059	rBV	274840	685456	39.43%	5.123%
25	4.568	1095	1097	1100	rBV3	592	305	0.02%	0.002%
26	4.751	1150	1154	1156	rBV2	277	193	0.01%	0.001%
27	4.793	1165	1167	1169	rBV	297	156	0.01%	0.001%
28	4.886	1193	1196	1197	rBV	395	248	0.01%	0.002%
29	4.966	1219	1221	1223	rBV	259	133	0.01%	0.001%
30	5.043	1226	1245	1282	rBV2	676597	1738507	100.00%	12.992%
31	5.339	1335	1337	1341	rBV5	691	520	0.03%	0.004%
32	5.368	1343	1346	1349	rVB4	814	512	0.03%	0.004%
33	5.410	1357	1359	1361	rVB3	537	211	0.01%	0.002%
34	5.494	1381	1385	1389	rBV4	436	431	0.02%	0.003%
35	5.616	1410	1423	1459	rBV	502977	1027272	59.09%	7.677%
36	5.908	1503	1514	1527	rBV3	18672	38830	2.23%	0.290%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021552.D
 Acq On : 23 Jun 2021 12:04
 Operator : SY/MD
 Sample : VV0623MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.005	1542	1544	1548	rBV4	358	268	0.02%	0.002%
38	6.069	1549	1564	1588	rBV	385096	786985	45.27%	5.881%
39	6.336	1645	1647	1650	rBV2	361	127	0.01%	0.001%
40	6.413	1668	1671	1672	rBV2	595	257	0.01%	0.002%
41	6.426	1672	1675	1678	rVB3	833	488	0.03%	0.004%
42	6.523	1704	1705	1707	rVB	429	163	0.01%	0.001%
43	6.632	1732	1739	1740	rBV4	1464	1323	0.08%	0.010%
44	6.706	1759	1762	1765	rBV2	675	489	0.03%	0.004%
45	6.725	1765	1768	1771	rVV2	803	488	0.03%	0.004%
46	6.754	1774	1777	1782	rVV4	514	357	0.02%	0.003%
47	6.777	1782	1784	1786	rVV	307	146	0.01%	0.001%
48	6.789	1786	1788	1789	rVB2	479	181	0.01%	0.001%
49	6.870	1810	1813	1816	rBV2	346	279	0.02%	0.002%
50	6.886	1816	1818	1822	rBV2	582	395	0.02%	0.003%
51	6.918	1826	1828	1834	rVB3	274	168	0.01%	0.001%
52	6.986	1838	1849	1881	rBV	229980	430148	24.74%	3.215%
53	7.317	1939	1952	1971	rBV	808507	1425416	81.99%	10.652%
54	7.622	2034	2047	2070	rBV	158117	284472	16.36%	2.126%
55	7.912	2135	2137	2140	rVB2	488	224	0.01%	0.002%
56	7.944	2140	2147	2150	rVB3	1003	1246	0.07%	0.009%
57	7.963	2150	2153	2154	rBV2	530	307	0.02%	0.002%
58	7.979	2154	2158	2159	rBV3	808	457	0.03%	0.003%
59	8.047	2177	2179	2182	rBV2	380	250	0.01%	0.002%
60	8.088	2182	2192	2237	rVV	463956	895425	51.51%	6.692%
61	8.609	2350	2354	2355	rBV2	435	289	0.02%	0.002%
62	8.645	2363	2365	2368	rBV3	422	187	0.01%	0.001%
63	8.764	2400	2402	2407	rBV5	614	408	0.02%	0.003%
64	8.850	2417	2429	2457	rBV	725870	1205679	69.35%	9.010%
65	9.127	2513	2515	2518	rBV2	452	237	0.01%	0.002%
66	9.143	2518	2520	2521	rBV2	893	449	0.03%	0.003%
67	9.220	2540	2544	2547	rBV3	413	251	0.01%	0.002%
68	9.243	2549	2551	2554	rBV4	445	281	0.02%	0.002%
69	9.429	2606	2609	2611	rBV2	486	229	0.01%	0.002%
70	9.538	2640	2643	2644	rBV2	522	283	0.02%	0.002%
71	9.571	2652	2653	2655	rBV	305	163	0.01%	0.001%
72	9.629	2669	2671	2673	rBV	487	170	0.01%	0.001%
73	9.661	2679	2681	2684	rBV	204	137	0.01%	0.001%
74	9.770	2712	2715	2718	rBV2	245	155	0.01%	0.001%
75	9.805	2722	2726	2729	rBV3	362	313	0.02%	0.002%
76	9.866	2739	2745	2749	rBV3	250	344	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021552.D
 Acq On : 23 Jun 2021 12:04
 Operator : SY/MD
 Sample : VV0623MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

77	9.944	2760	2769	2779	rVB4	1617	2746	0.16%	0.021%
78	9.989	2779	2783	2785	rBV3	363	295	0.02%	0.002%
79	10.130	2817	2827	2832	rVV4	2457	3529	0.20%	0.026%
80	10.217	2842	2854	2871	rBV	525294	826975	47.57%	6.180%
81	10.445	2923	2925	2929	rVB3	348	178	0.01%	0.001%
82	10.471	2931	2933	2937	rBV2	387	179	0.01%	0.001%
83	10.506	2941	2944	2947	rVB2	493	375	0.02%	0.003%
84	10.545	2947	2956	2960	rBV6	1325	2056	0.12%	0.015%
85	10.632	2981	2983	2988	rVB2	516	297	0.02%	0.002%
86	10.882	3058	3061	3063	rBV2	470	273	0.02%	0.002%
87	10.921	3063	3073	3082	rVV6	4097	6243	0.36%	0.047%
88	11.030	3101	3107	3108	rBV4	762	714	0.04%	0.005%
89	11.188	3151	3156	3161	rBV5	1694	2200	0.13%	0.016%
90	11.249	3164	3175	3202	rVV	774687	1222778	70.33%	9.138%
91	11.564	3271	3273	3276	rBV2	489	272	0.02%	0.002%
92	11.625	3280	3292	3311	rBV	803629	1271160	73.12%	9.500%
93	12.050	3422	3424	3427	rVB	566	226	0.01%	0.002%
94	12.079	3431	3433	3435	rBV	485	296	0.02%	0.002%
95	12.339	3511	3514	3518	rBV4	471	384	0.02%	0.003%
96	12.654	3604	3612	3621	rBV6	3412	5007	0.29%	0.037%
97	12.934	3696	3699	3702	rBV3	601	464	0.03%	0.003%
98	13.271	3796	3804	3814	rBV4	4708	7434	0.43%	0.056%
99	13.509	3872	3878	3889	rBV2	7632	11650	0.67%	0.087%
100	13.747	3945	3952	3962	rBV2	6625	9396	0.54%	0.070%




Sum of corrected areas: 13381096

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021552.D
Acq On : 23 Jun 2021 12:04
Operator : SY/MD
Sample : VV0623MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

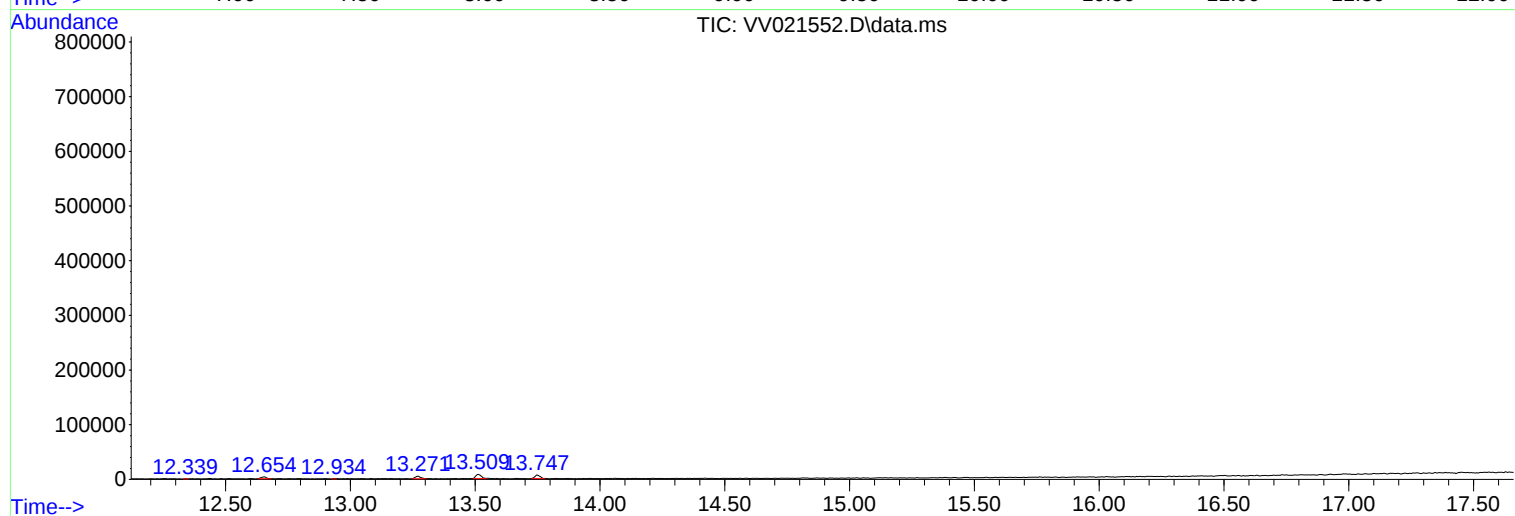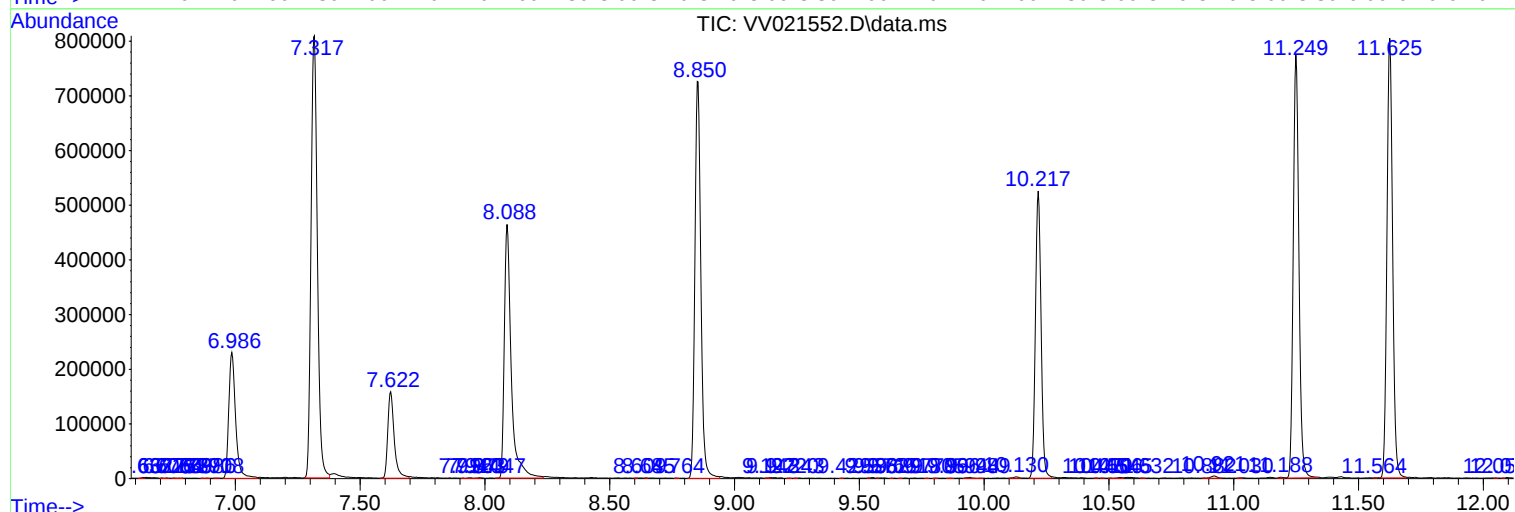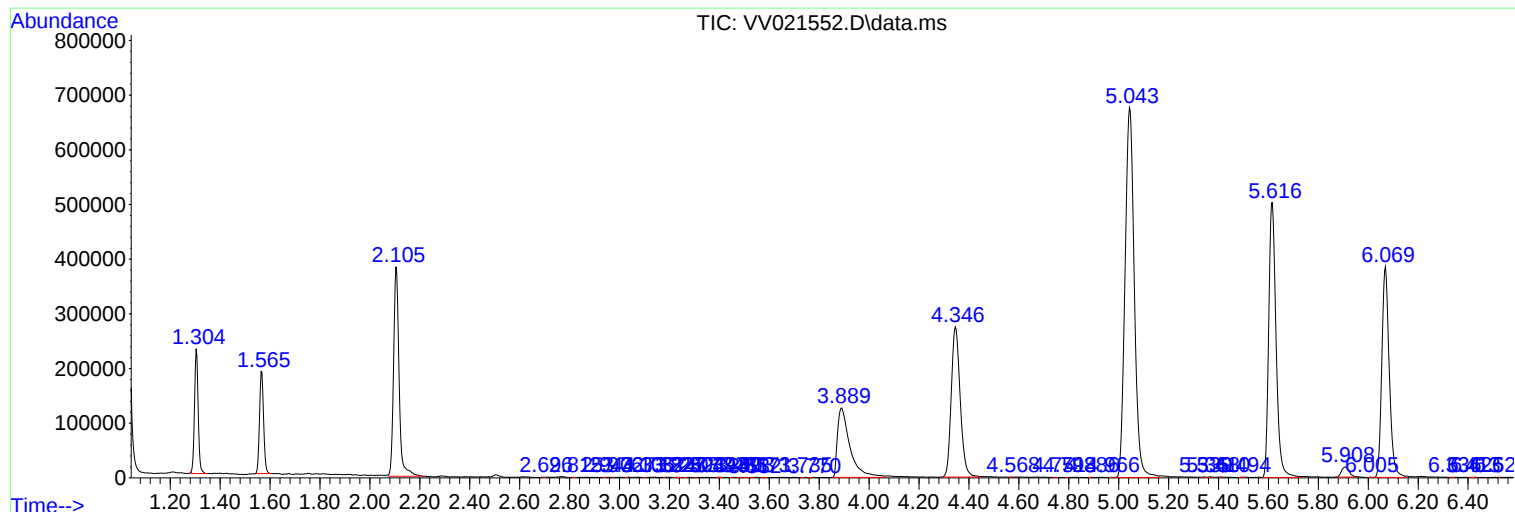

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021552.D
Acq On : 23 Jun 2021 12:04
Operator : SY/MD
Sample : VV0623MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021552.D
Acq On : 23 Jun 2021 12:04
Operator : SY/MD
Sample : VV0623MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK194

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc