

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021553.D
 Acq On : 23 Jun 2021 12:53
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	217627	221445	13.19%	1.719%
2	1.564	156	163	178	rBV	183662	206374	12.29%	1.602%
3	2.105	321	331	377	rVB	366530	574970	34.25%	4.464%
4	2.873	568	570	572	rBV	360	163	0.01%	0.001%
5	2.928	585	587	589	rBV2	411	170	0.01%	0.001%
6	3.130	648	650	651	rBV	294	113	0.01%	0.001%
7	3.217	675	677	678	rBV	542	239	0.01%	0.002%
8	3.252	683	688	690	rBV3	408	265	0.02%	0.002%
9	3.272	690	694	695	rBV3	283	146	0.01%	0.001%
10	3.336	712	714	717	rBV2	495	316	0.02%	0.002%
11	3.375	721	726	731	rVV3	619	604	0.04%	0.005%
12	3.400	732	734	738	rVB	424	249	0.01%	0.002%
13	3.426	738	742	746	rBV2	421	440	0.03%	0.003%
14	3.458	750	752	756	rVB2	360	168	0.01%	0.001%
15	3.494	759	763	764	rBV2	519	327	0.02%	0.003%
16	3.510	764	768	774	rVB3	514	522	0.03%	0.004%
17	3.539	774	777	780	rBV3	346	254	0.02%	0.002%
18	3.590	791	793	794	rBV	198	77	0.00%	0.001%
19	3.600	794	796	797	rVB2	337	92	0.01%	0.001%
20	3.661	811	815	816	rBV2	423	243	0.01%	0.002%
21	3.706	827	829	833	rVB2	606	379	0.02%	0.003%
22	3.735	833	838	840	rBV2	455	375	0.02%	0.003%
23	3.789	852	855	859	rVB3	474	287	0.02%	0.002%
24	3.809	859	861	864	rBV2	512	355	0.02%	0.003%
25	3.886	874	885	933	rBV2	117746	424728	25.30%	3.297%
26	4.342	1012	1027	1057	rBV	265435	656436	39.10%	5.096%
27	4.587	1101	1103	1105	rBV3	537	235	0.01%	0.002%
28	4.658	1123	1125	1128	rVB2	484	189	0.01%	0.001%
29	4.773	1156	1161	1164	rBV4	519	410	0.02%	0.003%
30	4.796	1166	1168	1170	rVV2	244	101	0.01%	0.001%
31	4.828	1175	1178	1184	rVB4	564	523	0.03%	0.004%
32	4.876	1190	1193	1195	rBV3	401	220	0.01%	0.002%
33	4.905	1200	1202	1203	rBV3	340	117	0.01%	0.001%
34	5.040	1226	1244	1274	rBV2	651565	1678755	100.00%	13.033%
35	5.358	1341	1343	1346	rBV	733	466	0.03%	0.004%
36	5.465	1371	1376	1379	rBV3	537	478	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021553.D
 Acq On : 23 Jun 2021 12:53
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	5.612	1409	1422	1450	rBV	482971	975032	58.08%	7.569%
38	5.902	1502	1512	1537	rVB3	19839	42982	2.56%	0.334%
39	6.066	1549	1563	1586	rBV	366510	754686	44.96%	5.859%
40	6.352	1649	1652	1655	rVB3	755	371	0.02%	0.003%
41	6.371	1655	1658	1660	rBV3	513	288	0.02%	0.002%
42	6.410	1668	1670	1672	rVB	390	155	0.01%	0.001%
43	6.448	1677	1682	1684	rBV2	294	243	0.01%	0.002%
44	6.458	1684	1685	1687	rBV	408	137	0.01%	0.001%
45	6.493	1694	1696	1697	rBV	230	72	0.00%	0.001%
46	6.506	1697	1700	1706	rBV3	615	643	0.04%	0.005%
47	6.577	1718	1722	1725	rVB2	483	364	0.02%	0.003%
48	6.638	1732	1741	1742	rBV4	1464	1880	0.11%	0.015%
49	6.754	1774	1777	1780	rBV2	511	392	0.02%	0.003%
50	6.831	1796	1801	1803	rBV2	320	240	0.01%	0.002%
51	6.844	1803	1805	1807	rBV	329	179	0.01%	0.001%
52	6.886	1816	1818	1819	rBV2	138	71	0.00%	0.001%
53	6.892	1819	1820	1823	rVV	225	114	0.01%	0.001%
54	6.944	1833	1836	1837	rBV	365	178	0.01%	0.001%
55	6.982	1837	1848	1876	rBV	223968	417755	24.88%	3.243%
56	7.313	1939	1951	1972	rBV	787629	1367907	81.48%	10.619%
57	7.587	2034	2036	2037	rBV2	557	290	0.02%	0.002%
58	7.619	2037	2046	2071	rVV	152527	272651	16.24%	2.117%
59	7.834	2111	2113	2116	rVB2	656	353	0.02%	0.003%
60	7.899	2130	2133	2136	rBV	589	410	0.02%	0.003%
61	7.950	2148	2149	2154	rVB2	537	243	0.01%	0.002%
62	7.976	2154	2157	2159	rBV3	840	547	0.03%	0.004%
63	8.040	2175	2177	2178	rBV3	187	78	0.00%	0.001%
64	8.088	2182	2192	2234	rVV	439010	852437	50.78%	6.618%
65	8.471	2309	2311	2314	rVB3	543	222	0.01%	0.002%
66	8.506	2318	2322	2325	rBV3	559	460	0.03%	0.004%
67	8.686	2376	2378	2379	rBV2	408	159	0.01%	0.001%
68	8.760	2399	2401	2403	rBV	291	125	0.01%	0.001%
69	8.770	2403	2404	2406	rVB	579	207	0.01%	0.002%
70	8.783	2406	2408	2410	rBV2	466	277	0.02%	0.002%
71	8.850	2417	2429	2458	rBV	705811	1167682	69.56%	9.065%
72	9.095	2503	2505	2509	rBV3	427	195	0.01%	0.002%
73	9.149	2517	2522	2532	rVB6	1013	1822	0.11%	0.014%
74	9.204	2535	2539	2542	rBV2	547	561	0.03%	0.004%
75	9.284	2562	2564	2567	rBV	341	176	0.01%	0.001%
76	9.300	2567	2569	2574	rVV3	385	393	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021553.D
 Acq On : 23 Jun 2021 12:53
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.333	2577	2579	2586	rVB3	584	458	0.03%	0.004%
78	9.362	2586	2588	2591	rBV2	274	154	0.01%	0.001%
79	9.432	2608	2610	2612	rBV	390	173	0.01%	0.001%
80	9.548	2640	2646	2648	rBV4	677	734	0.04%	0.006%
81	9.583	2656	2657	2659	rVB	611	154	0.01%	0.001%
82	9.667	2681	2683	2686	rBV2	568	456	0.03%	0.004%
83	9.988	2781	2783	2787	rVB	413	218	0.01%	0.002%
84	10.014	2787	2791	2792	rBV	334	187	0.01%	0.001%
85	10.217	2841	2854	2873	rBV	497733	804500	47.92%	6.246%
86	10.461	2924	2930	2934	rBV2	522	709	0.04%	0.006%
87	10.538	2950	2954	2957	rBV4	656	684	0.04%	0.005%
88	10.696	2999	3003	3005	rBV2	496	411	0.02%	0.003%
89	10.738	3014	3016	3018	rBV2	325	168	0.01%	0.001%
90	10.799	3033	3035	3038	rVB2	259	76	0.00%	0.001%
91	10.834	3044	3046	3050	rBV2	433	332	0.02%	0.003%
92	10.918	3062	3072	3083	rBV8	2872	5578	0.33%	0.043%
93	11.001	3096	3098	3099	rBV8	305	137	0.01%	0.001%
94	11.146	3138	3143	3152	rVB5	1746	2552	0.15%	0.020%
95	11.249	3163	3175	3194	rBV	767250	1189947	70.88%	9.238%
96	11.529	3260	3262	3264	rBV3	443	274	0.02%	0.002%
97	11.625	3280	3292	3310	rBV	763470	1238398	73.77%	9.614%
98	12.066	3427	3429	3430	rBV	495	215	0.01%	0.002%
99	12.397	3530	3532	3536	rVB	509	223	0.01%	0.002%
100	12.583	3587	3590	3591	rBV2	463	268	0.02%	0.002%




Sum of corrected areas: 12881214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021553.D
Acq On : 23 Jun 2021 12:53
Operator : SY/MD
Sample : VV0623WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK195

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

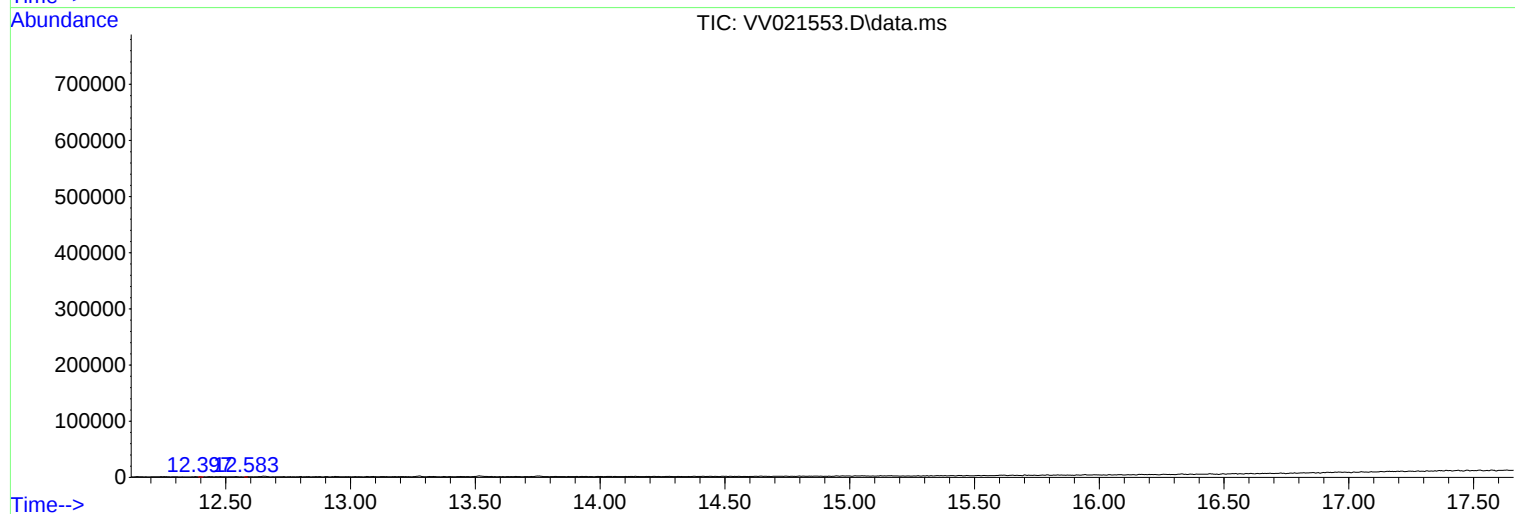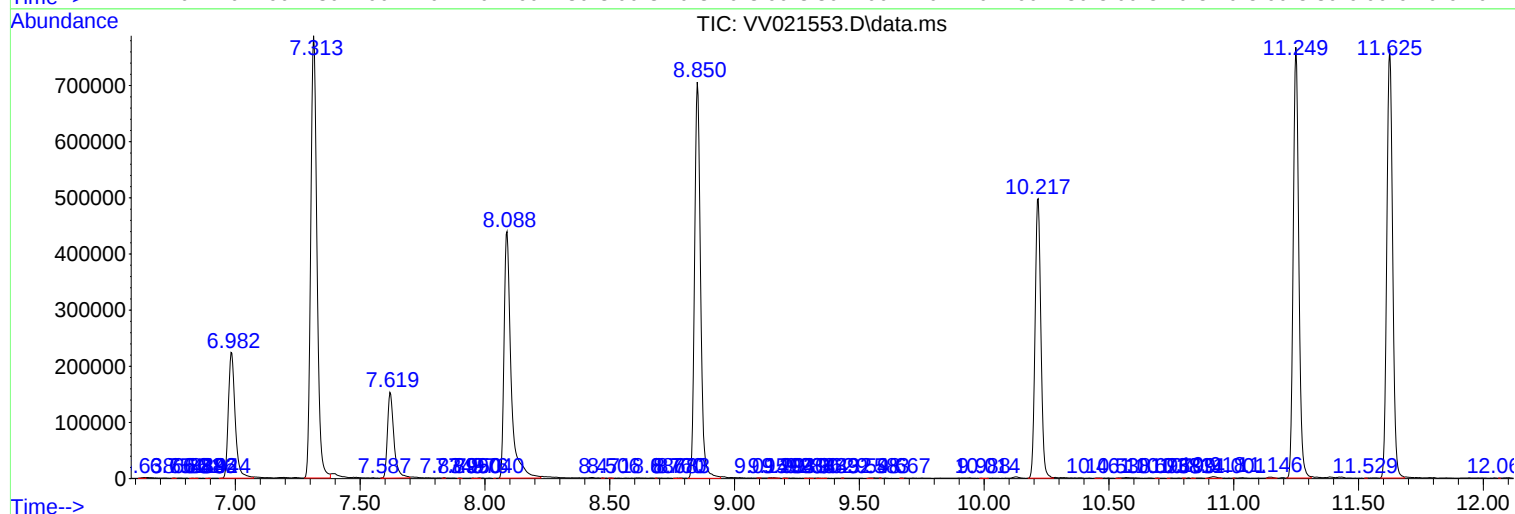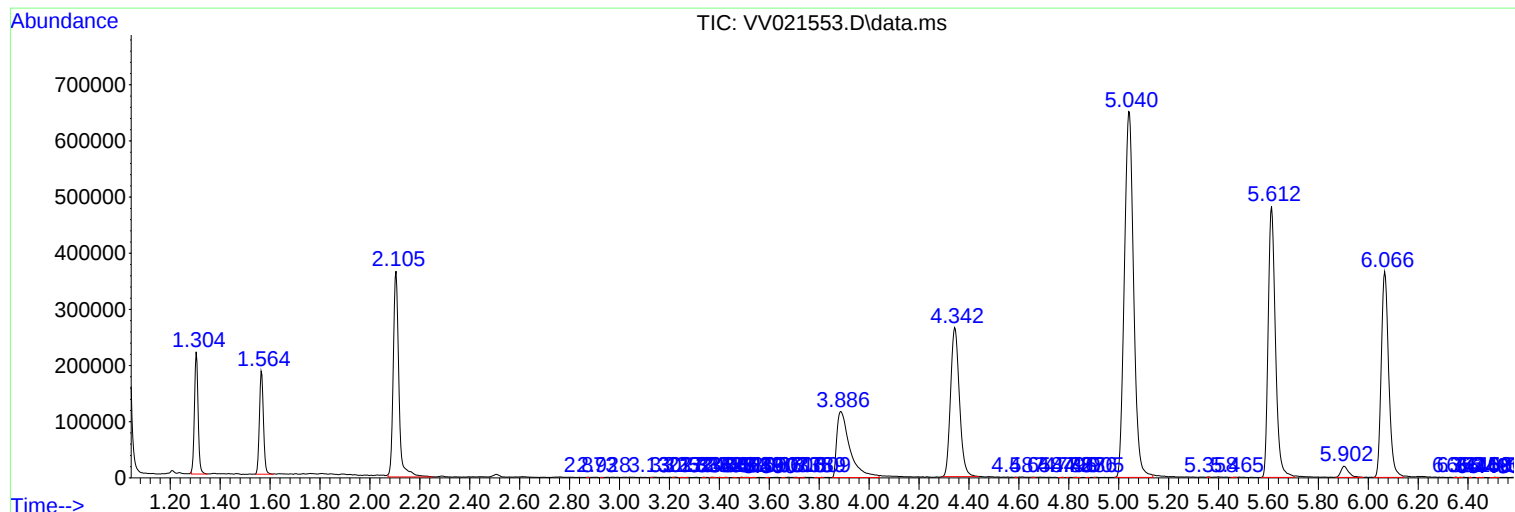

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021553.D
Acq On : 23 Jun 2021 12:53
Operator : SY/MD
Sample : VV0623WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK195

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021553.D
Acq On : 23 Jun 2021 12:53
Operator : SY/MD
Sample : VV0623WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK195

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
