

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021556.D
 Acq On : 23 Jun 2021 14:27
 Operator : SY/MD
 Sample : M2808-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

Signal : TIC: VV021556.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	221823	231219	13.20%	1.699%
2	1.568	157	164	177	rBV	193794	213085	12.16%	1.566%
3	2.108	322	332	372	rVB	372460	572483	32.67%	4.206%
4	2.510	448	457	470	rBV2	8143	14301	0.82%	0.105%
5	2.725	522	524	526	rBV	668	265	0.02%	0.002%
6	2.863	565	567	569	rBV2	449	170	0.01%	0.001%
7	2.937	586	590	592	rBV	616	443	0.03%	0.003%
8	3.002	608	610	613	rVB2	614	249	0.01%	0.002%
9	3.140	651	653	655	rVB	316	102	0.01%	0.001%
10	3.172	660	663	665	rBV	458	330	0.02%	0.002%
11	3.265	690	692	694	rBV2	396	188	0.01%	0.001%
12	3.297	697	702	706	rBV3	571	659	0.04%	0.005%
13	3.336	712	714	716	rVB	244	92	0.01%	0.001%
14	3.381	725	728	729	rBV3	247	135	0.01%	0.001%
15	3.391	729	731	734	rVB2	457	215	0.01%	0.002%
16	3.445	746	748	751	rBV	289	176	0.01%	0.001%
17	3.481	757	759	760	rBV	260	129	0.01%	0.001%
18	3.513	766	769	771	rBV2	384	237	0.01%	0.002%
19	3.677	818	820	822	rBV	387	200	0.01%	0.001%
20	3.693	823	825	831	rVB3	482	373	0.02%	0.003%
21	3.722	831	834	835	rBV	255	128	0.01%	0.001%
22	3.735	835	838	839	rBV	413	200	0.01%	0.001%
23	3.902	878	890	942	rBV	105540	420568	24.00%	3.090%
24	4.349	1015	1029	1060	rVB	274389	674387	38.49%	4.955%
25	4.670	1127	1129	1130	rBV	329	117	0.01%	0.001%
26	4.838	1177	1181	1185	rBV2	472	412	0.02%	0.003%
27	4.860	1185	1188	1189	rVB2	291	111	0.01%	0.001%
28	4.870	1189	1191	1193	rBV	267	115	0.01%	0.001%
29	4.899	1197	1200	1203	rBV3	382	277	0.02%	0.002%
30	4.918	1203	1206	1210	rBV3	381	334	0.02%	0.002%
31	4.989	1225	1228	1230	rBV2	410	278	0.02%	0.002%
32	5.047	1230	1246	1283	rVV2	689457	1752166	100.00%	12.874%
33	5.513	1387	1391	1397	rBV4	670	843	0.05%	0.006%
34	5.558	1404	1405	1407	rBV	281	95	0.01%	0.001%
35	5.619	1411	1424	1452	rBV	530234	1075883	61.40%	7.905%
36	5.908	1503	1514	1533	rBV2	18761	41311	2.36%	0.304%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021556.D
 Acq On : 23 Jun 2021 14:27
 Operator : SY/MD
 Sample : M2808-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	5.995	1539	1541	1543	rVB2	473	182	0.01%	0.001%
38	6.072	1550	1565	1591	rBV	385757	792780	45.25%	5.825%
39	6.310	1637	1639	1641	rBV3	712	356	0.02%	0.003%
40	6.346	1647	1650	1651	rVB	263	136	0.01%	0.001%
41	6.429	1674	1676	1677	rVB	376	93	0.01%	0.001%
42	6.455	1682	1684	1689	rVB2	414	301	0.02%	0.002%
43	6.474	1689	1690	1694	rVB2	233	103	0.01%	0.001%
44	6.513	1694	1702	1704	rBV3	732	765	0.04%	0.006%
45	6.529	1704	1707	1710	rVB2	354	216	0.01%	0.002%
46	6.548	1710	1713	1714	rBV	185	105	0.01%	0.001%
47	6.603	1724	1730	1732	rBV	295	295	0.02%	0.002%
48	6.709	1759	1763	1765	rBV3	533	394	0.02%	0.003%
49	6.799	1785	1791	1795	rBV4	440	414	0.02%	0.003%
50	6.870	1810	1813	1820	rBV3	323	251	0.01%	0.002%
51	6.921	1823	1829	1830	rBV	225	235	0.01%	0.002%
52	6.989	1835	1850	1888	rBV	234842	438323	25.02%	3.221%
53	7.317	1940	1952	1974	rBV	823362	1439574	82.16%	10.577%
54	7.622	2037	2047	2070	rBV	163478	285891	16.32%	2.101%
55	7.870	2122	2124	2127	rBV	525	398	0.02%	0.003%
56	7.924	2137	2141	2142	rBV	423	264	0.02%	0.002%
57	7.937	2142	2145	2150	rVV3	584	590	0.03%	0.004%
58	8.091	2182	2193	2232	rBV	471329	911357	52.01%	6.696%
59	8.458	2305	2307	2311	rBV3	463	407	0.02%	0.003%
60	8.587	2345	2347	2348	rBV3	414	141	0.01%	0.001%
61	8.612	2353	2355	2356	rBV	427	161	0.01%	0.001%
62	8.677	2371	2375	2377	rBV2	341	272	0.02%	0.002%
63	8.757	2398	2400	2402	rBV	240	113	0.01%	0.001%
64	8.776	2402	2406	2407	rBV2	311	242	0.01%	0.002%
65	8.854	2417	2430	2453	rBV	778619	1273831	72.70%	9.360%
66	9.053	2490	2492	2496	rBV2	493	368	0.02%	0.003%
67	9.111	2507	2510	2512	rBV2	430	259	0.01%	0.002%
68	9.153	2518	2523	2526	rBV5	612	706	0.04%	0.005%
69	9.259	2554	2556	2558	rBV2	277	110	0.01%	0.001%
70	9.387	2594	2596	2599	rBV2	236	128	0.01%	0.001%
71	9.448	2611	2615	2616	rBV2	276	200	0.01%	0.001%
72	9.461	2616	2619	2624	rVB2	465	372	0.02%	0.003%
73	9.554	2645	2648	2651	rBV3	607	361	0.02%	0.003%
74	9.590	2657	2659	2661	rBV2	301	196	0.01%	0.001%
75	9.603	2661	2663	2666	rVV3	668	390	0.02%	0.003%
76	9.731	2701	2703	2707	rVB3	496	260	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021556.D
 Acq On : 23 Jun 2021 14:27
 Operator : SY/MD
 Sample : M2808-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.776	2715	2717	2720	rVB	372	172	0.01%	0.001%
78	9.831	2729	2734	2736	rBV2	416	325	0.02%	0.002%
79	9.860	2739	2743	2744	rBV	352	211	0.01%	0.002%
80	9.895	2751	2754	2755	rBV	347	197	0.01%	0.001%
81	9.992	2781	2784	2786	rBV2	262	177	0.01%	0.001%
82	10.130	2820	2827	2837	rVB4	2513	3737	0.21%	0.027%
83	10.217	2843	2854	2882	rBV	535406	838687	47.87%	6.162%
84	10.439	2919	2923	2927	rVB2	513	385	0.02%	0.003%
85	10.458	2927	2929	2930	rBV	423	191	0.01%	0.001%
86	10.490	2937	2939	2943	rBV2	427	357	0.02%	0.003%
87	10.876	3057	3059	3061	rBV2	299	125	0.01%	0.001%
88	10.921	3066	3073	3080	rVB7	2465	3531	0.20%	0.026%
89	11.033	3102	3108	3112	rBV3	906	1124	0.06%	0.008%
90	11.143	3137	3142	3151	rBV5	2147	3033	0.17%	0.022%
91	11.181	3152	3154	3157	rBV2	387	269	0.02%	0.002%
92	11.249	3164	3175	3203	rBV	834904	1302511	74.34%	9.570%
93	11.625	3280	3292	3318	rBV	834166	1298105	74.09%	9.538%
94	11.853	3357	3363	3365	rBV4	809	925	0.05%	0.007%
95	12.120	3444	3446	3449	rBV	418	310	0.02%	0.002%
96	12.207	3470	3473	3477	rBV2	397	337	0.02%	0.002%
97	12.300	3500	3502	3506	rBV2	434	289	0.02%	0.002%
98	12.349	3515	3517	3520	rBV3	538	303	0.02%	0.002%
99	12.660	3609	3614	3615	rBV2	553	512	0.03%	0.004%
100	12.898	3686	3688	3690	rBV2	535	315	0.02%	0.002%


Sum of corrected areas: 13609944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021556.D
Acq On : 23 Jun 2021 14:27
Operator : SY/MD
Sample : M2808-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

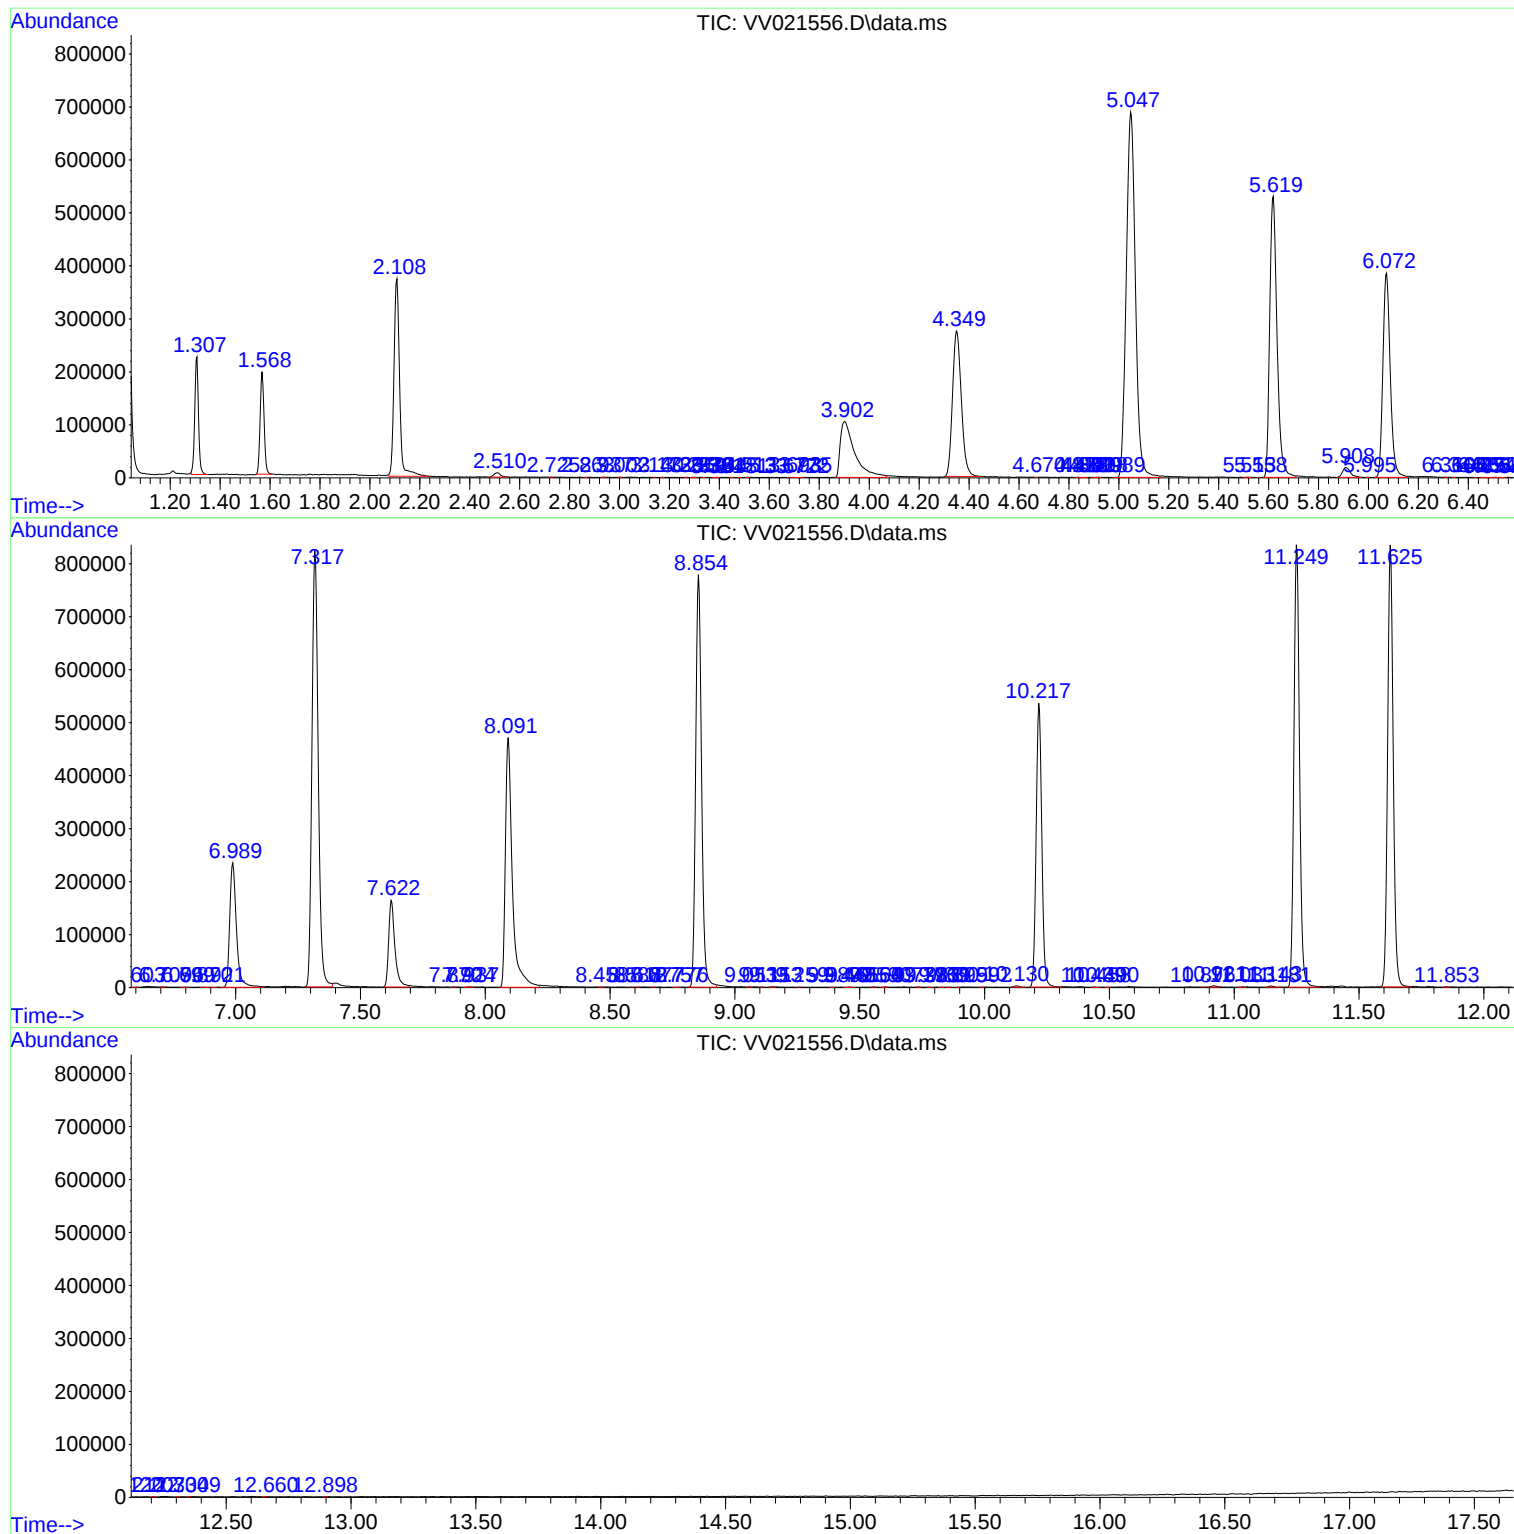

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021556.D
Acq On : 23 Jun 2021 14:27
Operator : SY/MD
Sample : M2808-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
Data File : VV021556.D
Acq On : 23 Jun 2021 14:27
Operator : SY/MD
Sample : M2808-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
