
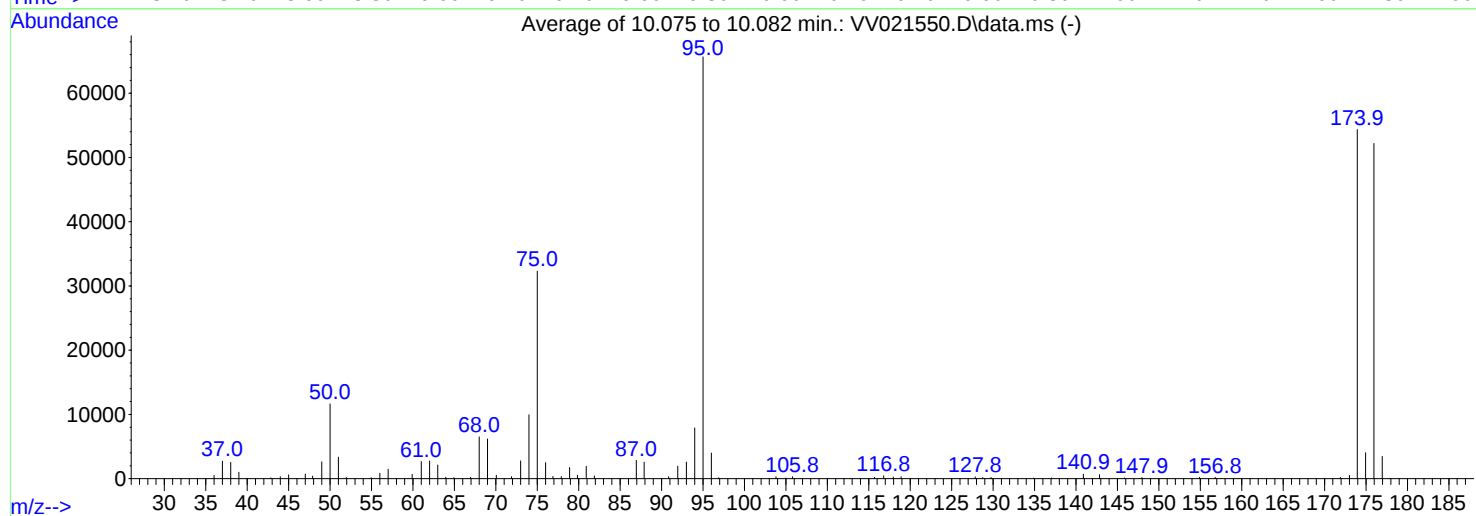


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062321\
 Data File : VV021550.D
 Acq On : 23 Jun 2021 10:07
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB171

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 25 03:01:05 2021

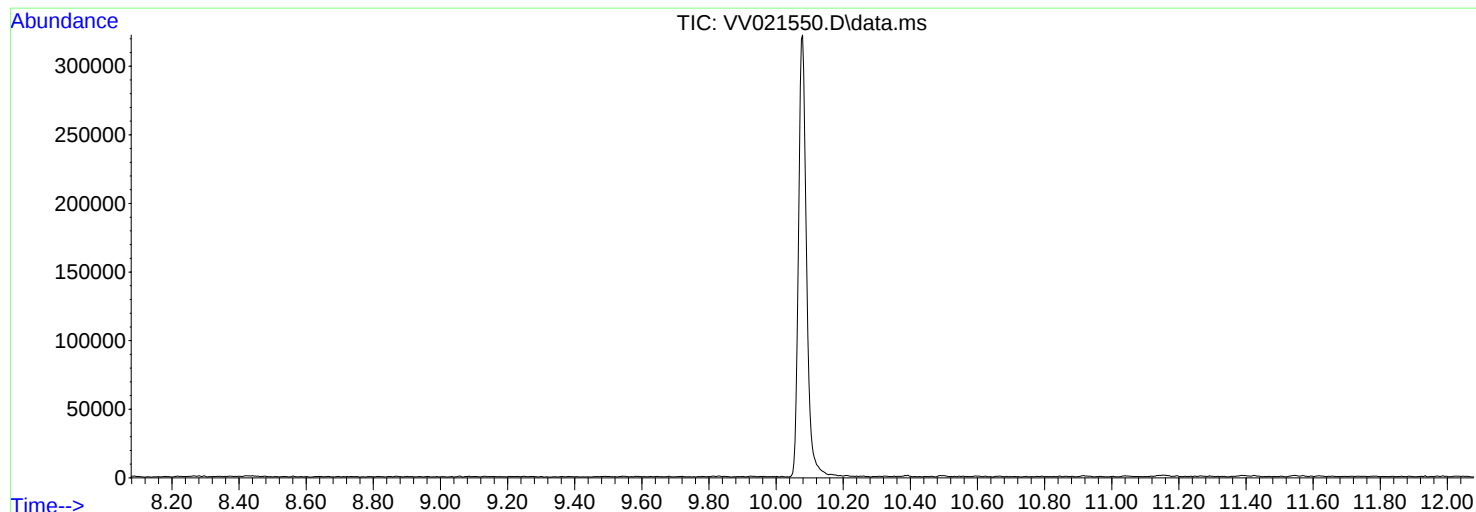

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	11631	PASS
75	95	30	80	49.2	32304	PASS
95	95	100	100	100.0	65661	PASS
96	95	5	9	6.1	3976	PASS
173	174	0.00	2	0.9	503	PASS
174	95	50	120	82.8	54349	PASS
175	174	5	9	7.4	4029	PASS
176	174	95	105	96.0	52181	PASS
177	176	5	10	6.6	3461	PASS

m/z	Abundance
36.00	537.0
37.00	2709.0
38.00	2542.0
39.00	1064.0
39.90	238.0
41.00	135.0
42.80	133.0
44.00	755.0
45.00	659.0
47.00	779.0
47.90	388.0
49.00	2725.0
50.00	12109.0
51.00	3416.0
51.90	187.0
55.00	284.0
56.00	977.0
57.00	1499.0
59.90	666.0
61.00	2853.0
62.00	2839.0
63.00	2208.0
64.10	187.0
65.00	177.0
66.90	214.0
68.00	6720.0
69.00	6392.0
70.00	568.0
71.90	333.0
73.00	2879.0
74.00	10341.0
75.00	33408.0
76.00	2567.0
76.90	378.0
77.90	301.0
78.90	1753.0
79.90	562.0
80.90	1951.0
81.90	465.0
87.00	3014.0
87.90	2562.0
90.90	333.0
92.00	2016.0
93.00	2677.0
94.00	8267.0
95.00	66704.0
96.00	4109.0
96.90	145.0
103.80	367.0
105.00	137.0
105.80	291.0
112.00	121.0
112.80	109.0
115.70	205.0
116.80	459.0
117.90	265.0
118.90	360.0
127.90	266.0
128.70	181.0
129.70	191.0
130.00	190.0
134.90	157.0
137.10	139.0
140.90	661.0
142.80	654.0
145.80	141.0
148.00	180.0
154.90	170.0
156.80	178.0
171.90	221.0
173.00	541.0
173.90	54728.0
175.00	4058.0
176.00	52504.0
177.00	3431.0
177.80	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB171

m/z	Abundance
36.00	521.0
37.00	2859.0
38.00	2621.0
39.00	998.0
39.90	236.0
40.90	124.0
42.80	127.0
44.00	731.0
45.00	604.0
47.00	709.0
47.90	403.0
49.00	2687.0
50.00	12035.0
51.00	3457.0
52.00	177.0
55.00	262.0
56.00	884.0
57.00	1497.0
59.90	699.0
61.00	2673.0
62.00	2877.0
63.00	2200.0
63.90	213.0
65.00	166.0
66.90	216.0
68.00	6766.0
69.00	6356.0
70.00	546.0
71.90	321.0
73.00	2853.0
74.00	10223.0
75.00	33296.0
76.00	2488.0
76.90	350.0
77.90	345.0
78.90	1810.0
79.90	531.0
80.90	2024.0
81.90	445.0
86.00	114.0
87.00	2930.0
87.90	2611.0
90.90	303.0
92.00	1994.0
93.00	2651.0
94.00	8183.0
95.00	67592.0
96.00	4068.0
96.90	145.0
103.80	328.0
105.00	129.0
105.80	336.0
106.80	111.0
115.70	210.0
116.80	455.0
117.90	254.0
118.90	328.0
127.80	271.0
128.80	177.0
129.70	226.0
134.90	141.0
137.00	136.0
140.90	714.0
142.90	628.0
145.80	151.0
148.00	171.0
154.90	205.0
156.80	207.0
171.90	216.0
173.00	521.0
174.00	55984.0
175.00	4162.0
176.00	54024.0
176.90	3628.0
178.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB171

m/z	Abundance
36.00	470.0
37.00	2620.0
38.00	2432.0
39.00	926.0
39.90	257.0
40.80	117.0
42.90	110.0
44.00	715.0
45.00	544.0
47.00	718.0
47.90	376.0
49.00	2399.0
50.00	10749.0
51.00	3153.0
52.00	190.0
55.00	252.0
56.00	707.0
57.00	1408.0
59.90	662.0
61.00	2455.0
62.00	2528.0
63.00	1939.0
63.90	258.0
64.90	123.0
66.50	111.0
67.00	219.0
68.00	6041.0
69.00	5812.0
70.10	489.0
71.90	281.0
73.00	2549.0
74.00	9289.0
75.00	30208.0
76.00	2404.0
76.90	348.0
77.90	345.0
78.90	1672.0
79.80	491.0
80.90	1810.0
81.90	387.0
86.00	110.0
86.90	2542.0
87.90	2494.0
90.80	269.0
91.90	1790.0
93.00	2466.0
94.00	7220.0
95.00	62688.0
96.00	3750.0
96.90	129.0
103.80	244.0
105.80	319.0
115.70	207.0
116.80	428.0
118.00	226.0
118.90	241.0
127.80	275.0
128.80	138.0
129.80	223.0
137.00	113.0
140.90	691.0
142.90	603.0
145.90	117.0
147.90	154.0
154.90	192.0
156.80	187.0
171.90	177.0
173.00	446.0
174.00	52336.0
174.90	3866.0
175.90	50016.0
176.90	3324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB171

Scan 2799 (10.040 min): VV021550.D\data.ms
BFB71

m/z	Abundance
39.90	186.0
41.00	164.0
44.00	422.0
54.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB171