




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026511.D
 Acq On : 23 Jun 2022 13:55
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Manual IntegrationsAPPROVED

Quant Time: Jun 24 00:51:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

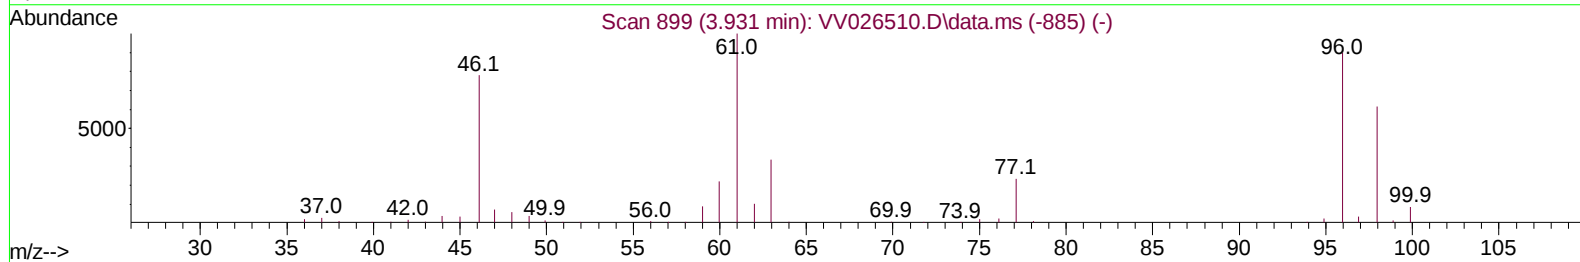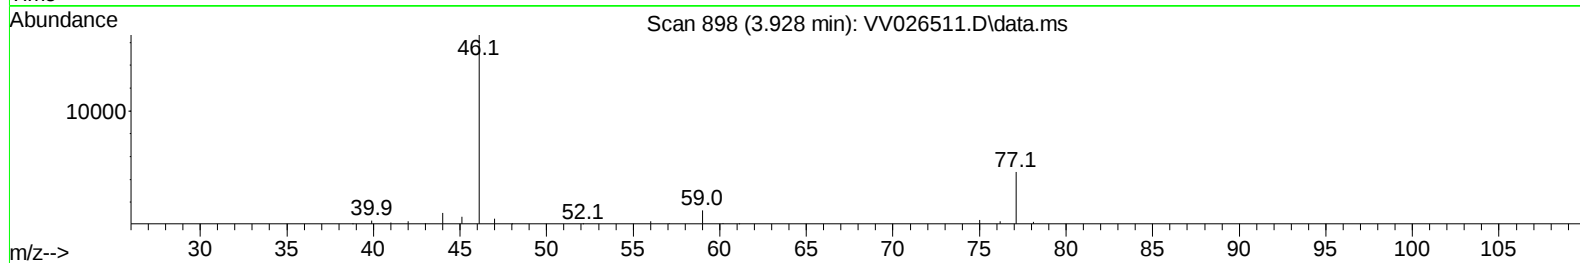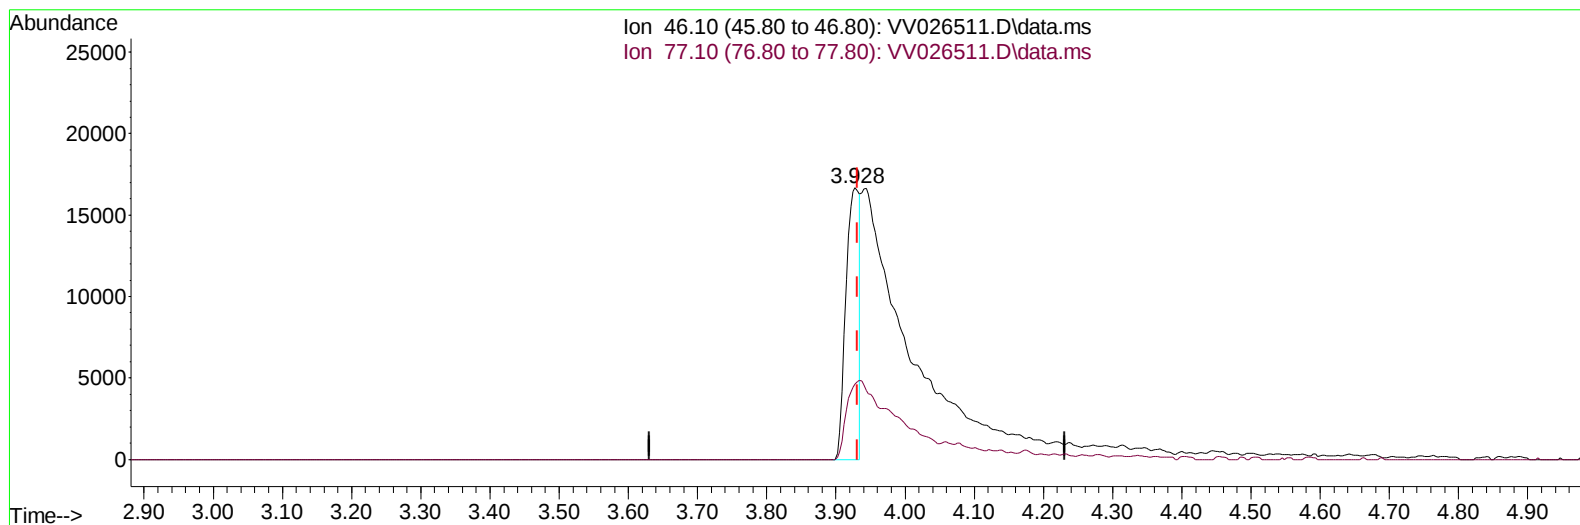

TIC: VV026511.D\data.ms

(20) 2-Butanone-d5 (S)

3.928min (-0.003) 13.81 ug/L

response 23178

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	28.50	102.76#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026511.D
 Acq On : 23 Jun 2022 13:55
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Manual IntegrationsAPPROVED

Quant Time: Jun 24 00:51:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

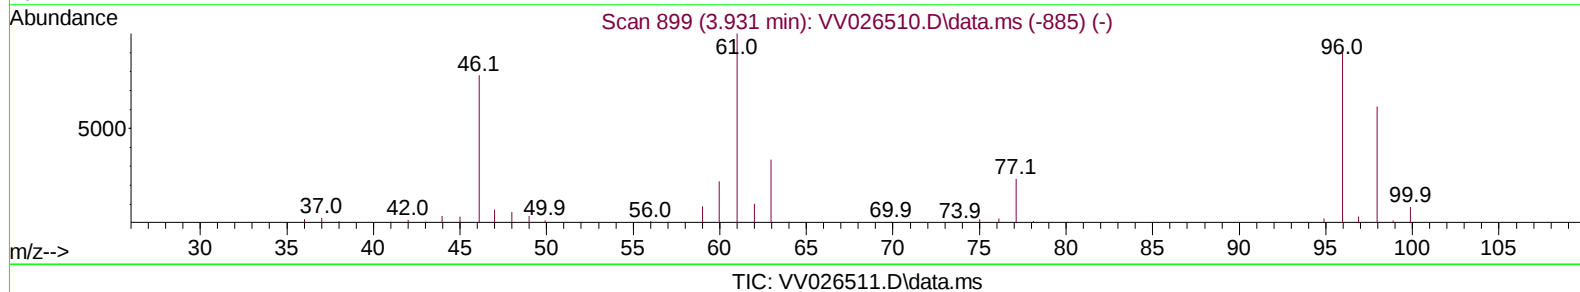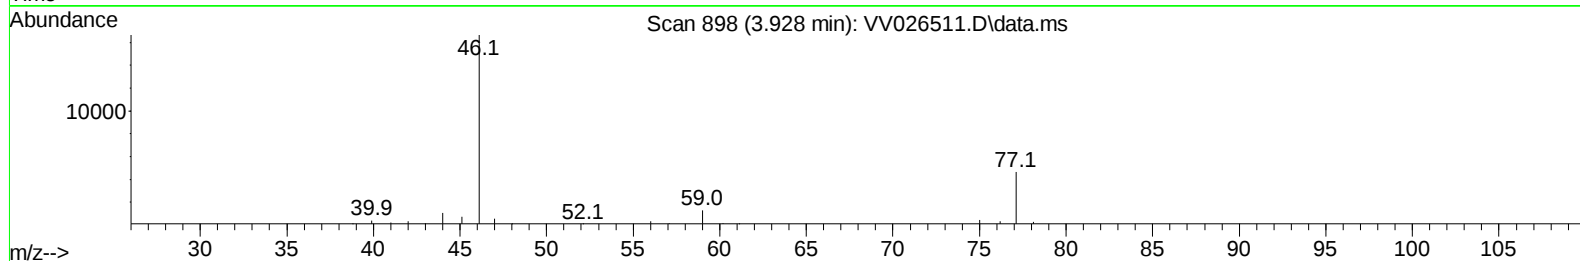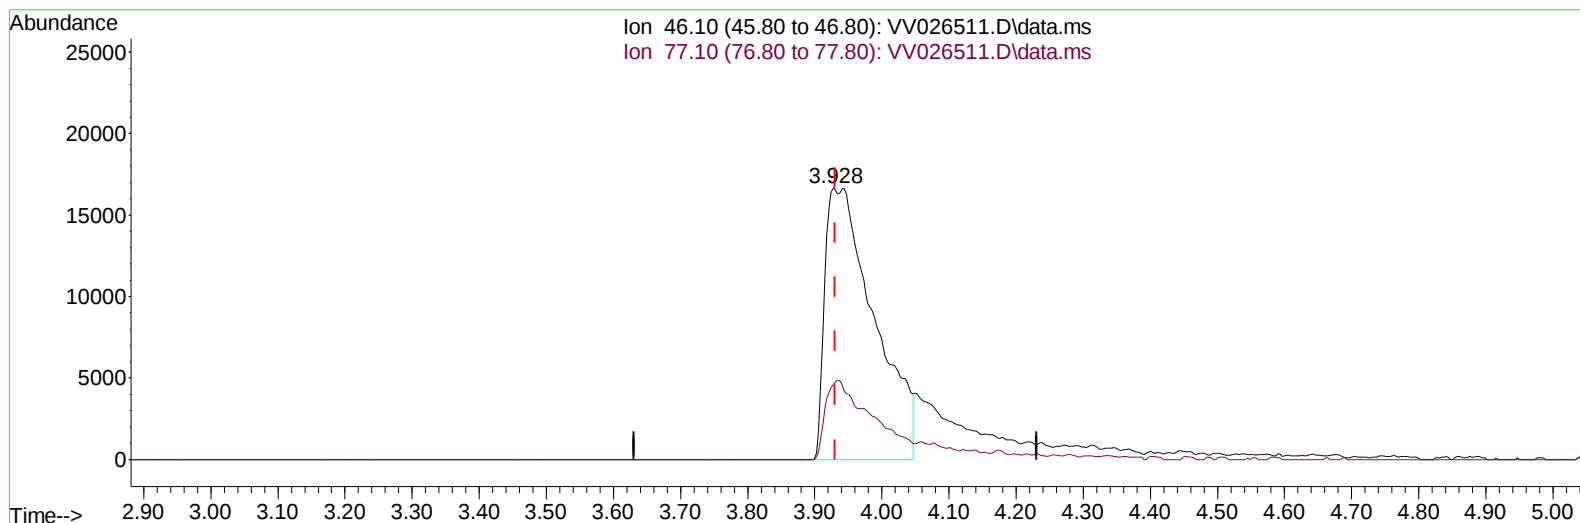

(20) 2-Butanone-d5 (S)

3.928min (-0.003) 50.69 ug/L m

response 85063

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	28.50	28.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026511.D
 Acq On : 23 Jun 2022 13:55
 Operator : SY/MD
 Sample : VV0623WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Manual IntegrationsAPPROVED

Quant Time: Jun 24 00:51:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	209893	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	197012	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	85023	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.314	65	81893	4.852	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	97.000%		
7) Chloroethane-d5	1.574	69	65963	4.864	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	97.200%		
11) 1,1-Dichloroethene-d2	2.114	63	109694	3.657	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	73.200%		
20) 2-Butanone-d5	3.928	46	85063m	50.687	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	101.380%		
24) Chloroform-d	4.359	84	128833	4.669	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	93.400%		
26) 1,2-Dichloroethane-d4	5.040	65	55533	5.225	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	104.600%		
32) Benzene-d6	5.056	84	271523	4.798	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	96.000%		
36) 1,2-Dichloropropane-d6	6.076	67	81783	5.256	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	105.200%		
41) Toluene-d8	7.317	98	227341	4.467	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	89.400%		
43) trans-1,3-Dichloroprop...	7.629	79	17801	4.426	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	88.600%		
46) 2-Hexanone-d5	8.092	63	79931	52.172	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	104.340%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	51761	5.085	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	101.600%		
66) 1,2-Dichlorobenzene-d4	11.622	152	73864	5.250	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	105.000%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026511.D
Acq On : 23 Jun 2022 13:55
Operator : SY/MD
Sample : VV0623WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 24 00:51:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

