




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026517.D
 Acq On : 23 Jun 2022 16:20
 Operator : SY/MD
 Sample : N3425-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:02:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

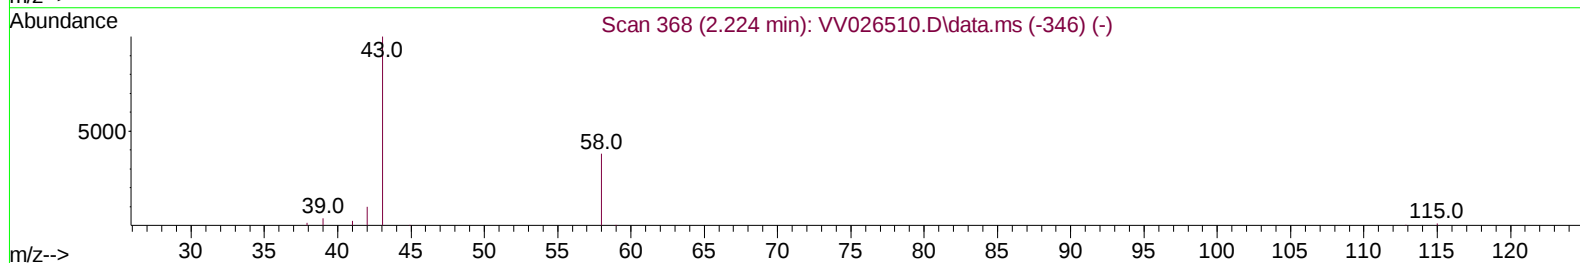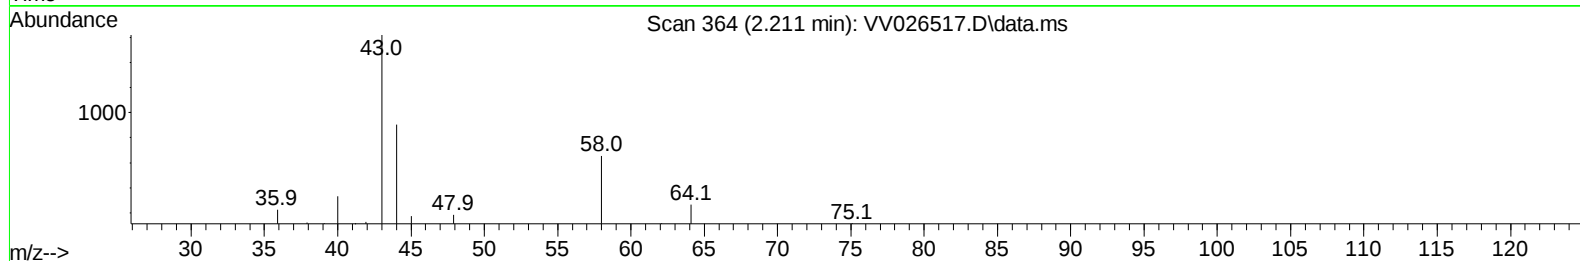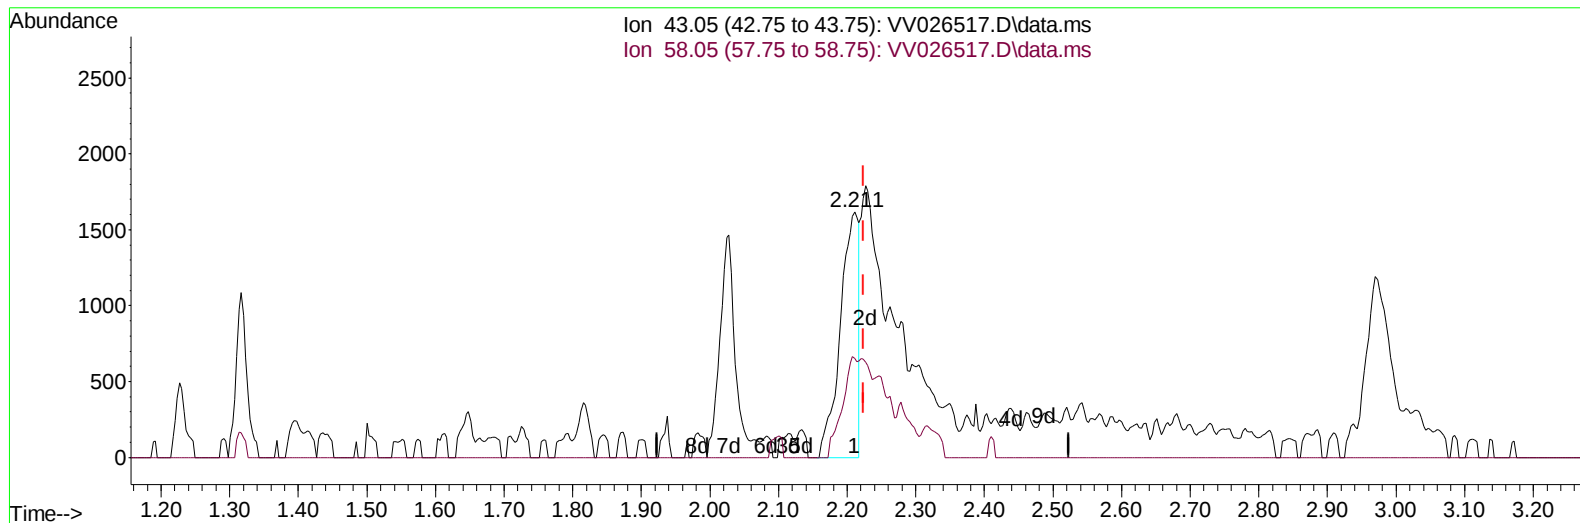

TIC: VV026517.D\data.ms

(13) Acetone (T)

2.211min (-0.013) 2.84 ug/L

response 3041

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	32.49
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026517.D
 Acq On : 23 Jun 2022 16:20
 Operator : SY/MD
 Sample : N3425-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:02:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

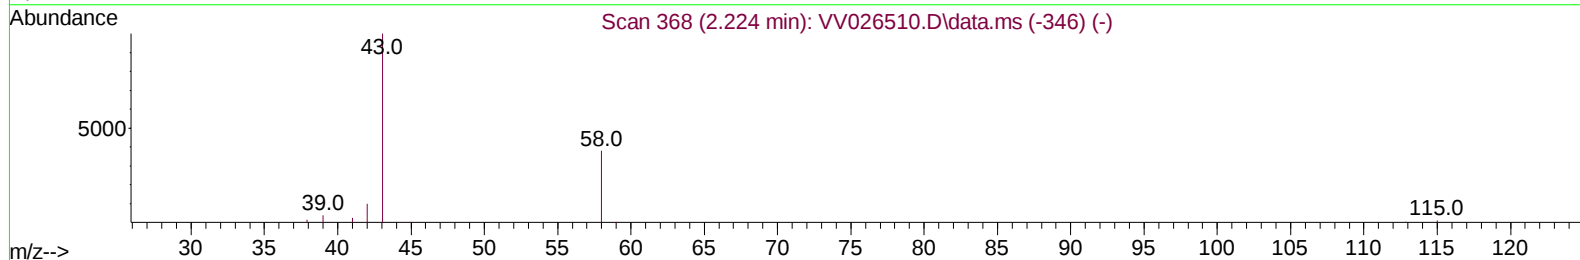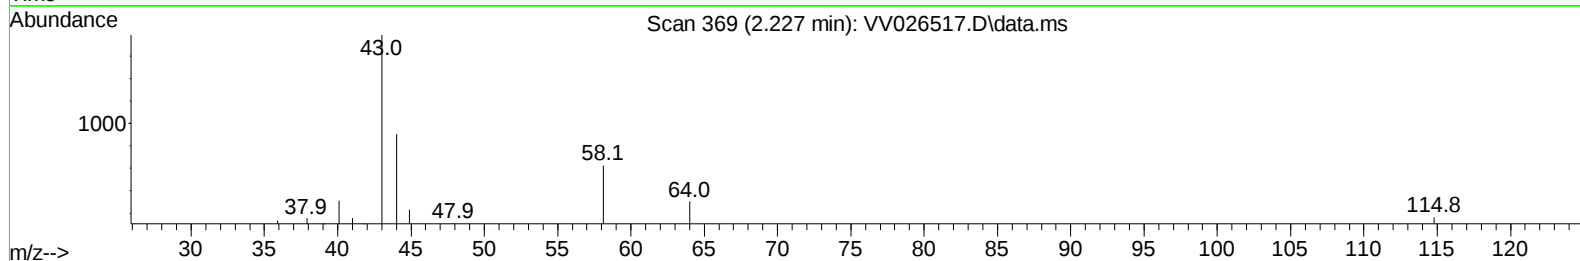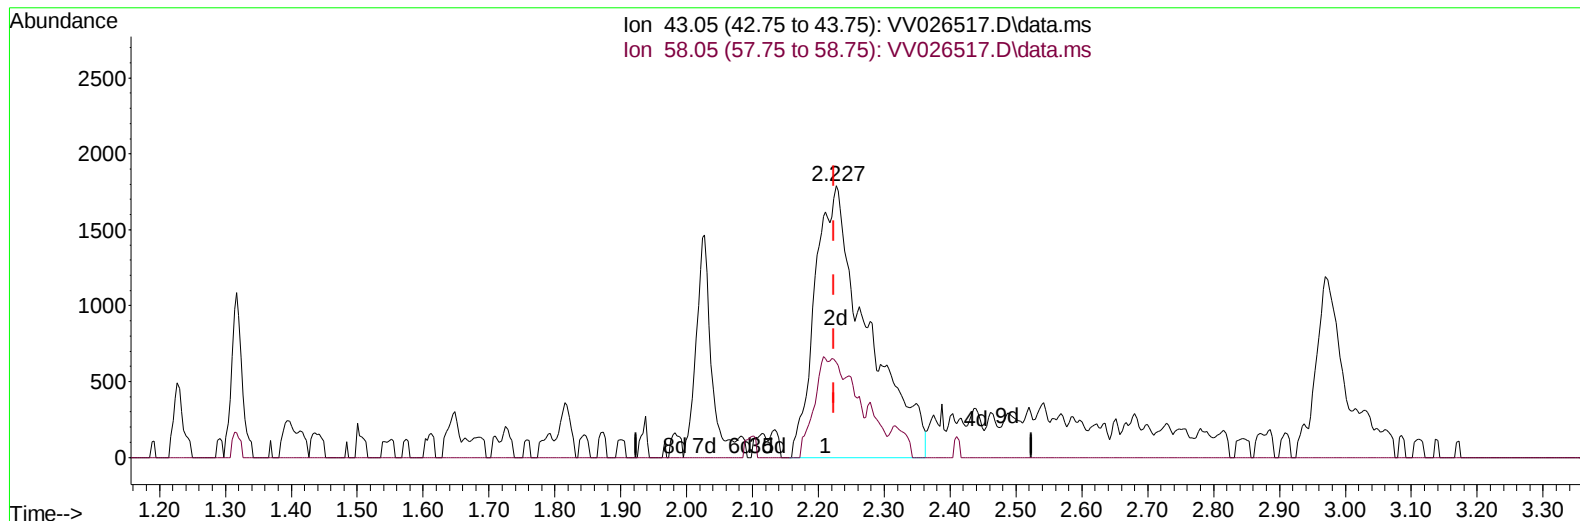

TIC: VV026517.D\data.ms

(13) Acetone (T)

2.227min (+ 0.003) 9.18 ug/L m

response 9828

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	10.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026517.D
 Acq On : 23 Jun 2022 16:20
 Operator : SY/MD
 Sample : N3425-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COALO

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:02:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	211101	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	199507	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	85141	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	84248	4.963	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	99.200%	
7) Chloroethane-d5	1.577	69	67947	4.982	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	99.600%	
11) 1,1-Dichloroethene-d2	2.118	63	114376	3.791	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	75.800%	
20) 2-Butanone-d5	3.925	46	103749	61.468	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	122.940%	
24) Chloroform-d	4.359	84	138653	4.996	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.000%	
26) 1,2-Dichloroethane-d4	5.040	65	56188	5.257	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.200%	
32) Benzene-d6	5.056	84	277148	4.836	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	96.800%	
36) 1,2-Dichloropropane-d6	6.072	67	80910	5.134	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	102.600%	
41) Toluene-d8	7.317	98	242113	4.698	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	94.000%	
43) trans-1,3-Dichloroprop...	7.629	79	17875	4.388	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	87.800%	
46) 2-Hexanone-d5	8.092	63	83874	54.061	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	108.120%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	53283	5.169	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	103.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	79060	5.611	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	112.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.227	43	9828m	9.178	ug/L	
14) Carbon disulfide	2.304	76	15326	0.407	ug/L	99
25) Chloroform	4.384	83	59505	2.130	ug/L	99
42) Toluene	7.397	91	14977	0.249	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026517.D
Acq On : 23 Jun 2022 16:20
Operator : SY/MD
Sample : N3425-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
COALO

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:02:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

