




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026518.D
 Acq On : 23 Jun 2022 16:44
 Operator : SY/MD
 Sample : N3425-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

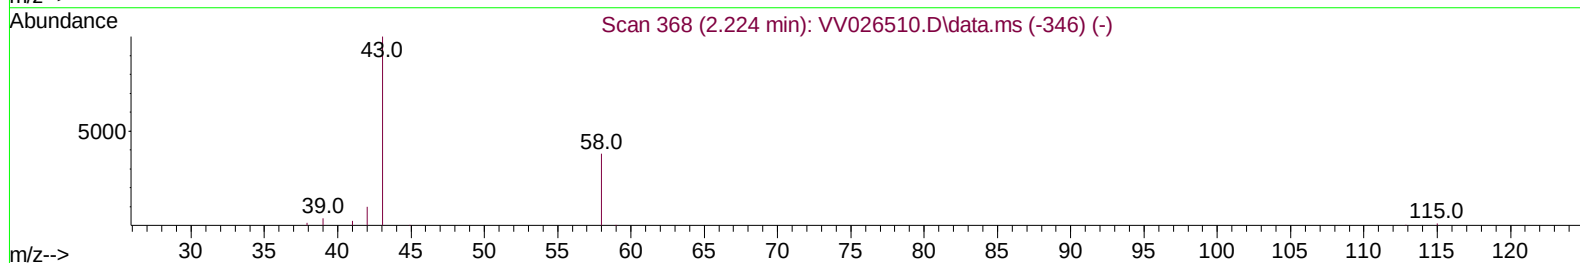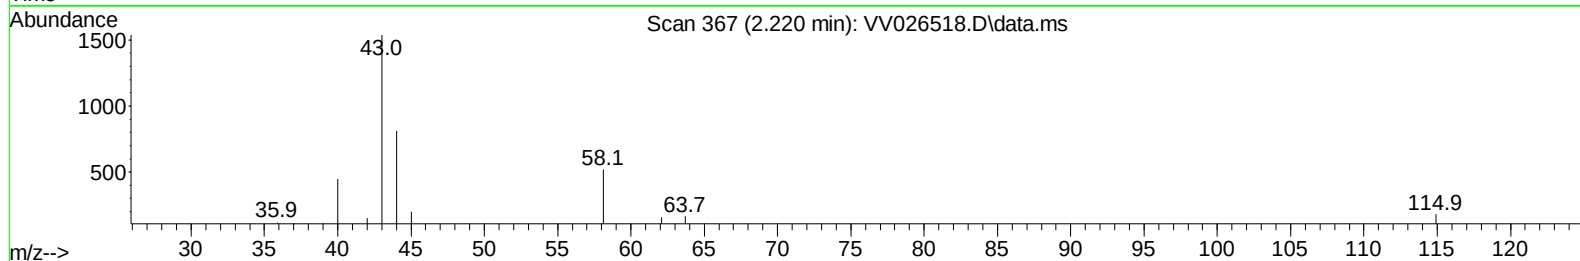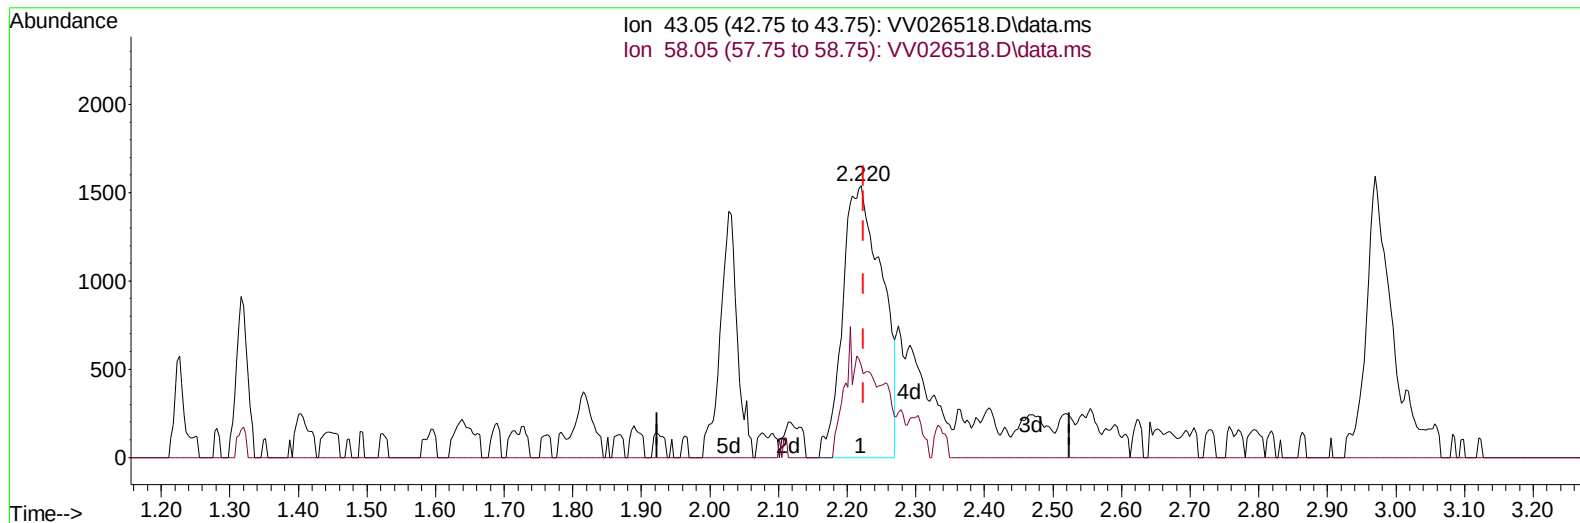

TIC: VV026518.D\data.ms

(13) Acetone (T)

2.220min (-0.003) 5.54 ug/L

response 6083

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	6.15
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026518.D
 Acq On : 23 Jun 2022 16:44
 Operator : SY/MD
 Sample : N3425-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

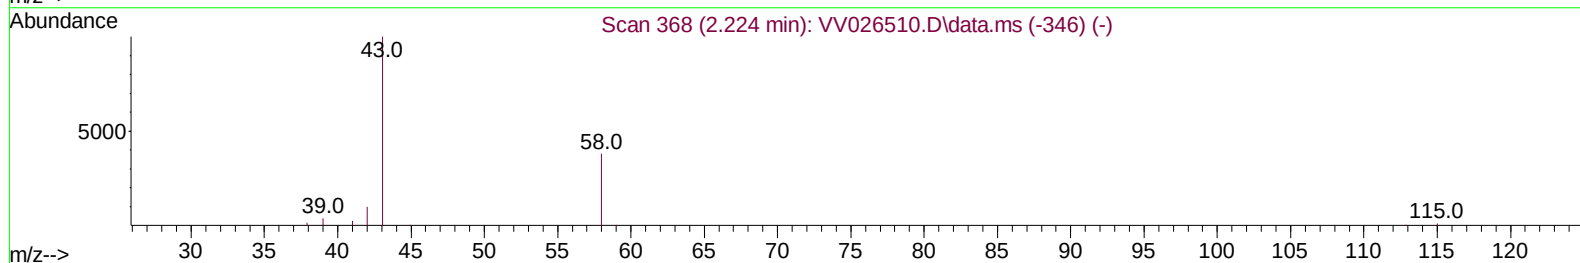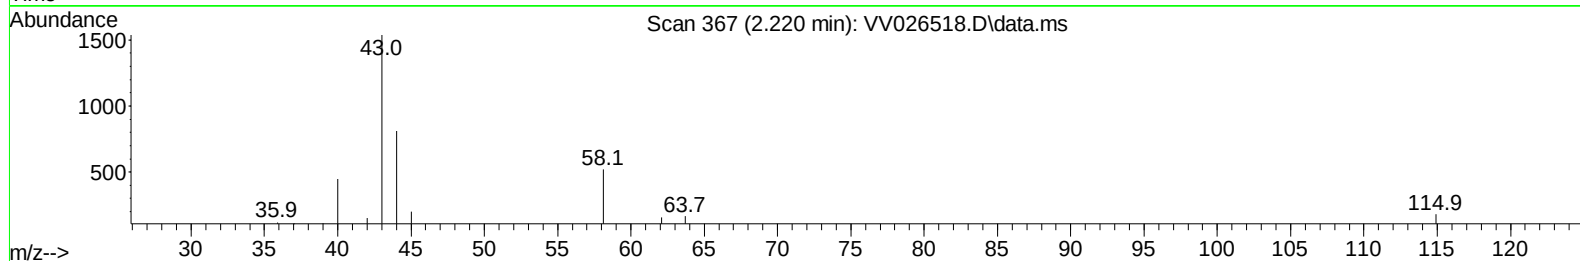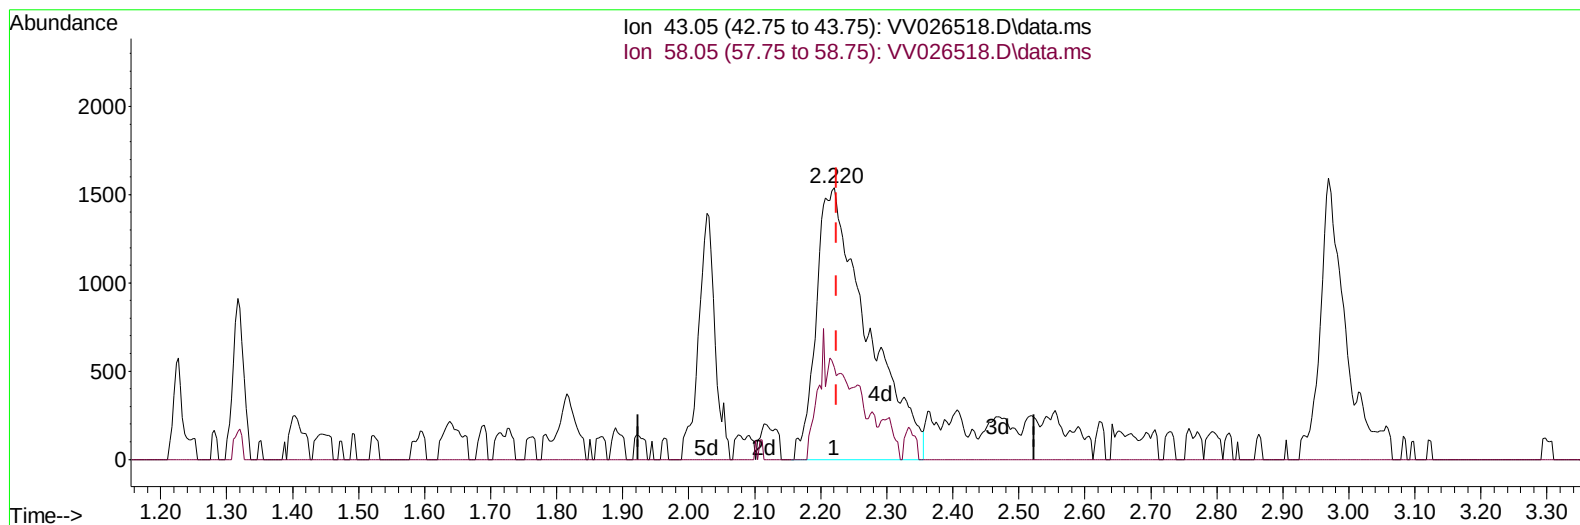

TIC: VV026518.D\data.ms

(13) Acetone (T)

2.220min (-0.003) 7.54 ug/L m

response 8289

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	4.51
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026518.D
 Acq On : 23 Jun 2022 16:44
 Operator : SY/MD
 Sample : N3425-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	216594	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	208523	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	91369	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	84316	4.841	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	96.800%		
7) Chloroethane-d5	1.577	69	69589	4.973	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	99.400%		
11) 1,1-Dichloroethene-d2	2.117	63	113943	3.681	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	73.600%		
20) 2-Butanone-d5	3.928	46	105880	61.140	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	122.280%		
24) Chloroform-d	4.359	84	139181	4.888	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.800%		
26) 1,2-Dichloroethane-d4	5.040	65	56377	5.140	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	102.800%		
32) Benzene-d6	5.056	84	276002	4.608	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	92.200%		
36) 1,2-Dichloropropane-d6	6.072	67	81790	4.966	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	99.400%		
41) Toluene-d8	7.317	98	241764	4.489	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	89.800%		
43) trans-1,3-Dichloroprop...	7.628	79	18093	4.250	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	85.000%		
46) 2-Hexanone-d5	8.091	63	82414	50.823	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	101.640%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	54030	5.015	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	100.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152	76819	5.080	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	101.600%		
Target Compounds						
13) Acetone	2.220	43	8289m	7.545	ug/L	
14) Carbon disulfide	2.304	76	14652	0.380	ug/L	99
25) Chloroform	4.387	83	58218	2.031	ug/L	96
42) Toluene	7.394	91	14354	0.228	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026518.D
Acq On : 23 Jun 2022 16:44
Operator : SY/MD
Sample : N3425-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL2

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

