




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026520.D
 Acq On : 23 Jun 2022 17:32
 Operator : SY/MD
 Sample : N3425-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

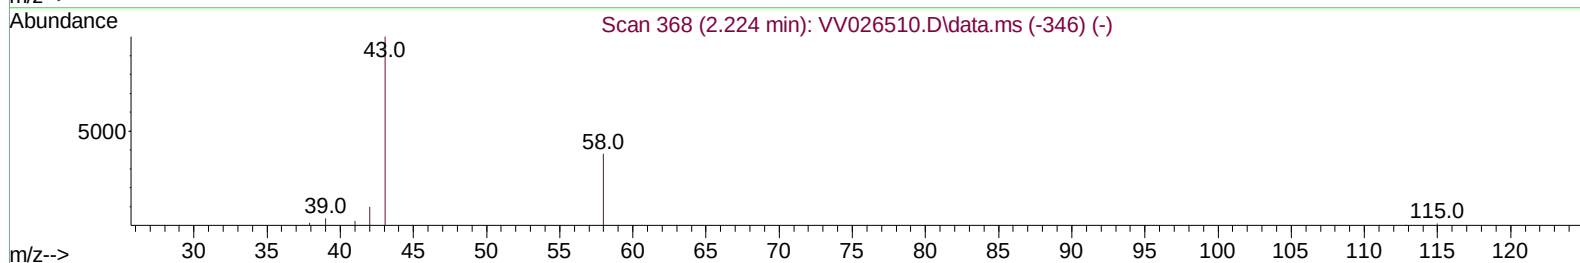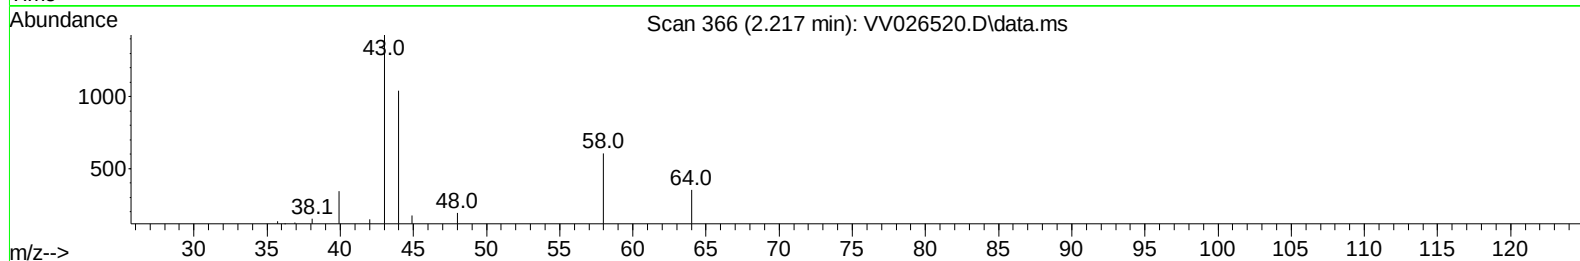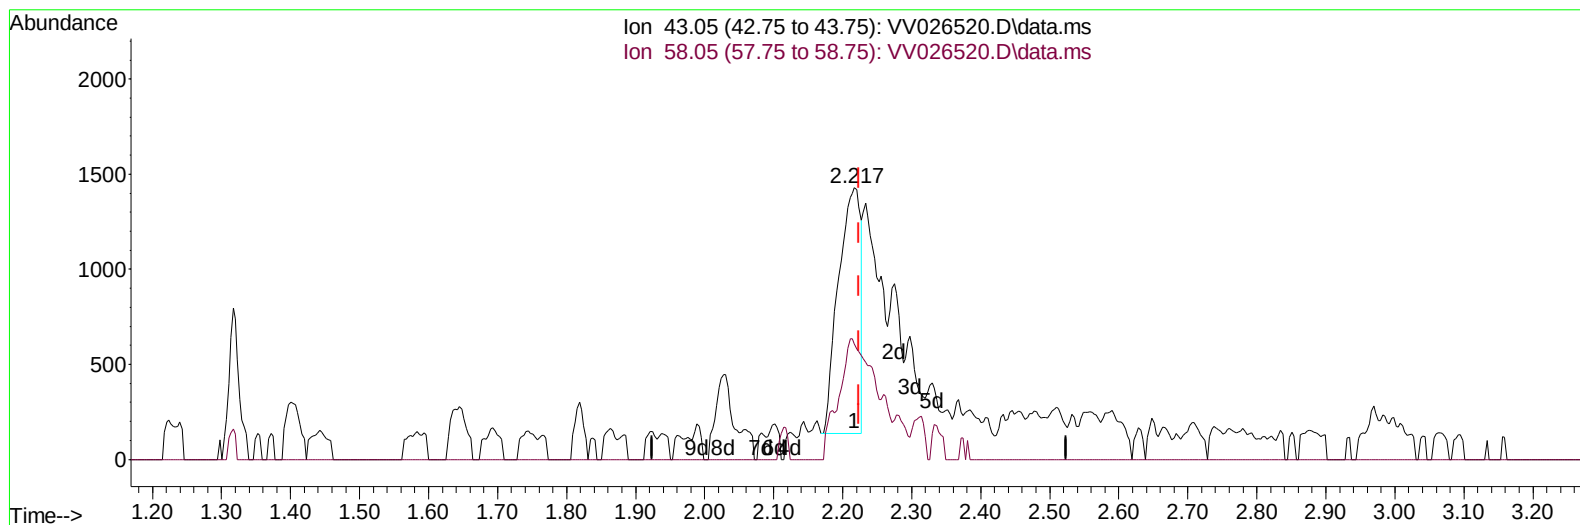

TIC: VV026520.D\data.ms

(13) Acetone (T)

2.217min (-0.007) 2.64 ug/L

response 2859

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	74.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026520.D
 Acq On : 23 Jun 2022 17:32
 Operator : SY/MD
 Sample : N3425-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

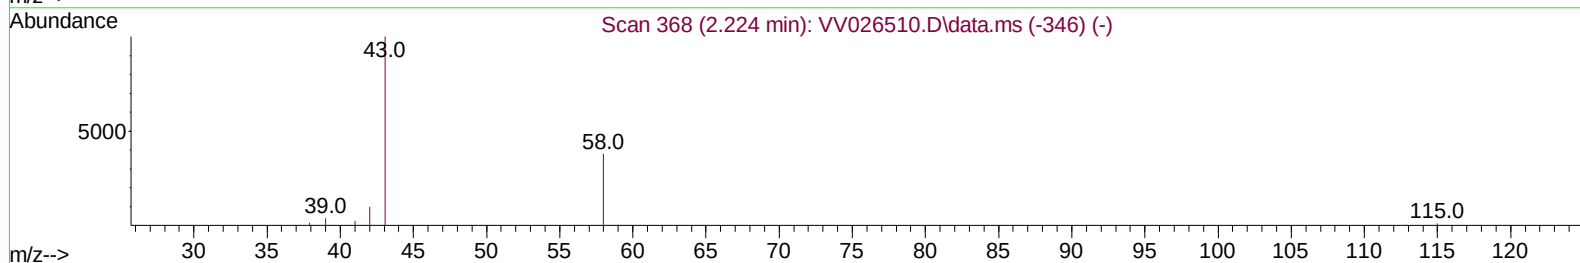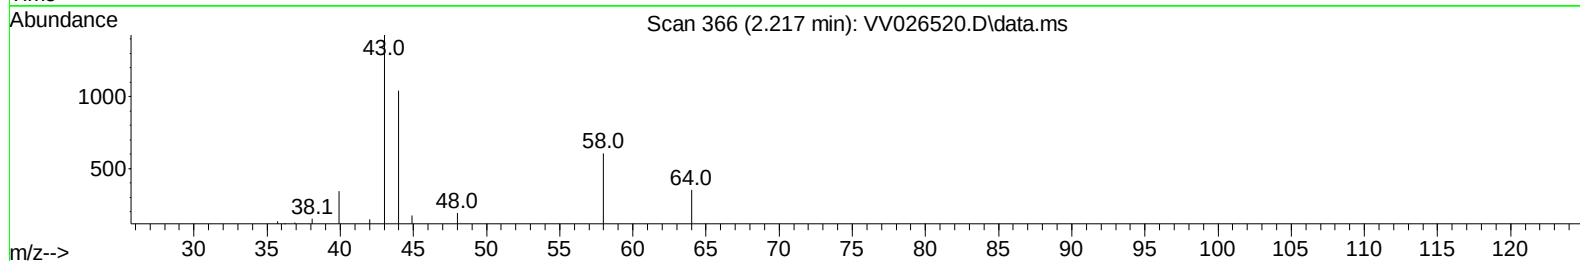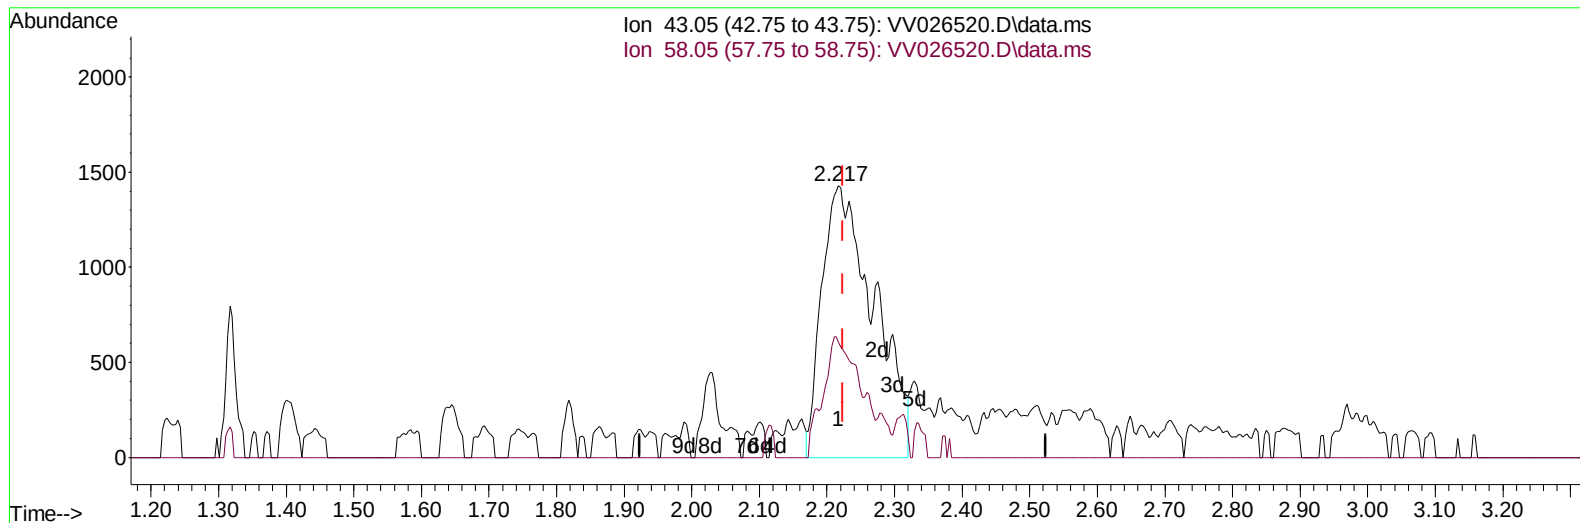

TIC: VV026520.D\data.ms

(13) Acetone (T)

2.217min (-0.007) 7.09 ug/L m

response 7660

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	27.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026520.D
 Acq On : 23 Jun 2022 17:32
 Operator : SY/MD
 Sample : N3425-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	213141	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	202480	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	85789	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	85584	4.993	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	99.800%		
7) Chloroethane-d5	1.577	69	68432	4.969	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	99.400%		
11) 1,1-Dichloroethene-d2	2.117	63	117196	3.848	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	77.000%		
20) 2-Butanone-d5	3.931	46	97219	57.048	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	114.100%		
24) Chloroform-d	4.358	84	139527	4.979	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	99.600%		
26) 1,2-Dichloroethane-d4	5.040	65	57969	5.371	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	107.400%		
32) Benzene-d6	5.056	84	275302	4.734	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	94.600%		
36) 1,2-Dichloropropane-d6	6.075	67	81391	5.089	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	101.800%		
41) Toluene-d8	7.317	98	237402	4.539	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.800%		
43) trans-1,3-Dichloroprop...	7.628	79	17788	4.303	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	86.000%		
46) 2-Hexanone-d5	8.091	63	77300	49.092	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	98.180%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	53912	5.153	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	103.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	76607	5.396	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	108.000%		
Target Compounds						
					Qvalue	
13) Acetone	2.217	43	7660m	7.085	ug/L	
14) Carbon disulfide	2.304	76	6430	0.169	ug/L #	93
25) Chloroform	4.391	83	13864	0.491	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026520.D
Acq On : 23 Jun 2022 17:32
Operator : SY/MD
Sample : N3425-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
COAL5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:03:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

