




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026522.D
 Acq On : 23 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3401-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

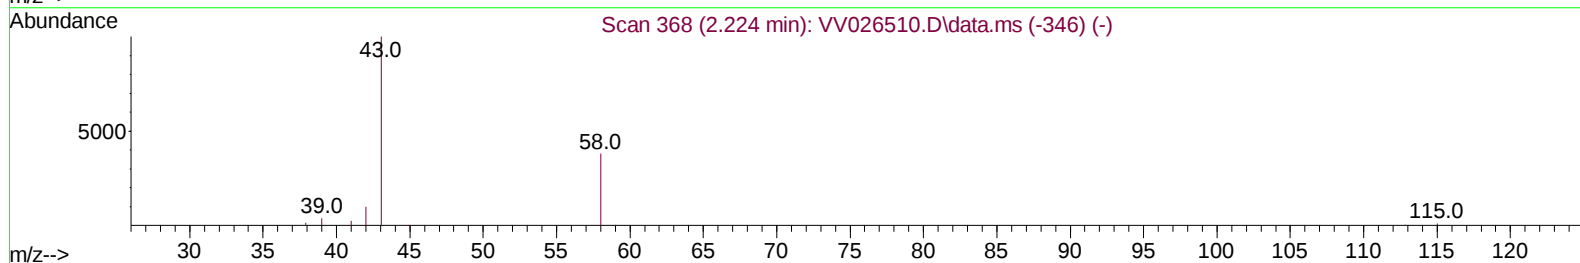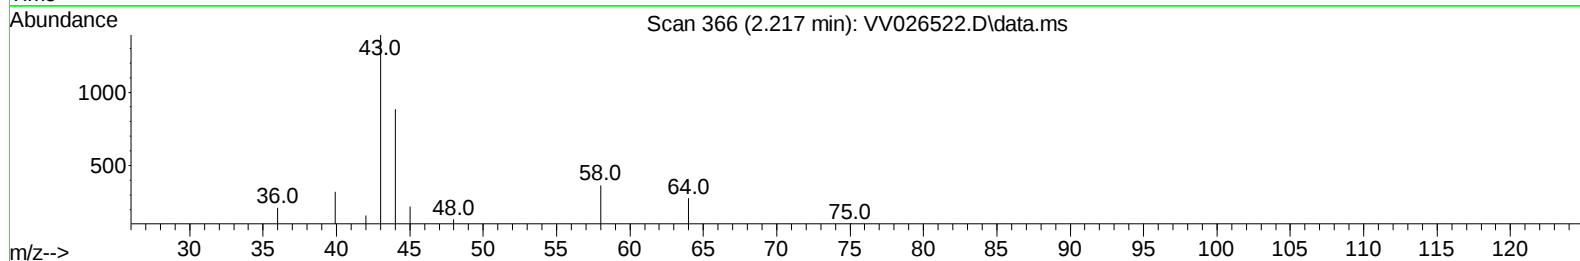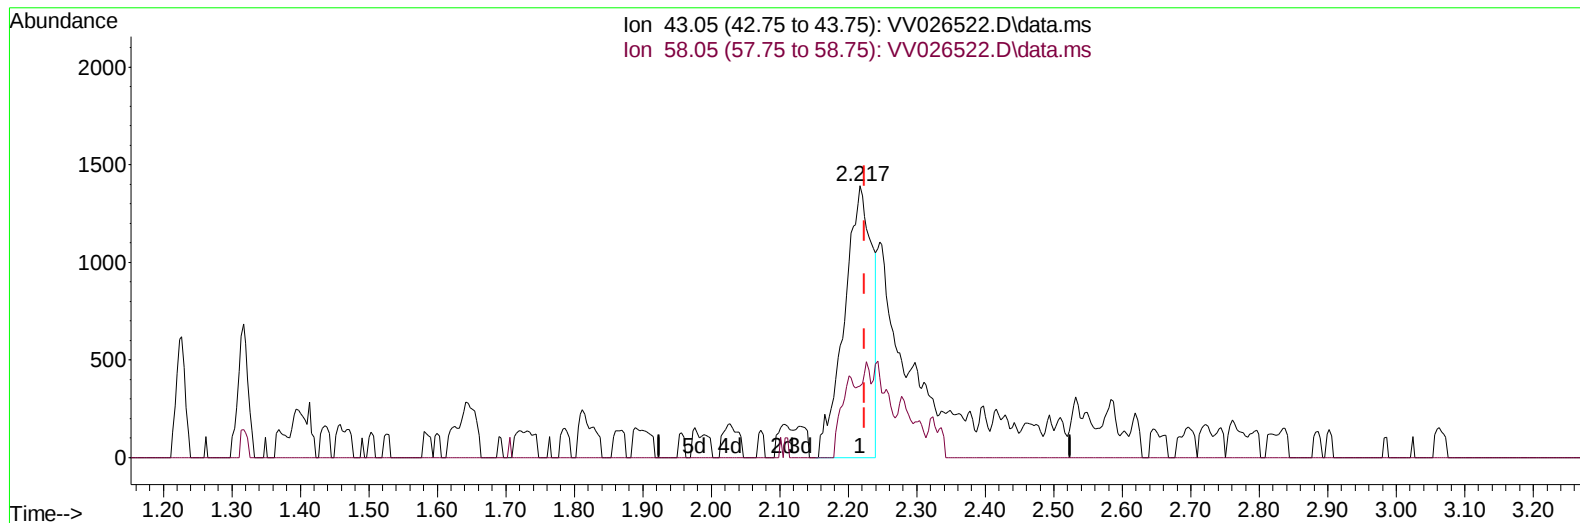

TIC: VV026522.D\data.ms

(13) Acetone (T)

2.217min (-0.007) 3.78 ug/L

response 3921

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	8.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026522.D
 Acq On : 23 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3401-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

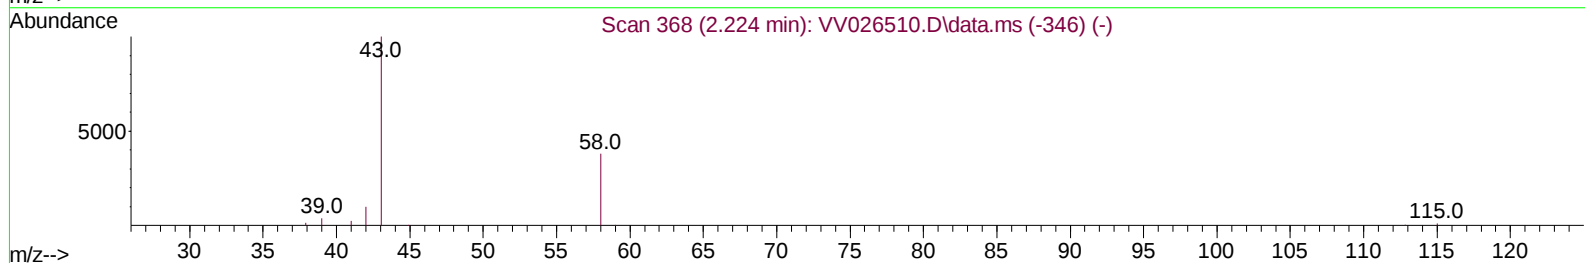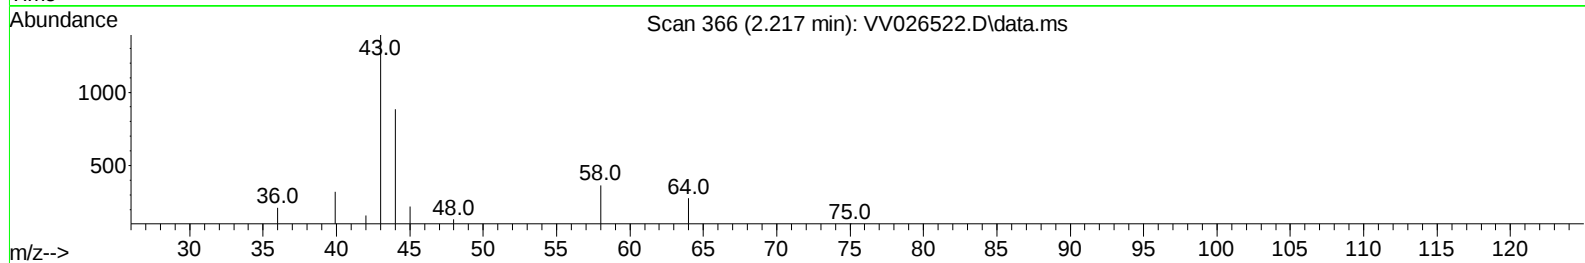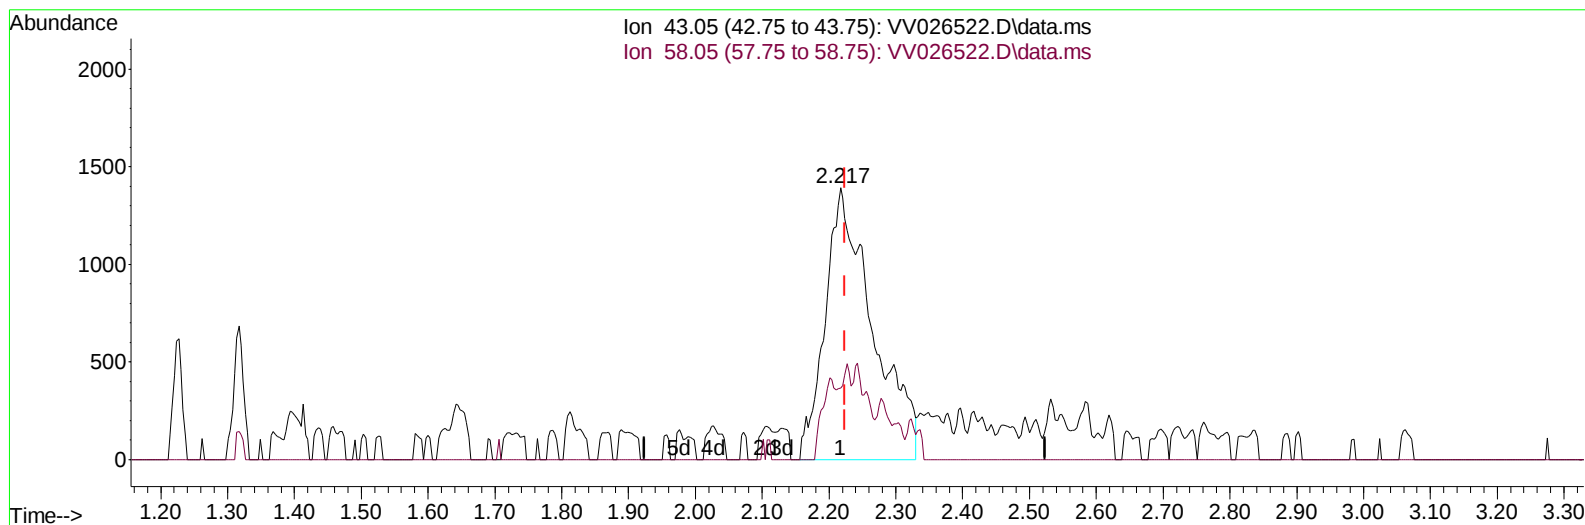

TIC: VV026522.D\data.ms

(13) Acetone (T)

2.217min (-0.007) 6.63 ug/L m

response 6871

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	4.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026522.D
 Acq On : 23 Jun 2022 18:20
 Operator : SY/MD
 Sample : N3401-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG0

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	204447	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	194881	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	81482	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	80916	4.921	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	98.400%	
7) Chloroethane-d5	1.577	69	65202	4.936	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	98.800%	
11) 1,1-Dichloroethene-d2	2.117	63	112056	3.835	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	76.800%	
20) 2-Butanone-d5	3.921	46	99572	60.913	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	121.820%	
24) Chloroform-d	4.358	84	130816	4.867	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	5.043	65	54810	5.294	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.800%	
32) Benzene-d6	5.056	84	265306	4.740	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.800%	
36) 1,2-Dichloropropane-d6	6.075	67	77912	5.062	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	101.200%	
41) Toluene-d8	7.317	98	218326	4.337	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...	7.628	79	16683	4.193	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	83.800%	
46) 2-Hexanone-d5	8.091	63	73921	48.776	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	97.560%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	50126	4.978	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	99.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	71623	5.312	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	106.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.217	43	6871m	6.626	ug/L	
14) Carbon disulfide	2.304	76	13356	0.367	ug/L	99
53) m,p-Xylene	9.149	106	2373	0.100	ug/L	77
54) o-Xylene	9.554	106	1226	0.055	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026522.D
Acq On : 23 Jun 2022 18:20
Operator : SY/MD
Sample : N3401-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0AG0

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

