




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026525.D
 Acq On : 23 Jun 2022 19:32
 Operator : SY/MD
 Sample : N3400-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

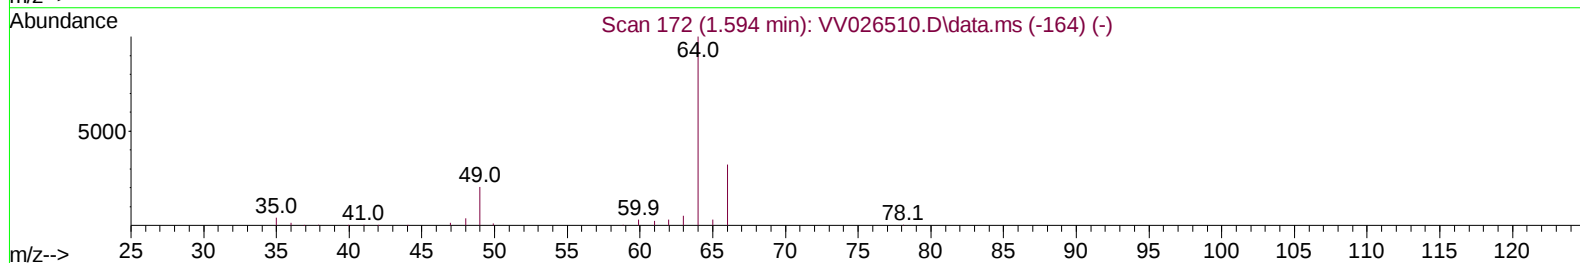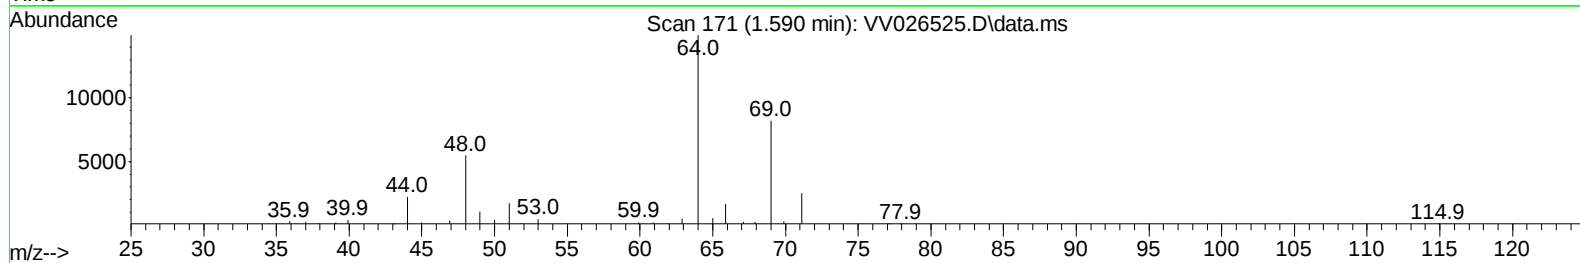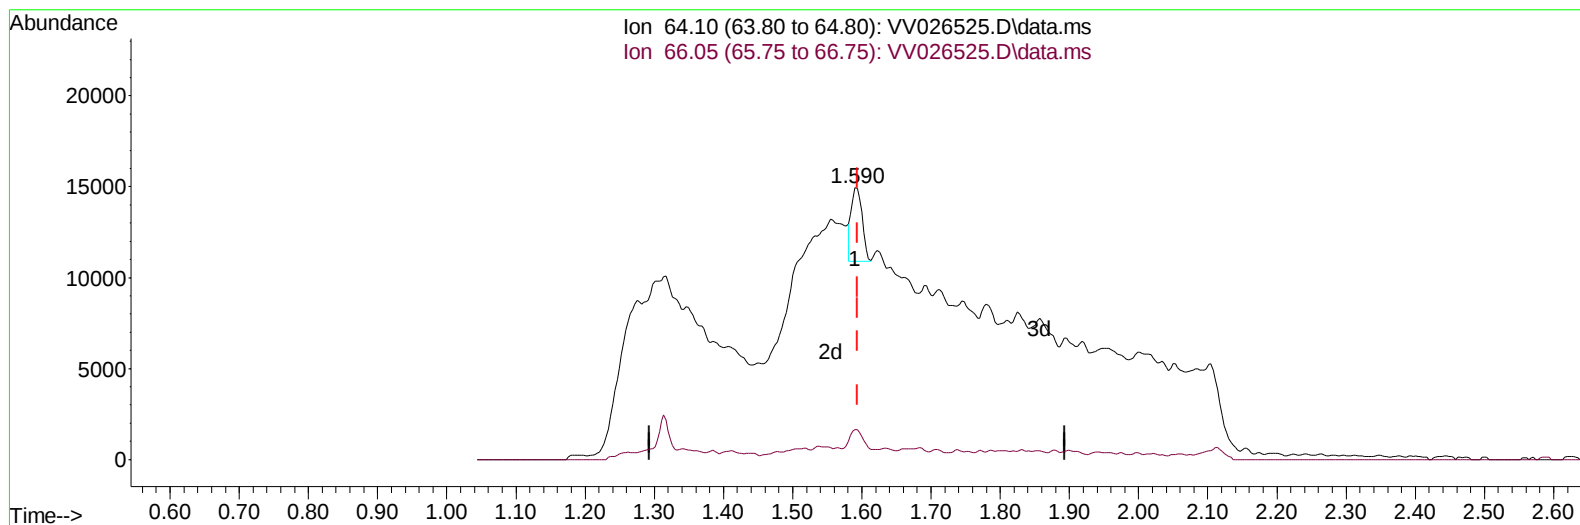

TIC: VV026525.D\data.ms

(8) Chloroethane (T)

1.590min (-0.003) 0.33 ug/L m

response 4391

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	28.60	11.05#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026525.D
 Acq On : 23 Jun 2022 19:32
 Operator : SY/MD
 Sample : N3400-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.622	114		223222	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		201663	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		95403	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.314	65		79654	4.437	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	88.800%		
7) Chloroethane-d5	1.574	69		65930	4.572	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	91.400%		
11) 1,1-Dichloroethene-d2	2.114	63		108796	3.411	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	68.200%		
20) 2-Butanone-d5	3.924	46		93492	52.383	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	104.760%		
24) Chloroform-d	4.352	84		129120	4.400	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	88.000%		
26) 1,2-Dichloroethane-d4	5.040	65		52967	4.686	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	93.800%		
32) Benzene-d6	5.053	84		273986	4.730	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	94.600%		
36) 1,2-Dichloropropane-d6	6.072	67		77136	4.843	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	96.800%		
41) Toluene-d8	7.317	98		230201	4.419	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	88.400%		
43) trans-1,3-Dichloroprop...	7.628	79		17381	4.221	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	84.400%		
46) 2-Hexanone-d5	8.091	63		78703	50.185	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	100.380%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84		50638	4.860	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	97.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152		86633	5.487	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	109.800%		
Target Compounds							
						Qvalue	
8) Chloroethane	1.590	64		4391m	0.326	ug/L	
19) 1,1-Dichloroethane	3.201	63		3666	0.133	ug/L	97
30) Cyclohexane	4.683	56		74122	3.773	ug/L	97
33) Benzene	5.104	78		237245	4.029	ug/L	100
35) Methylcyclohexane	6.133	83		97946	4.277	ug/L	95
51) Chlorobenzene	8.886	112		5407	0.136	ug/L	95
52) Ethylbenzene	9.018	91		10326	0.164	ug/L	99
53) m,p-Xylene	9.136	106		155352	6.335	ug/L	97
54) o-Xylene	9.548	106		3038	0.132	ug/L	93
60) Isopropylbenzene	9.931	105		204076	3.468	ug/L	99
63) 1,2,4-Trimethylbenzene	10.915	105		57906	1.263	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026525.D
Acq On : 23 Jun 2022 19:32
Operator : SY/MD
Sample : N3400-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:04:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

