




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026528.D
 Acq On : 23 Jun 2022 20:43
 Operator : SY/MD
 Sample : N3400-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

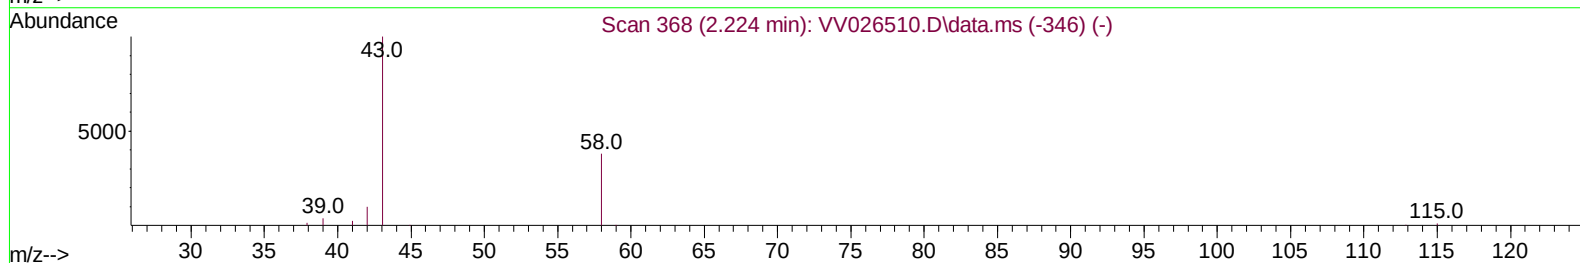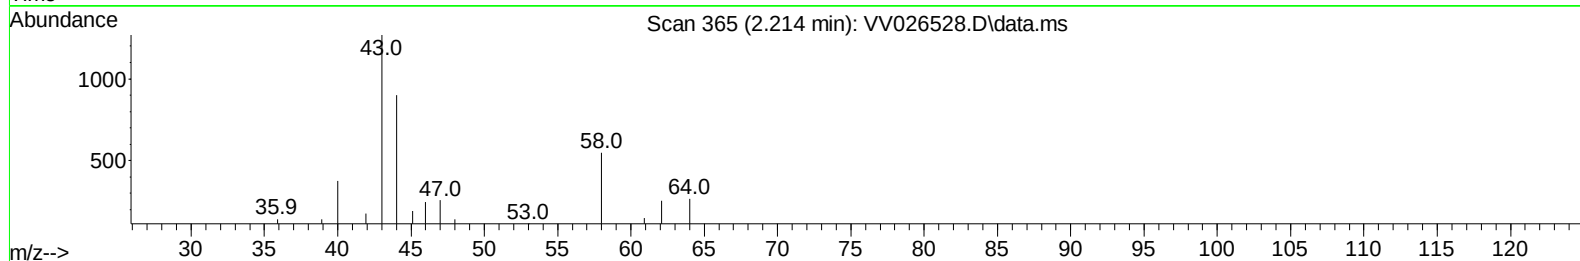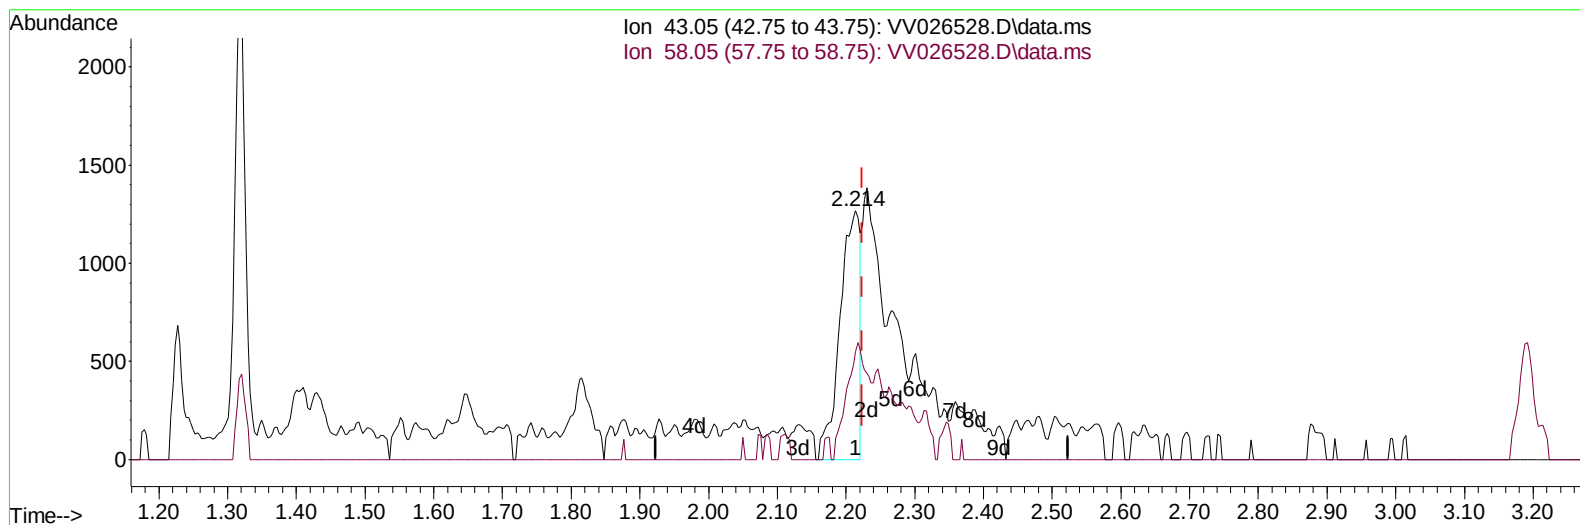

TIC: VV026528.D\data.ms

(13) Acetone (T)

2.214min (-0.010) 2.85 ug/L

response 2548

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	52.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026528.D
 Acq On : 23 Jun 2022 20:43
 Operator : SY/MD
 Sample : N3400-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

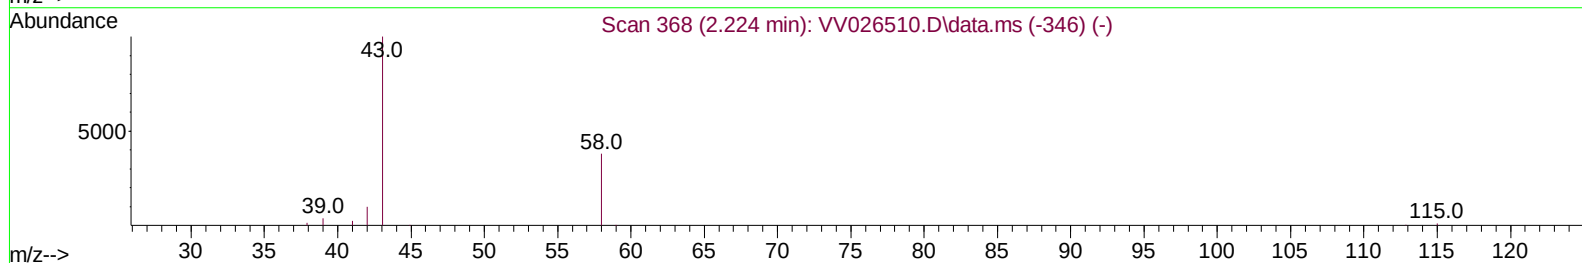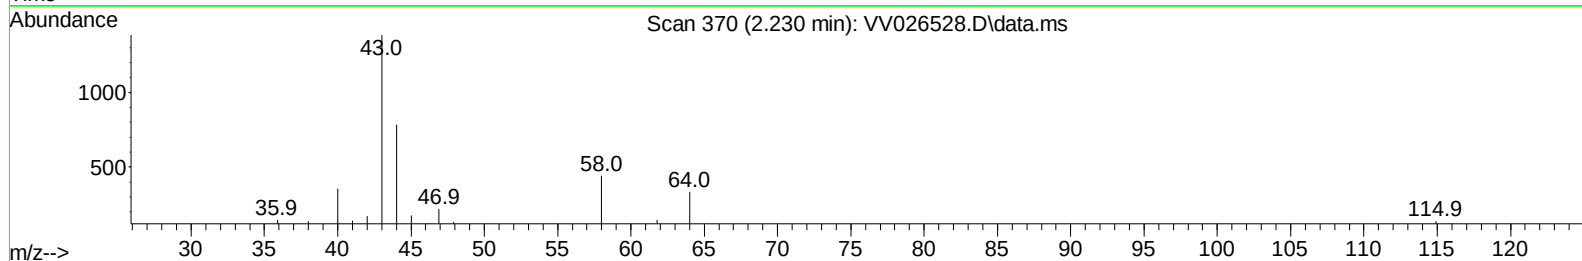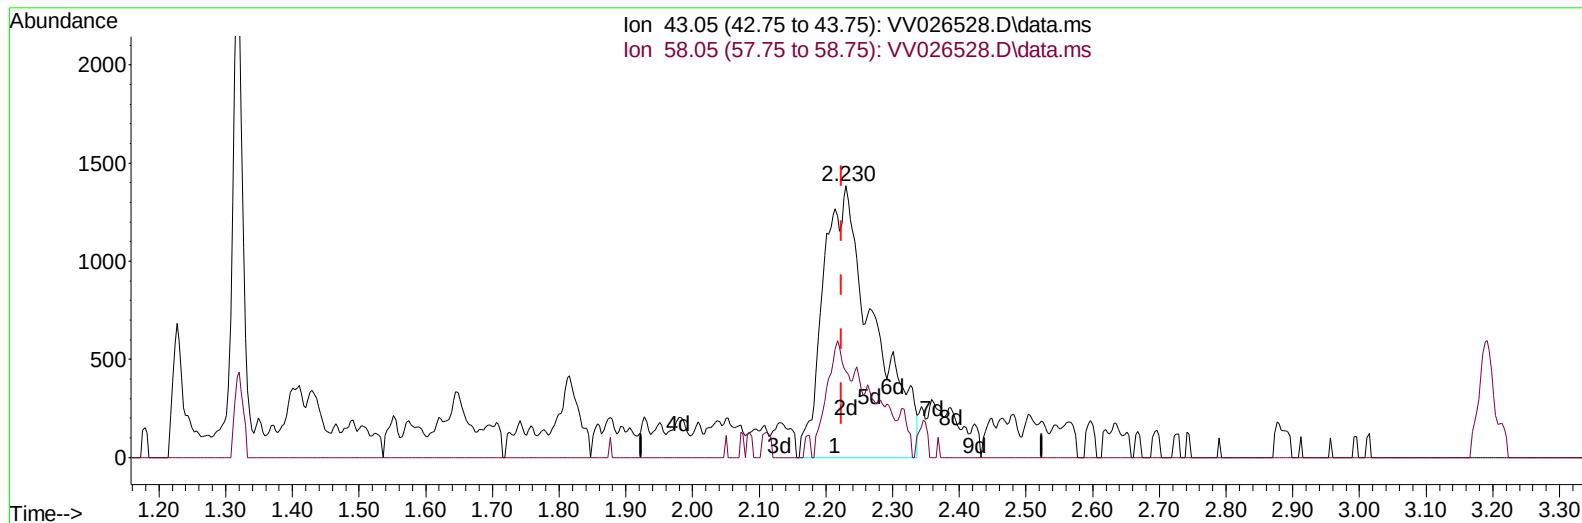

TIC: VV026528.D\data.ms

(13) Acetone (T)

2.230min (+ 0.006) 8.12 ug/L m

response 7251

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	18.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026528.D
 Acq On : 23 Jun 2022 20:43
 Operator : SY/MD
 Sample : N3400-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:05:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	176003	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	168533	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72774	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	54236	3.832	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	76.600%	
7) Chloroethane-d5	1.577	69	49276	4.333	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	86.600%	
11) 1,1-Dichloroethene-d2	2.118	63	80120	3.186	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	63.800%	
20) 2-Butanone-d5	3.928	46	91047	64.699	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	129.400%	
24) Chloroform-d	4.359	84	116775	5.047	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	101.000%	
26) 1,2-Dichloroethane-d4	5.043	65	48022	5.388	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	107.800%	
32) Benzene-d6	5.060	84	228634	4.723	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	6.072	67	69077	5.189	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	103.800%	
41) Toluene-d8	7.317	98	187725	4.312	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	86.200%	
43) trans-1,3-Dichloroprop...	7.632	79	11701	3.401	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	68.000%	
46) 2-Hexanone-d5	8.092	63	70088	53.477	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	106.960%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46698	5.362	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	107.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	67063	5.569	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	111.400%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.253	50	5065	0.346	ug/L	95
8) Chloroethane	1.597	64	3171	0.299	ug/L #	65
13) Acetone	2.230	43	7251m	8.122	ug/L	
14) Carbon disulfide	2.307	76	12567	0.401	ug/L	98
16) Methylene chloride	2.516	84	2463	0.195	ug/L	82
33) Benzene	5.121	78	4383	0.089	ug/L	100
42) Toluene	7.394	91	54529	1.073	ug/L	96
51) Chlorobenzene	8.879	112	1498	0.045	ug/L #	57
52) Ethylbenzene	9.021	91	5907	0.112	ug/L	92
53) m,p-Xylene	9.140	106	6322	0.308	ug/L	85
54) o-Xylene	9.548	106	4995	0.260	ug/L	94
62) 1,3,5-Trimethylbenzene	10.545	105	2261	0.064	ug/L	96
63) 1,2,4-Trimethylbenzene	10.918	105	9425	0.269	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026528.D
Acq On : 23 Jun 2022 20:43
Operator : SY/MD
Sample : N3400-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:05:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

