




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026532.D
 Acq On : 23 Jun 2022 22:19
 Operator : SY/MD
 Sample : N3374-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:06:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

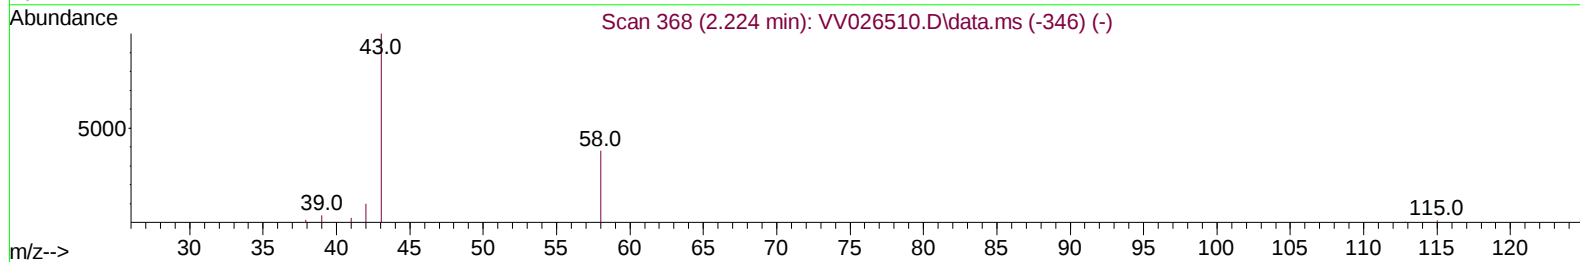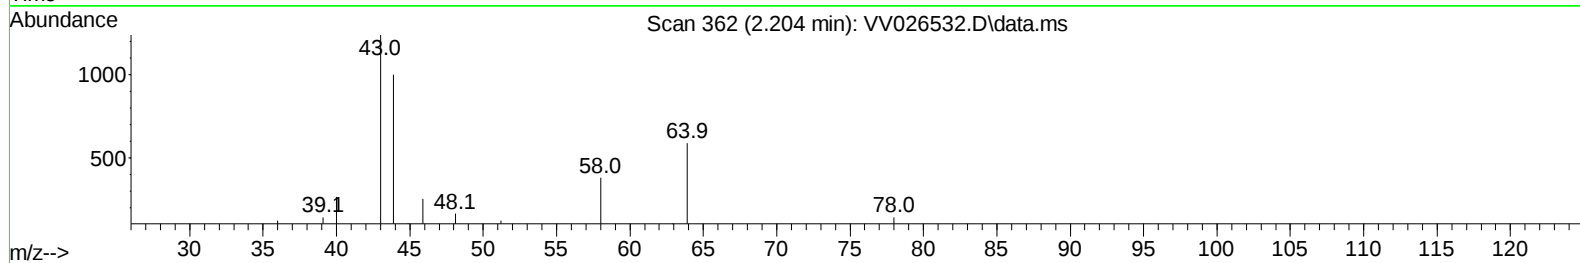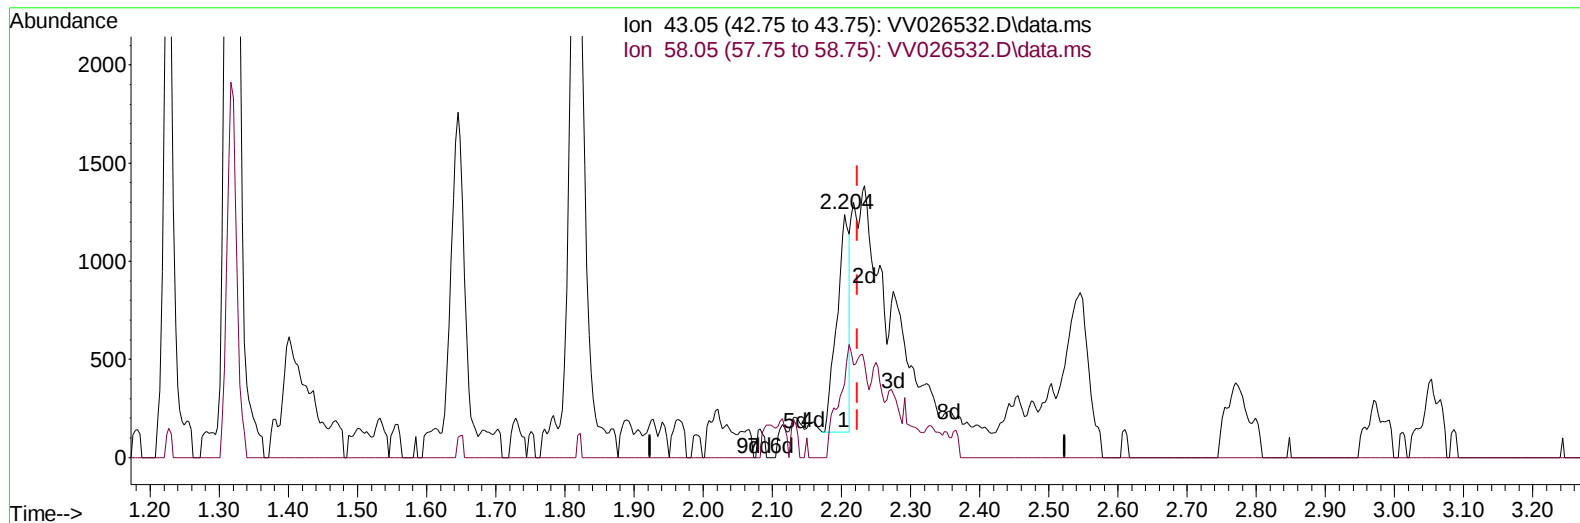

TIC: VV026532.D\data.ms

(13) Acetone (T)

2.204min (-0.019) 1.45 ug/L

response 1374

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	65.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026532.D
 Acq On : 23 Jun 2022 22:19
 Operator : SY/MD
 Sample : N3374-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:06:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

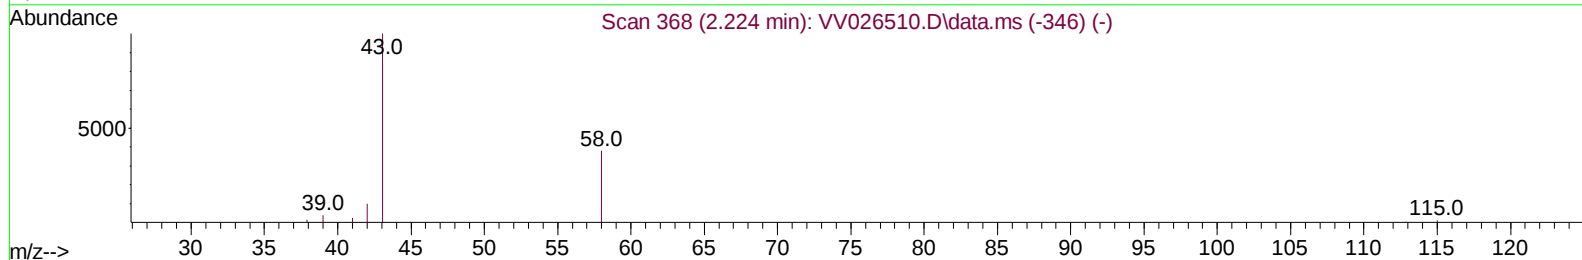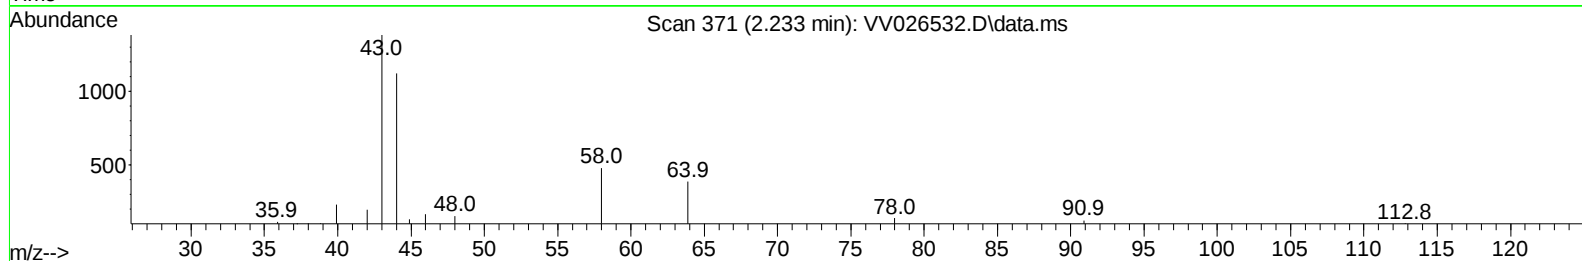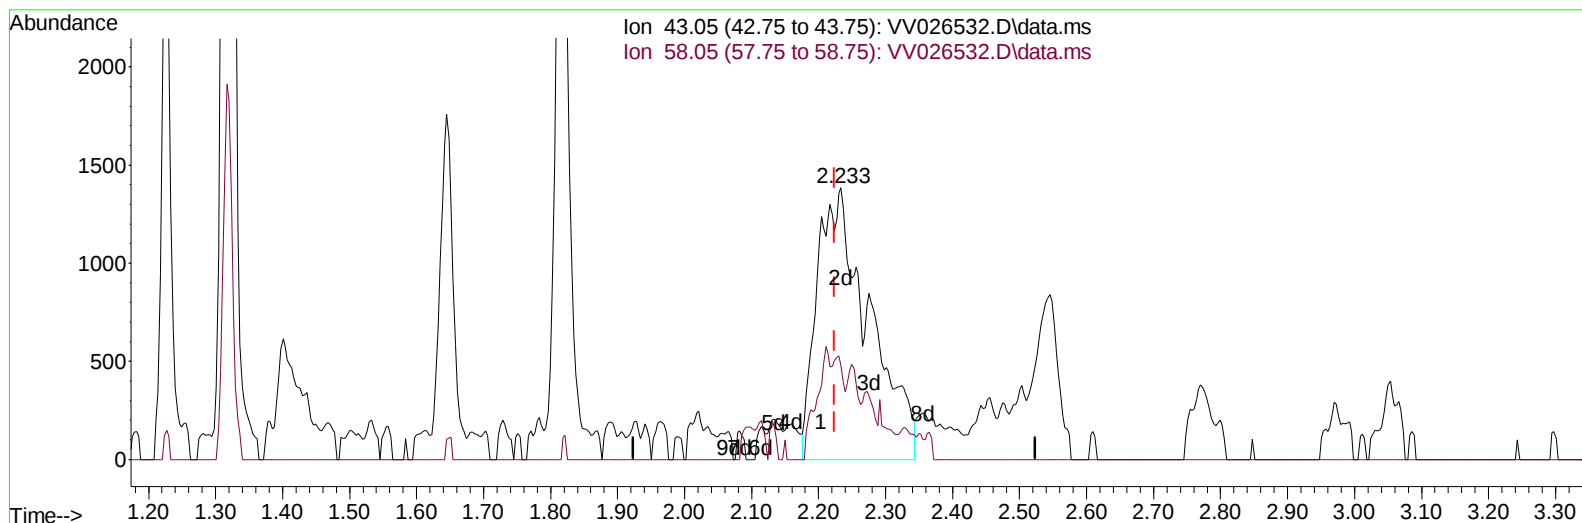

TIC: VV026532.D\data.ms

(13) Acetone (T)

2.233min (+ 0.010) 7.83 ug/L m

response 7427

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	12.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026532.D
 Acq On : 23 Jun 2022 22:19
 Operator : SY/MD
 Sample : N3374-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4T5

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:06:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	187094	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	177141	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75867	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	53324	3.544	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	70.800%	
7) Chloroethane-d5	1.577	69	49992	4.136	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	82.800%	
11) 1,1-Dichloroethene-d2	2.118	63	76380	2.857	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	57.200%#	
20) 2-Butanone-d5	3.928	46	94793	63.368	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	126.740%	
24) Chloroform-d	4.359	84	116819	4.749	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.000%	
26) 1,2-Dichloroethane-d4	5.040	65	50088	5.287	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.800%	
32) Benzene-d6	5.056	84	227531	4.472	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	89.400%	
36) 1,2-Dichloropropane-d6	6.076	67	70924	5.069	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	101.400%	
41) Toluene-d8	7.320	98	185476	4.054	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.000%	
43) trans-1,3-Dichloroprop...	7.632	79	10837	2.996	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	60.000%	
46) 2-Hexanone-d5	8.092	63	72589	52.694	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	105.380%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	47532	5.193	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	64807	5.162	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	103.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.233	43	7427m	7.826	ug/L	
14) Carbon disulfide	2.304	76	17700	0.531	ug/L	99
33) Benzene	5.114	78	12385	0.239	ug/L	100
52) Ethylbenzene	9.018	91	26075	0.472	ug/L	95
53) m,p-Xylene	9.140	106	19665	0.913	ug/L	94
63) 1,2,4-Trimethylbenzene	10.918	105	3086	0.085	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026532.D
Acq On : 23 Jun 2022 22:19
Operator : SY/MD
Sample : N3374-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4T5

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 24 02:06:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

