




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026533.D
 Acq On : 23 Jun 2022 22:43
 Operator : SY/MD
 Sample : N3374-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4W0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 24 02:06:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

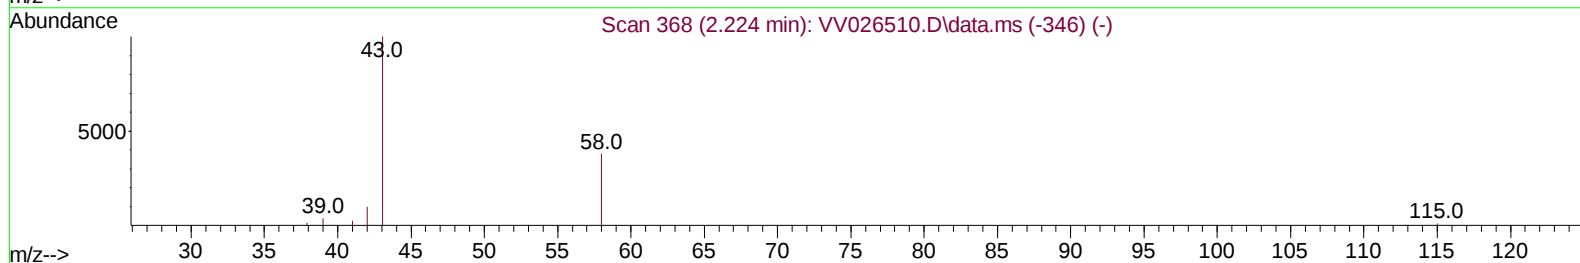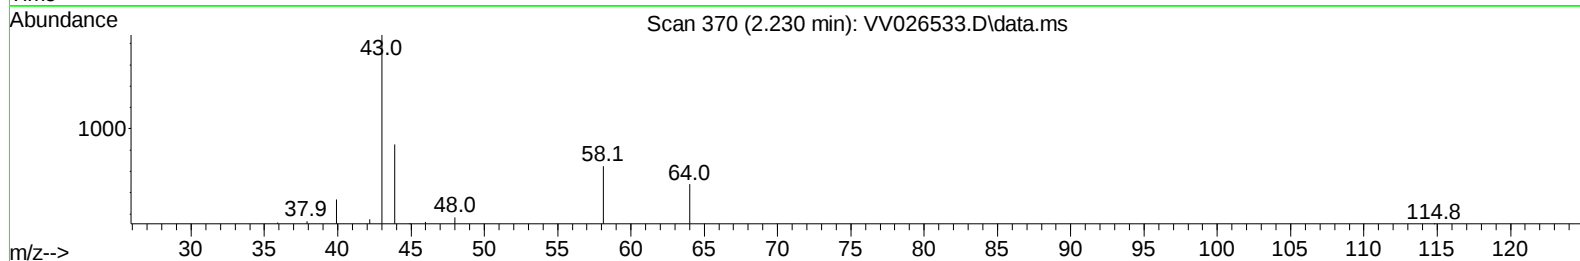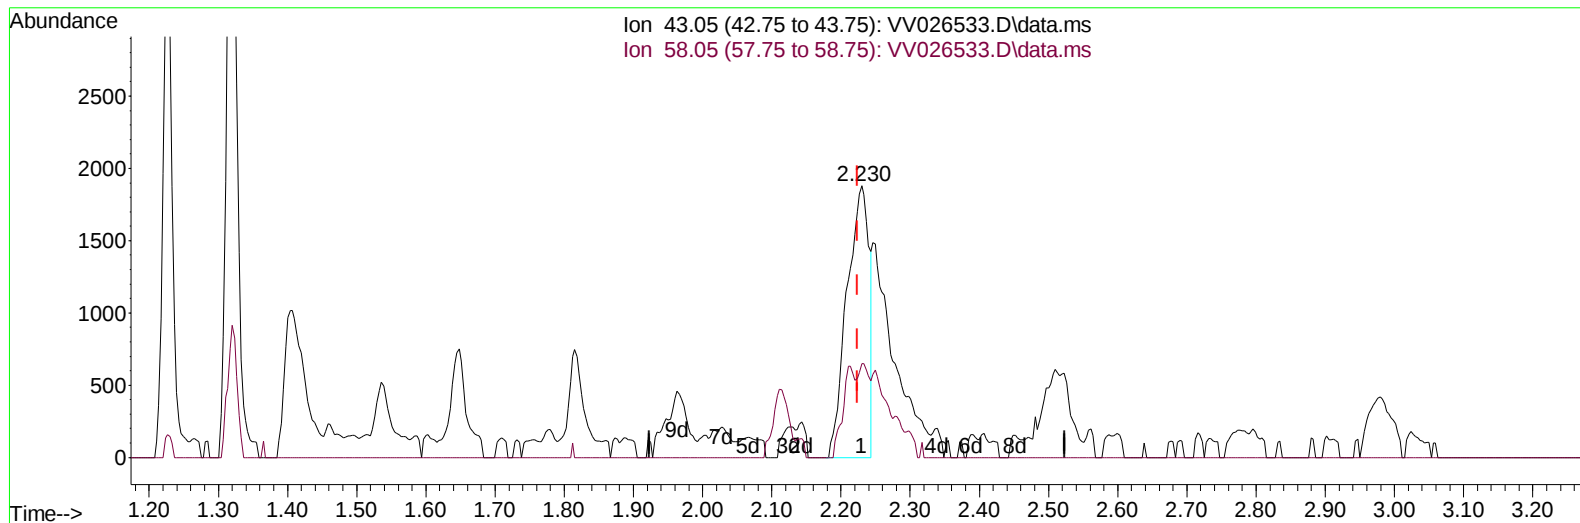

TIC: VV026533.D\data.ms

(13) Acetone (T)

2.230min (+ 0.006) 4.53 ug/L

response 4148

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	4.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026533.D
 Acq On : 23 Jun 2022 22:43
 Operator : SY/MD
 Sample : N3374-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4W0

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:06:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

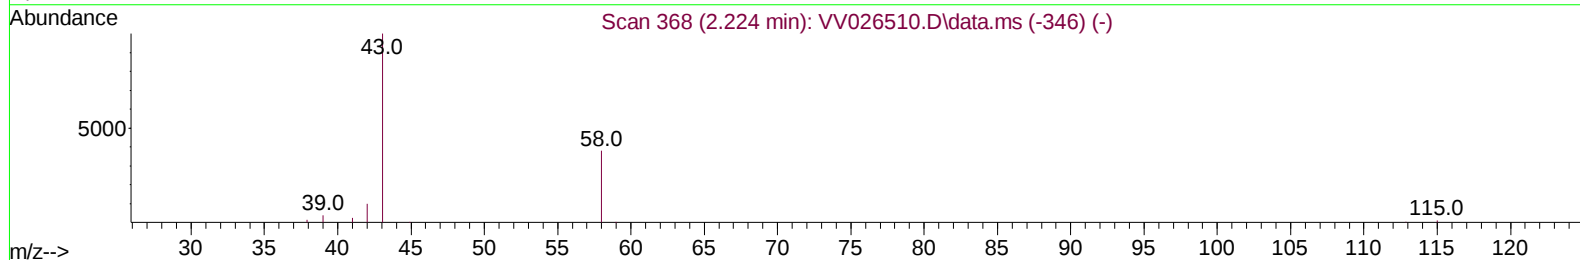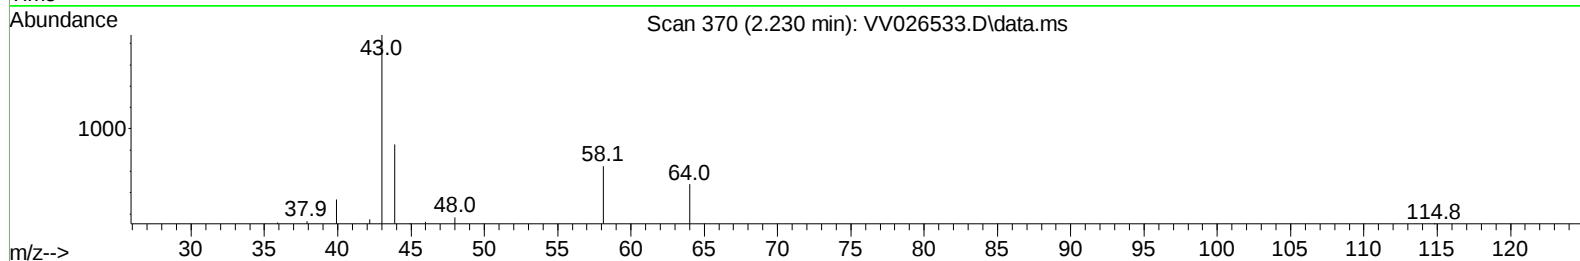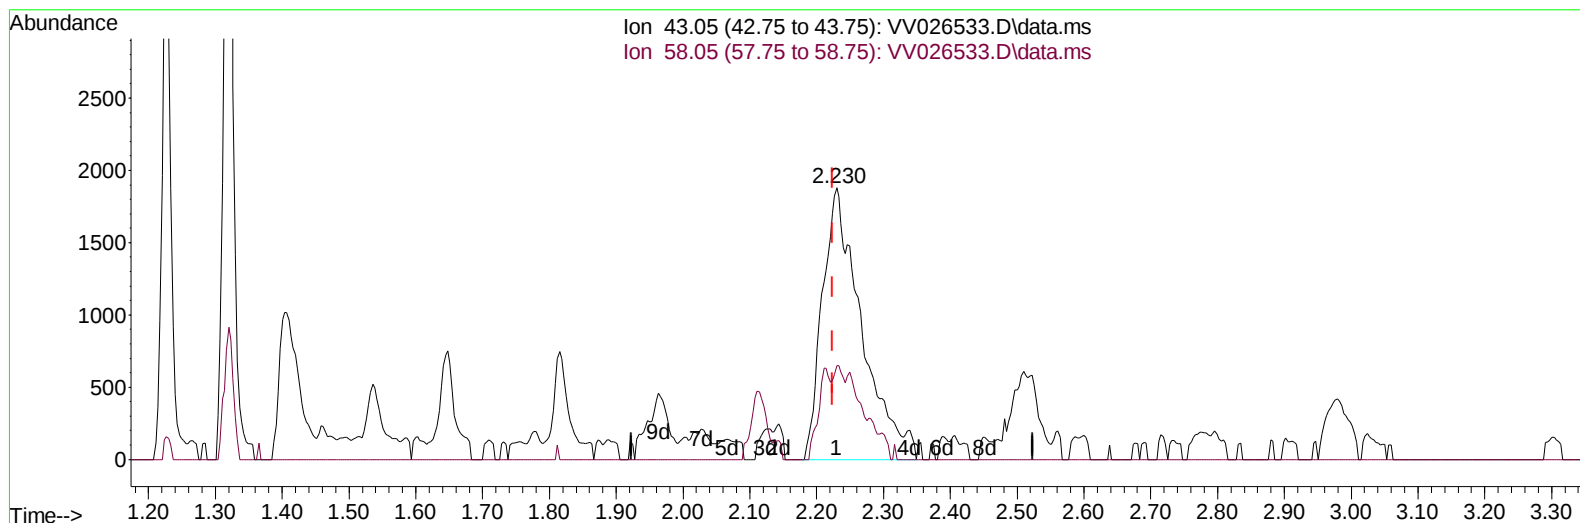

TIC: VV026533.D\data.ms

(13) Acetone (T)

2.230min (+ 0.006) 8.31 ug/L m

response 7613

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	2.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026533.D
 Acq On : 23 Jun 2022 22:43
 Operator : SY/MD
 Sample : N3374-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW4W0

Manual IntegrationsAPPROVED

Quant Time: Jun 24 02:06:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	180610	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	173504	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	75766	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	51227	3.527	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	70.600%		
7) Chloroethane-d5	1.581	69	46749	4.006	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	80.200%		
11) 1,1-Dichloroethene-d2	2.121	63	74359	2.881	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	57.600%#		
20) 2-Butanone-d5	3.931	46	75116	52.017	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	104.040%		
24) Chloroform-d	4.359	84	114837	4.836	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	96.800%		
26) 1,2-Dichloroethane-d4	5.043	65	47102	5.150	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	103.000%		
32) Benzene-d6	5.059	84	222594	4.466	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	89.400%		
36) 1,2-Dichloropropane-d6	6.075	67	67687	4.939	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	98.800%		
41) Toluene-d8	7.320	98	178190	3.976	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	79.600%		
43) trans-1,3-Dichloroprop...	7.632	79	9354	2.641	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	52.800%#		
46) 2-Hexanone-d5	8.095	63	64295	47.652	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	95.300%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	43174	4.816	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	96.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	65429	5.218	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	104.400%		
Target Compounds						
					Qvalue	
13) Acetone	2.230	43	7613m	8.310	ug/L	
14) Carbon disulfide	2.307	76	6422	0.200	ug/L	97
52) Ethylbenzene	9.018	91	6820	0.126	ug/L	96
53) m,p-Xylene	9.143	106	5558	0.263	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026533.D
Acq On : 23 Jun 2022 22:43
Operator : SY/MD
Sample : N3374-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW4W0

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 24 02:06:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

