




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026538.D
 Acq On : 24 Jun 2022 01:29
 Operator : SY/MD
 Sample : N3425-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL8

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:09:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

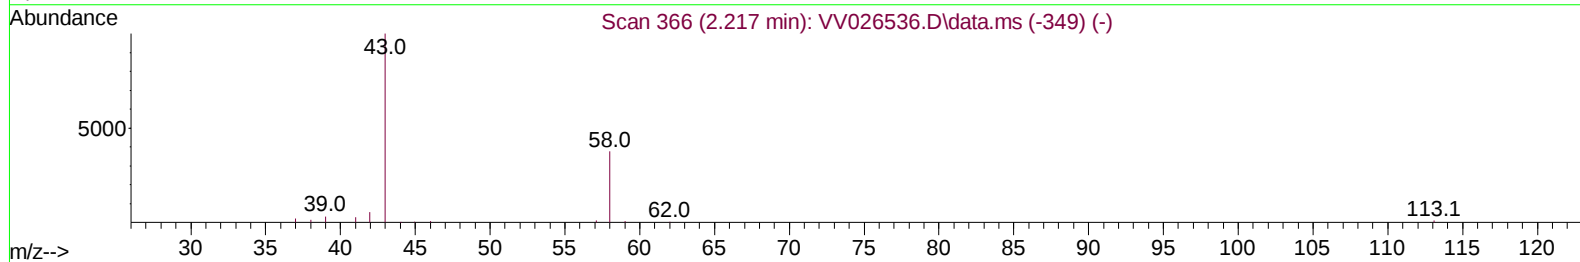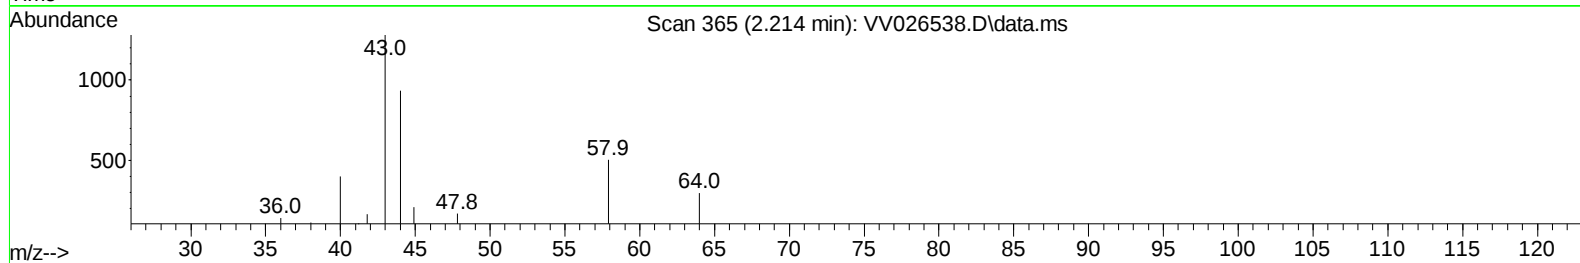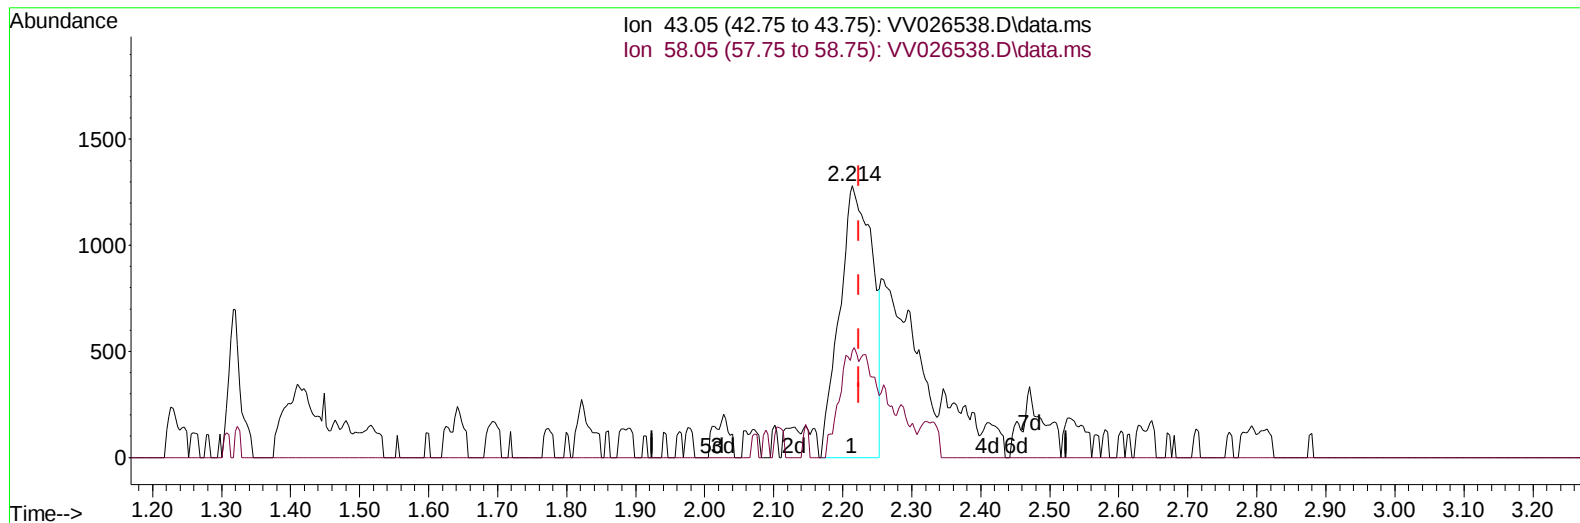

TIC: VV026538.D\data.ms

(13) Acetone (T)

2.214min (-0.010) 4.05 ug/L

response 4238

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	23.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026538.D
 Acq On : 24 Jun 2022 01:29
 Operator : SY/MD
 Sample : N3425-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL8

Manual IntegrationsAPPROVED

Quant Time: Jun 24 06:29:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

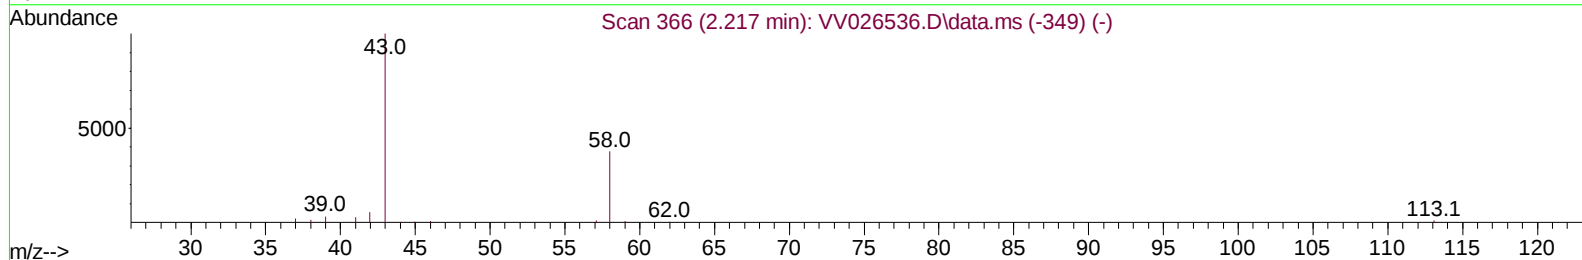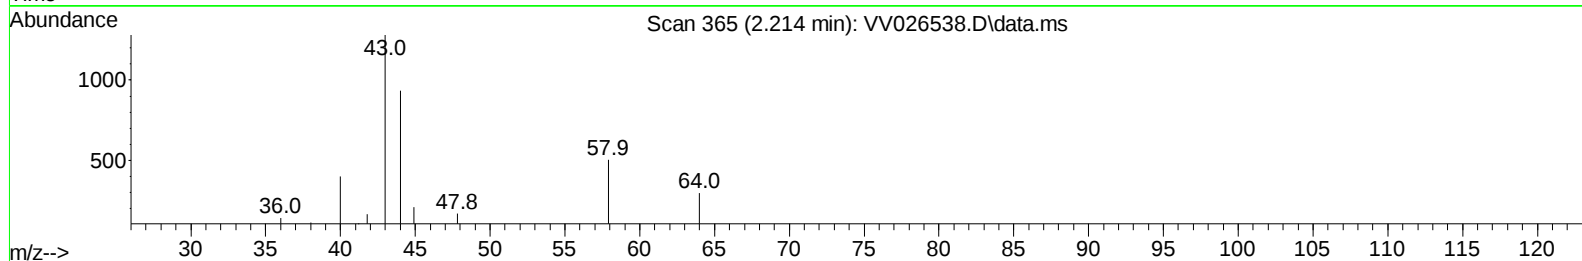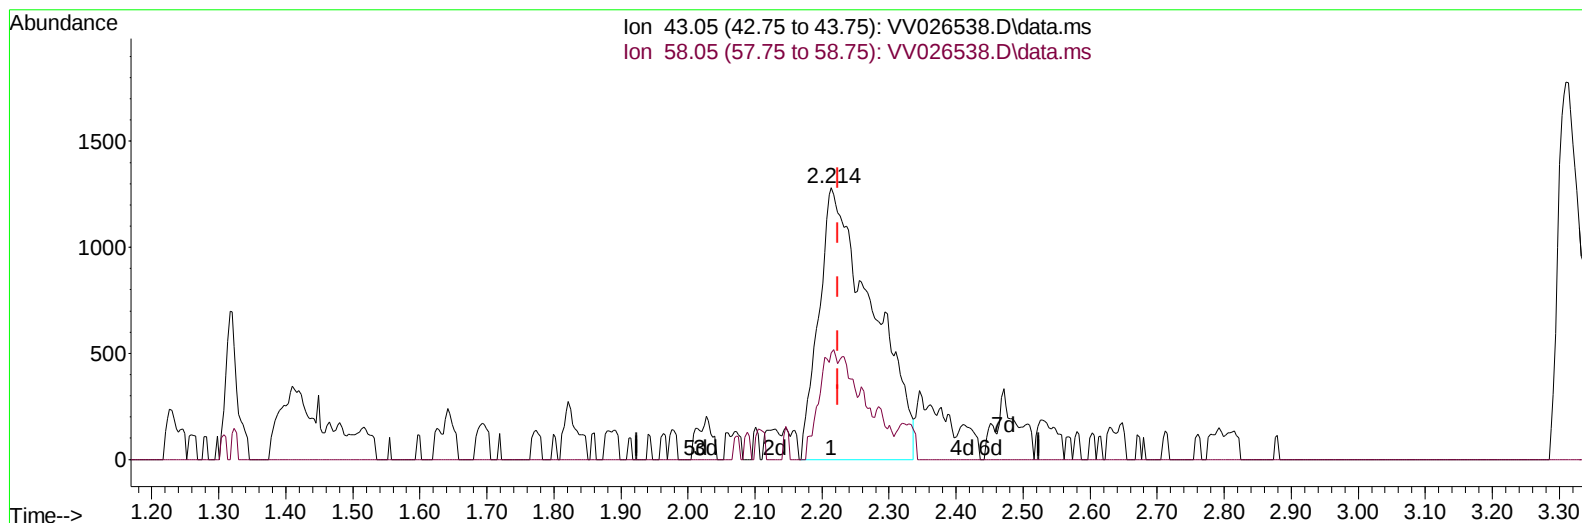

TIC: VV026538.D\data.ms

(13) Acetone (T)

2.214min (-0.010) 6.77 ug/L m

response 7085

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	13.93
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026538.D
 Acq On : 24 Jun 2022 01:29
 Operator : SY/MD
 Sample : N3425-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL8

Manual IntegrationsAPPROVED

Quant Time: Jun 24 06:29:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	206454	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	190873	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	80506	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	75287	4.534	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	90.600%	
7) Chloroethane-d5	1.580	69	63174	4.736	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	94.800%	
11) 1,1-Dichloroethene-d2	2.117	63	105944	3.591	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	71.800%	
20) 2-Butanone-d5	3.924	46	93882	56.874	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	113.740%	
24) Chloroform-d	4.362	84	136896	5.044	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	100.800%	
26) 1,2-Dichloroethane-d4	5.040	65	56437	5.399	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	108.000%	
32) Benzene-d6	5.059	84	271059	4.944	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	98.800%	
36) 1,2-Dichloropropane-d6	6.075	67	80604	5.346	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	107.000%	
41) Toluene-d8	7.316	98	223361	4.530	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	90.600%	
43) trans-1,3-Dichloroprop...	7.628	79	15793	4.053	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	81.000%	
46) 2-Hexanone-d5	8.091	63	76602	51.607	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	103.220%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	51457	5.217	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	104.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	72408	5.435	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	108.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.214	43	7085m	6.766	ug/L	
14) Carbon disulfide	2.304	76	6719	0.183	ug/L #	93
42) Toluene	7.397	91	13777	0.239	ug/L	96
52) Ethylbenzene	9.021	91	2831	0.048	ug/L	97
53) m,p-Xylene	9.146	106	2661	0.115	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026538.D
Acq On : 24 Jun 2022 01:29
Operator : SY/MD
Sample : N3425-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL8

Manual IntegrationsAPPROVED

Quant Time: Jun 24 06:29:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

