




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026539.D
 Acq On : 24 Jun 2022 01:53
 Operator : SY/MD
 Sample : N3425-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL7

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 25 02:10:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

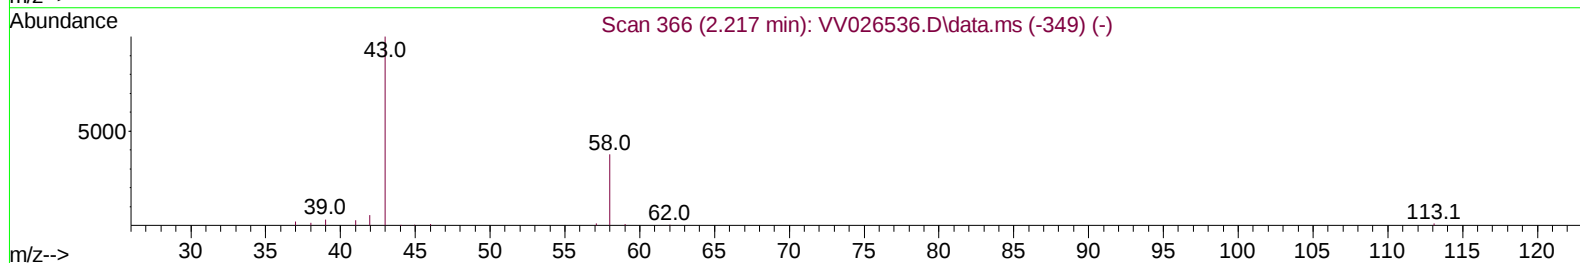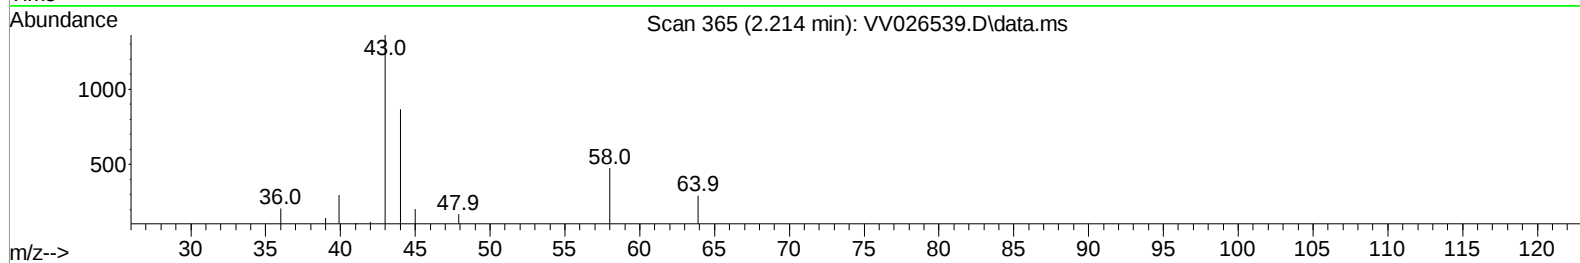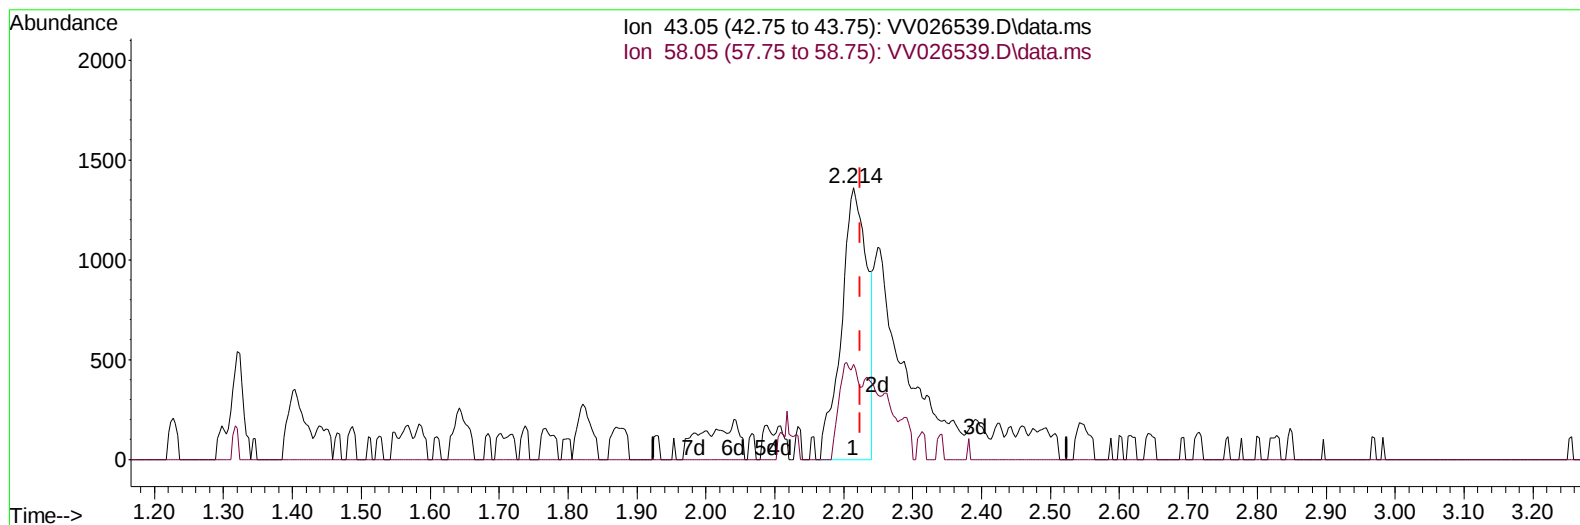

TIC: VV026539.D\data.ms

(13) Acetone (T)

2.214min (-0.010) 3.21 ug/L

response 3504

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	26.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026539.D
 Acq On : 24 Jun 2022 01:53
 Operator : SY/MD
 Sample : N3425-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL7

Manual IntegrationsAPPROVED

Quant Time: Jun 24 06:36:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

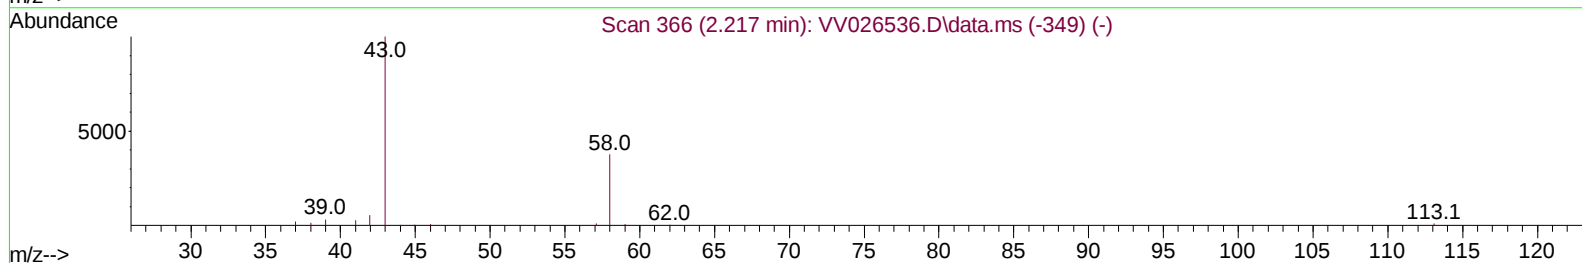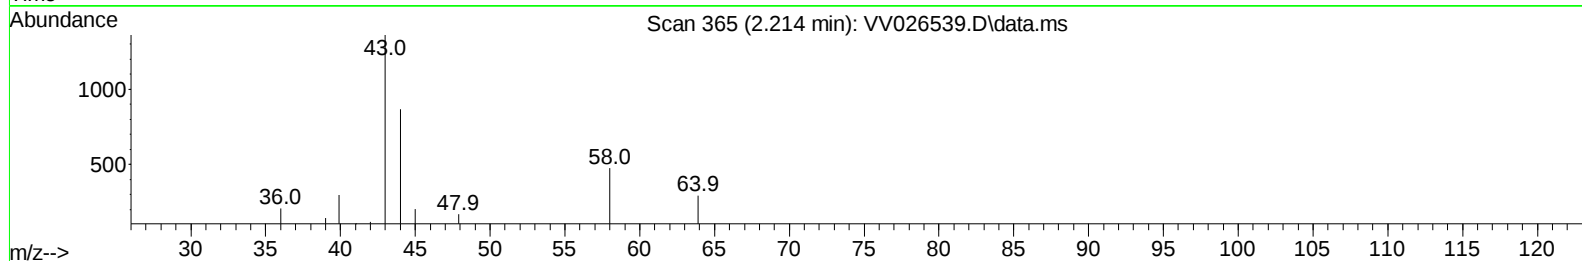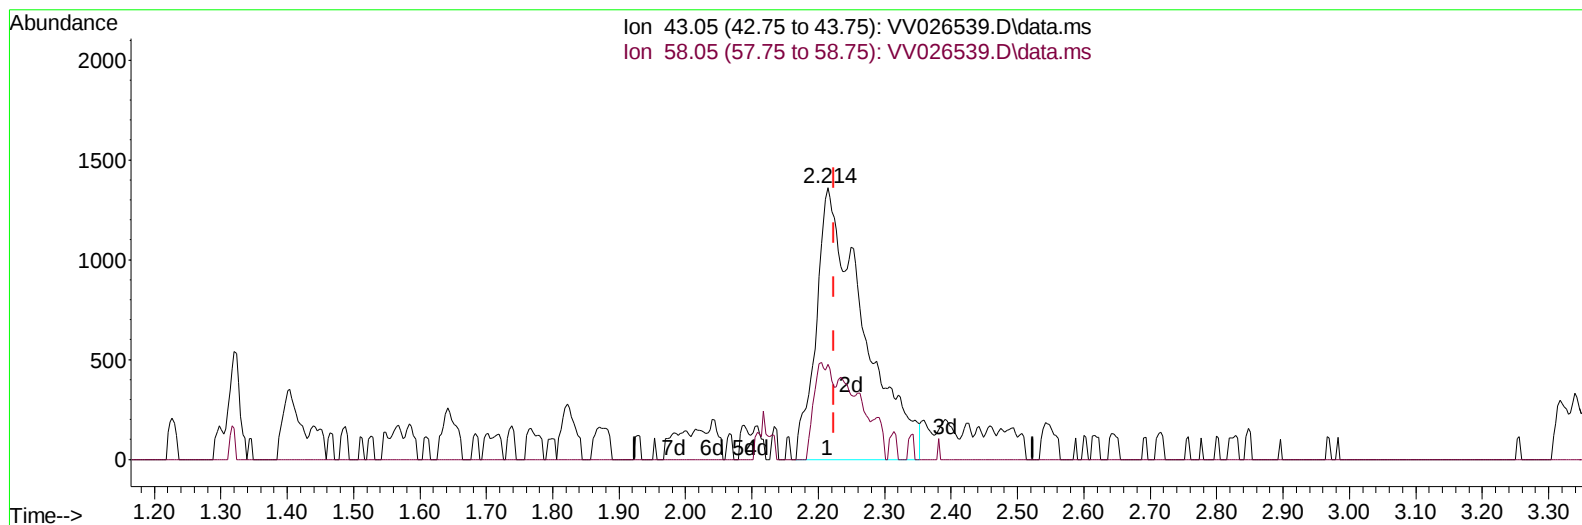

TIC: VV026539.D\data.ms

(13) Acetone (T)

2.214min (-0.010) 6.18 ug/L m

response 6742

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	13.96
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026539.D
 Acq On : 24 Jun 2022 01:53
 Operator : SY/MD
 Sample : N3425-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL7

Manual IntegrationsAPPROVED

Quant Time: Jun 24 06:36:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.622	114		214932	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		200879	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		85294	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.317	65		74621	4.317	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.400%	
7) Chloroethane-d5	1.581	69		63657	4.584	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%	
11) 1,1-Dichloroethene-d2	2.118	63		102722	3.344	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.800%	
20) 2-Butanone-d5	3.928	46		93550	54.437	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.880%	
24) Chloroform-d	4.359	84		131875	4.667	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	5.044	65		54575	5.015	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.060	84		260985	4.523	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.076	67		77978	4.915	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.320	98		213559	4.116	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.629	79		15281	3.726	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.600%	
46) 2-Hexanone-d5	8.092	63		75112	48.082	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.160%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		49448	4.764	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		71208	5.045	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%	
Target Compounds							
13) Acetone	2.214	43		6742m	6.184	ug/L	
14) Carbon disulfide	2.307	76		4797	0.125	ug/L #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026539.D
Acq On : 24 Jun 2022 01:53
Operator : SY/MD
Sample : N3425-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
COAL7

Manual IntegrationsAPPROVED

Quant Time: Jun 24 06:36:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

