




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026542.D
 Acq On : 24 Jun 2022 09:53
 Operator : SY/MD
 Sample : N3401-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

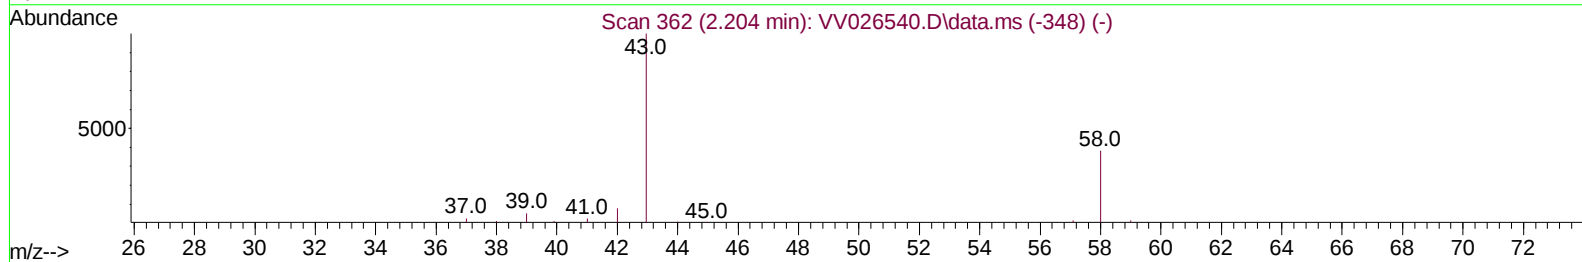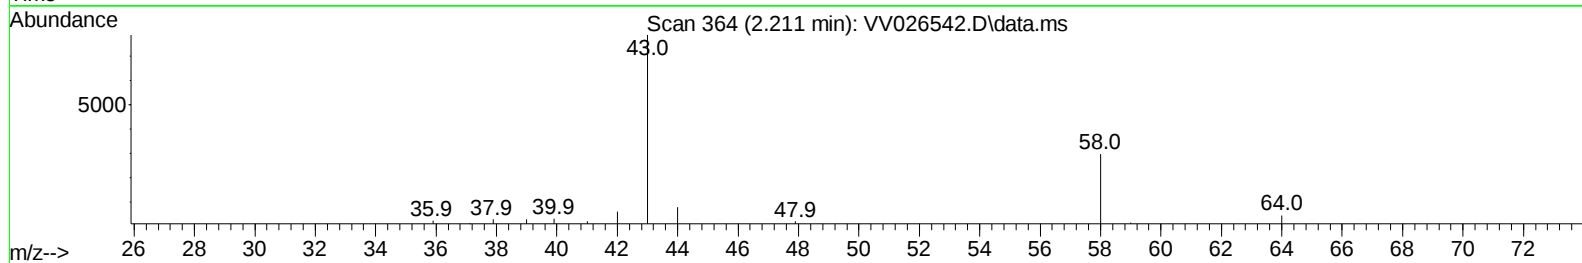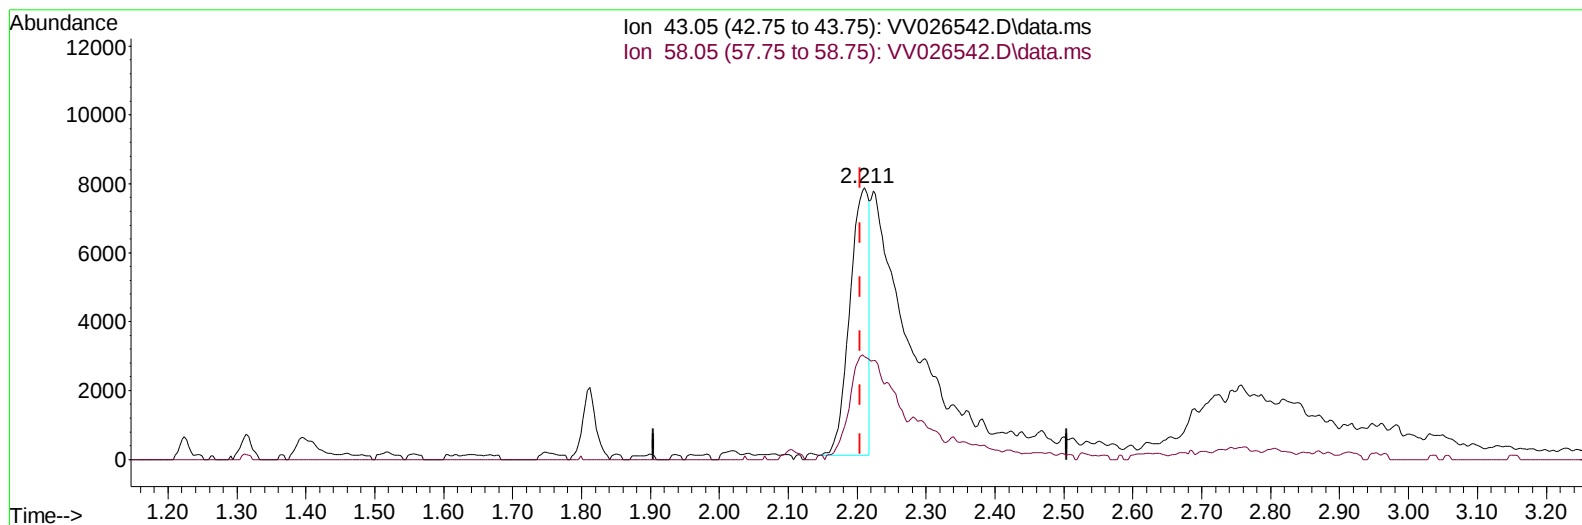

TIC: VV026542.D\data.ms

(13) Acetone (T)

2.211min (+ 0.006) 14.35 ug/L

response 14883

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	86.44#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026542.D
 Acq On : 24 Jun 2022 09:53
 Operator : SY/MD
 Sample : N3401-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

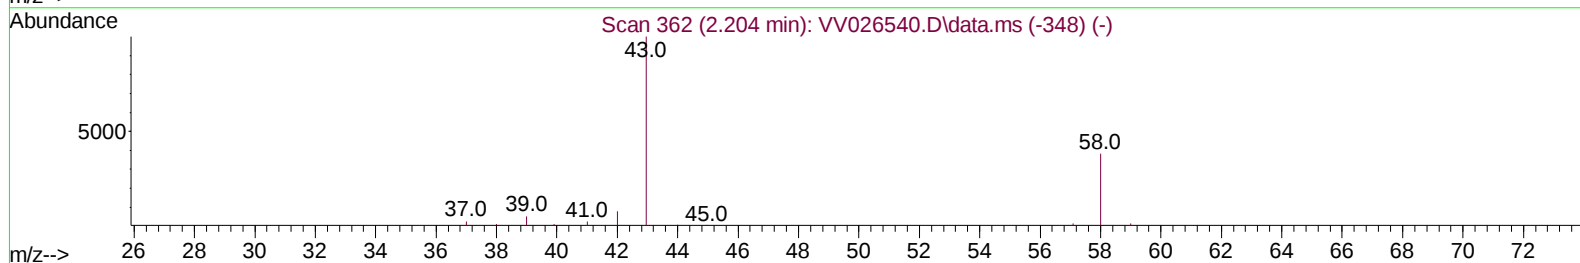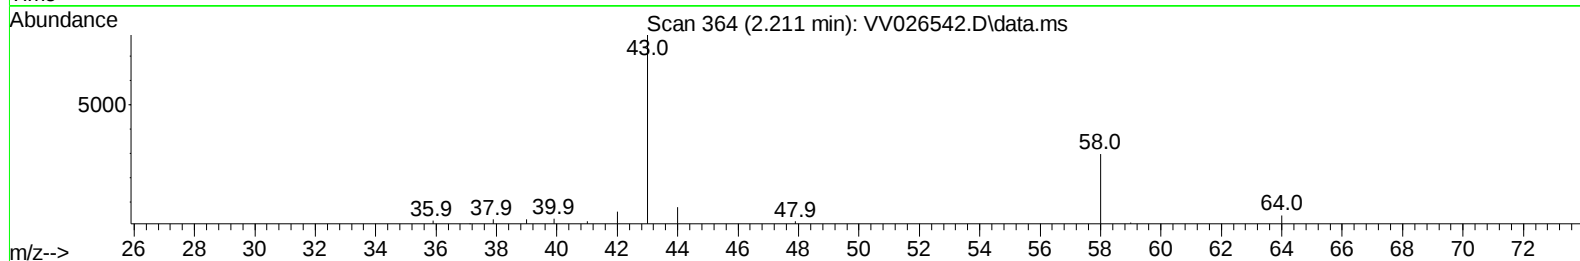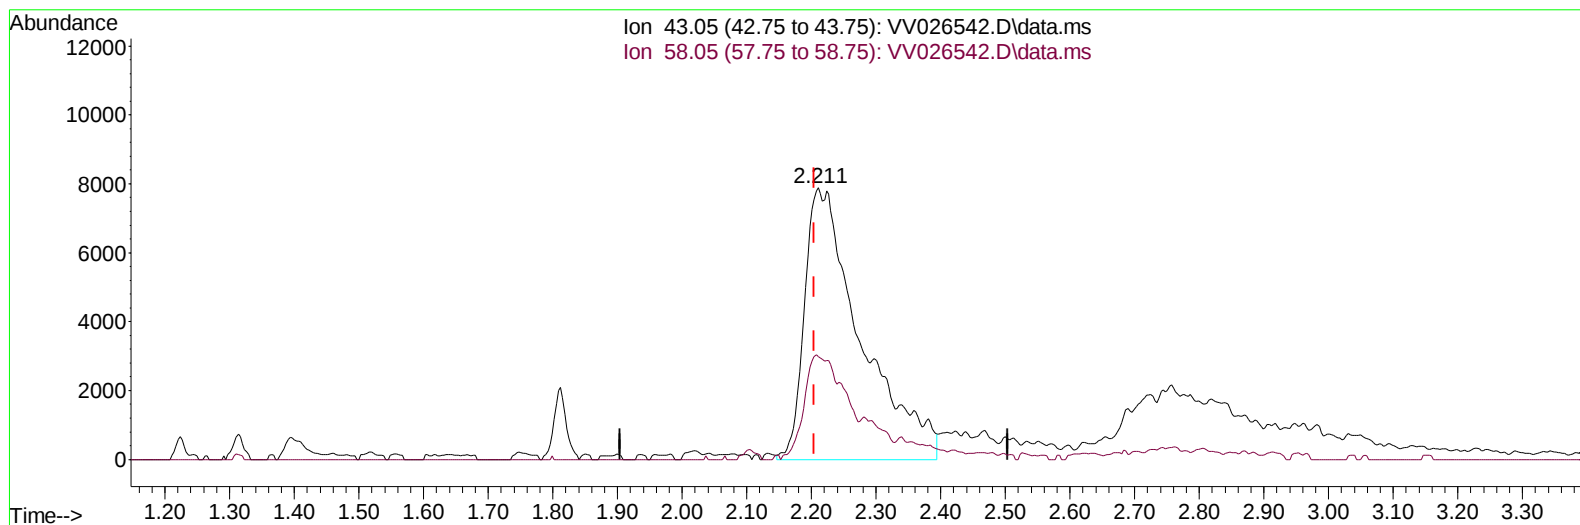

TIC: VV026542.D\data.ms

(13) Acetone (T)

2.211min (+ 0.006) 45.88 ug/L m

response 47580

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	37.50	27.04
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026542.D
 Acq On : 24 Jun 2022 09:53
 Operator : SY/MD
 Sample : N3401-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.619	114		204450	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		188475	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		78410	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.313	65		71897	4.373	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%	
7) Chloroethane-d5	1.574	69		61077	4.624	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.400%	
11) 1,1-Dichloroethene-d2	2.114	63		99696	3.412	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.200%	
20) 2-Butanone-d5	3.921	46		87972	53.816	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.640%	
24) Chloroform-d	4.349	84		126246	4.697	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.034	65		50954	4.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%	
32) Benzene-d6	5.050	84		255600	4.721	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	6.072	67		73262	4.921	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%	
41) Toluene-d8	7.316	98		216630	4.450	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%	
43) trans-1,3-Dichloroprop...	7.625	79		20149	5.236	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.800%	
46) 2-Hexanone-d5	8.091	63		61561	42.001	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.000%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84		44987	4.619	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		64599	4.978	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%	
Target Compounds							
13) Acetone	2.211	43		47580m	45.881	ug/L	
30) Cyclohexane	4.677	56		3417	0.186	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026542.D
Acq On : 24 Jun 2022 09:53
Operator : SY/MD
Sample : N3401-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG3

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 02:21:54 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

