




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV062322\  
 Data File : VV026543.D  
 Acq On : 24 Jun 2022 10:17  
 Operator : SY/MD  
 Sample : N3401-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AF8

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:35 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR062322WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 25 02:21:54 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022  
 Supervised By :Mahesh Dadoda 06/28/2022

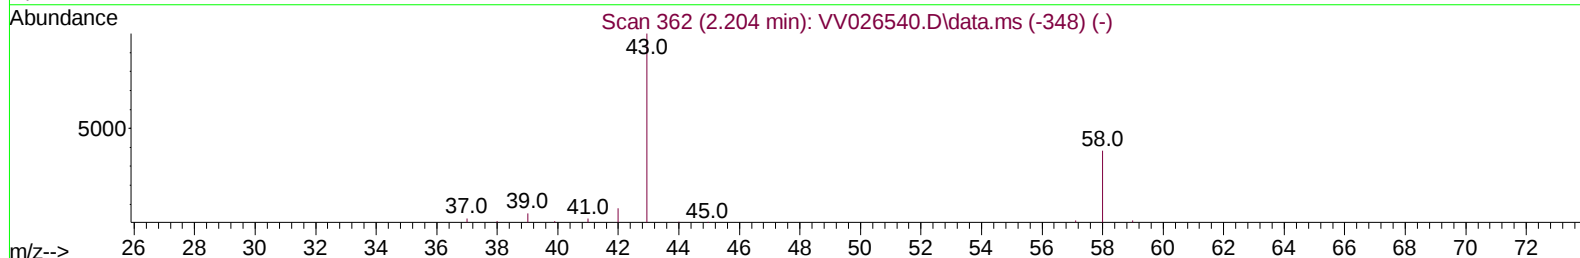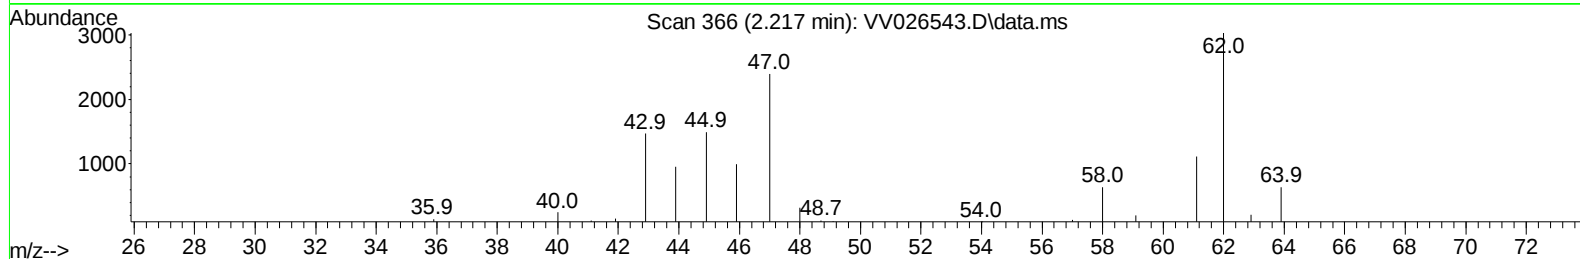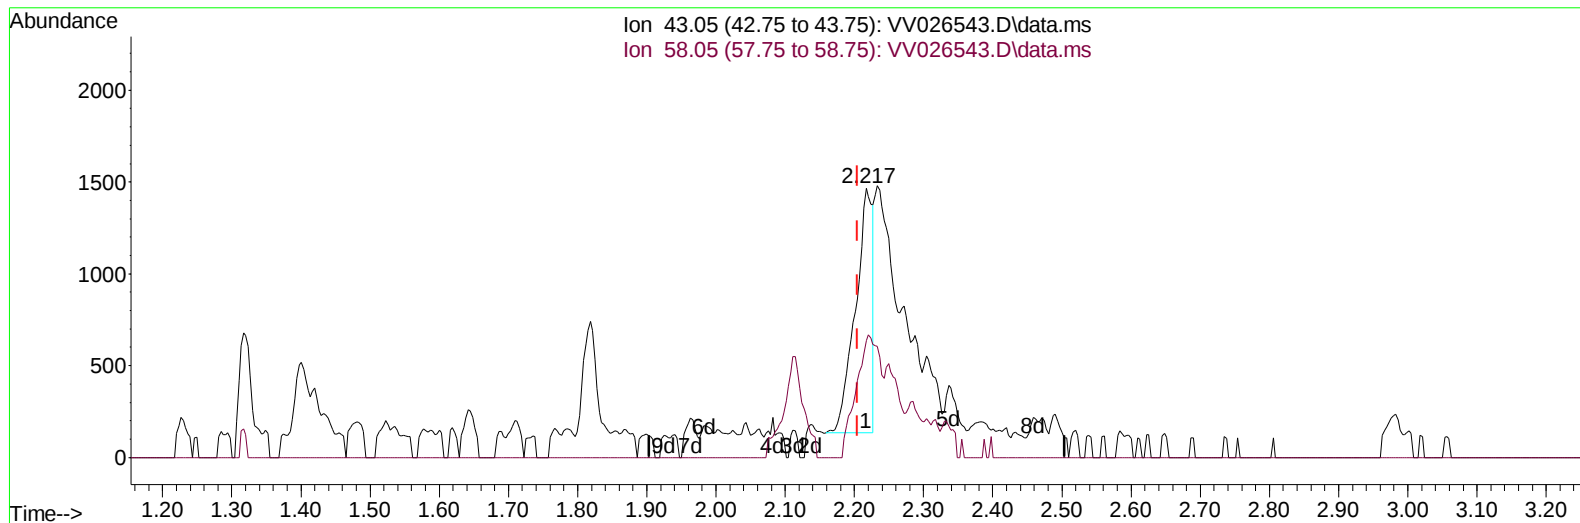

TIC: VV026543.D\data.ms

(13) Acetone (T)

2.217min (+ 0.013) 2.61 ug/L

response 2321

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 37.50  | 71.00  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV062322\  
 Data File : VV026543.D  
 Acq On : 24 Jun 2022 10:17  
 Operator : SY/MD  
 Sample : N3401-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AF8

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:35 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR062322WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 25 02:21:54 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022  
 Supervised By :Mahesh Dadoda 06/28/2022

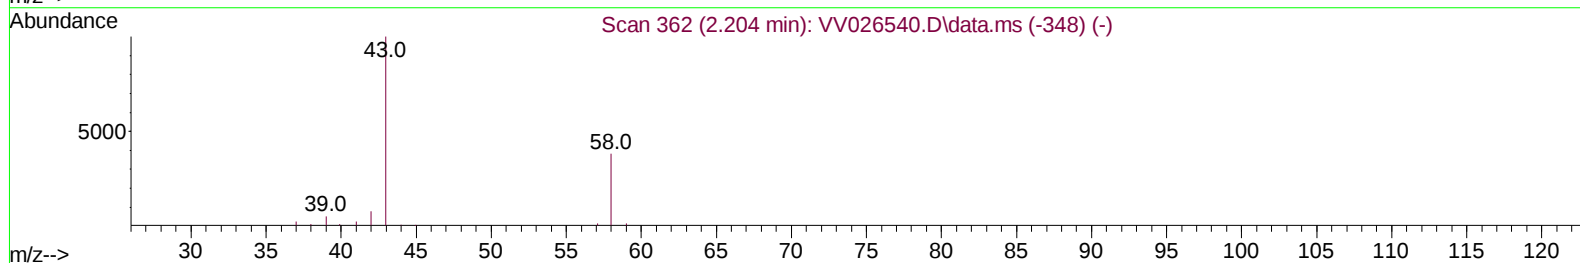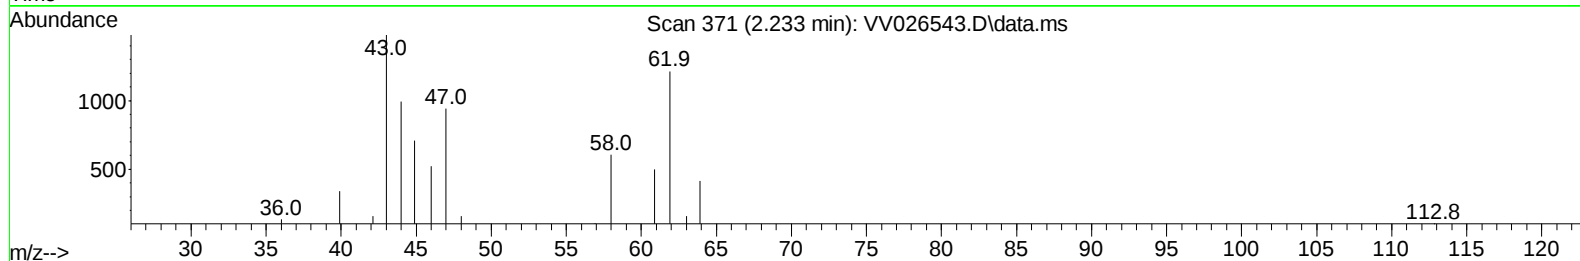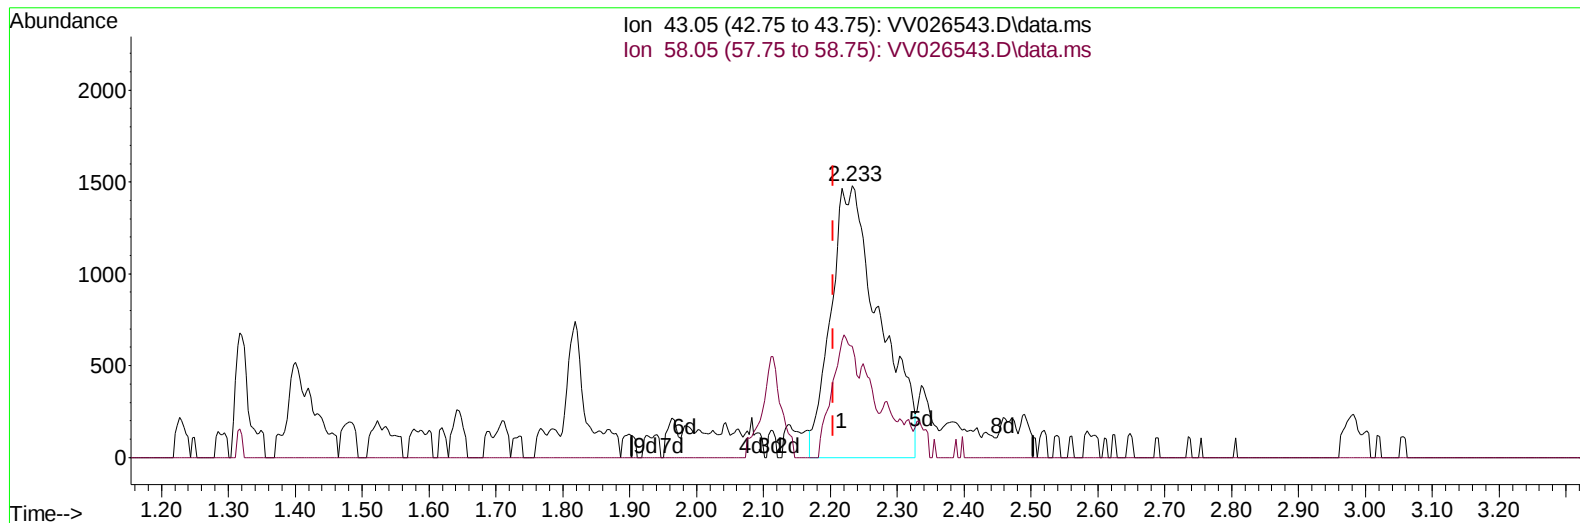

TIC: VV026543.D\data.ms

(13) Acetone (T)

2.233min (+ 0.029) 8.42 ug/L m

response 7479

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 37.50  | 22.04  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV062322\  
 Data File : VV026543.D  
 Acq On : 24 Jun 2022 10:17  
 Operator : SY/MD  
 Sample : N3401-04  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AF8

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:32:35 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR062322WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Jun 25 02:21:54 2022  
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022  
 Supervised By :Mahesh Dadoda 06/28/2022

| Compound                      | R.T.           | QIon | Response   | Conc     | Units | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|-------|----------|
| -----                         |                |      |            |          |       |          |
| Internal Standards            |                |      |            |          |       |          |
| 1) 1,4-Difluorobenzene        | 5.625          | 114  | 175052     | 5.000    | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.854          | 117  | 160260     | 5.000    | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249         | 152  | 67008      | 5.000    | ug/L  | 0.00     |
| System Monitoring Compounds   |                |      |            |          |       |          |
| 4) Vinyl Chloride-d3          | 1.317          | 65   | 50986      | 3.622    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 40 - 130 |      | Recovery = | 72.400%  |       |          |
| 7) Chloroethane-d5            | 1.581          | 69   | 48647      | 4.301    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 65 - 130 |      | Recovery = | 86.000%  |       |          |
| 11) 1,1-Dichloroethene-d2     | 2.118          | 63   | 78250      | 3.128    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 60 - 125 |      | Recovery = | 62.600%  |       |          |
| 20) 2-Butanone-d5             | 3.934          | 46   | 67757      | 48.411   | ug/L  | 0.02     |
| Spiked Amount 50.000          | Range 40 - 130 |      | Recovery = | 96.820%  |       |          |
| 24) Chloroform-d              | 4.359          | 84   | 112915     | 4.907    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 125 |      | Recovery = | 98.200%  |       |          |
| 26) 1,2-Dichloroethane-d4     | 5.043          | 65   | 45178      | 5.097    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 130 |      | Recovery = | 102.000% |       |          |
| 32) Benzene-d6                | 5.060          | 84   | 218795     | 4.753    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 125 |      | Recovery = | 95.000%  |       |          |
| 36) 1,2-Dichloropropane-d6    | 6.076          | 67   | 65715      | 5.191    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 60 - 140 |      | Recovery = | 103.800% |       |          |
| 41) Toluene-d8                | 7.320          | 98   | 178868     | 4.321    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 70 - 130 |      | Recovery = | 86.400%  |       |          |
| 43) trans-1,3-Dichloroprop... | 7.629          | 79   | 14070      | 4.300    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 55 - 130 |      | Recovery = | 86.000%  |       |          |
| 46) 2-Hexanone-d5             | 8.095          | 63   | 46532      | 37.337   | ug/L  | 0.00     |
| Spiked Amount 50.000          | Range 45 - 130 |      | Recovery = | 74.680%  |       |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217         | 84   | 40254      | 4.861    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 65 - 120 |      | Recovery = | 97.200%  |       |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622         | 152  | 56326      | 5.079    | ug/L  | 0.00     |
| Spiked Amount 5.000           | Range 80 - 120 |      | Recovery = | 101.600% |       |          |
| Target Compounds              |                |      |            |          |       |          |
|                               |                |      |            |          |       | Qvalue   |
| 13) Acetone                   | 2.233          | 43   | 7479m      | 8.423    | ug/L  |          |
| 42) Toluene                   | 7.397          | 91   | 27091      | 0.561    | ug/L  | 100      |
| -----                         |                |      |            |          |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV062322\  
Data File : VV026543.D  
Acq On : 24 Jun 2022 10:17  
Operator : SY/MD  
Sample : N3401-04  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AF8

## Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022  
Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 25 02:32:35 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR062322WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Jun 25 02:21:54 2022  
Response via : Initial Calibration

