

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026548.D
 Acq On : 24 Jun 2022 12:17
 Operator : SY/MD
 Sample : N3401-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Supervised By :Mahesh
 Dadoda
 06/28/2022

Quant Time: Jun 25 02:33:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

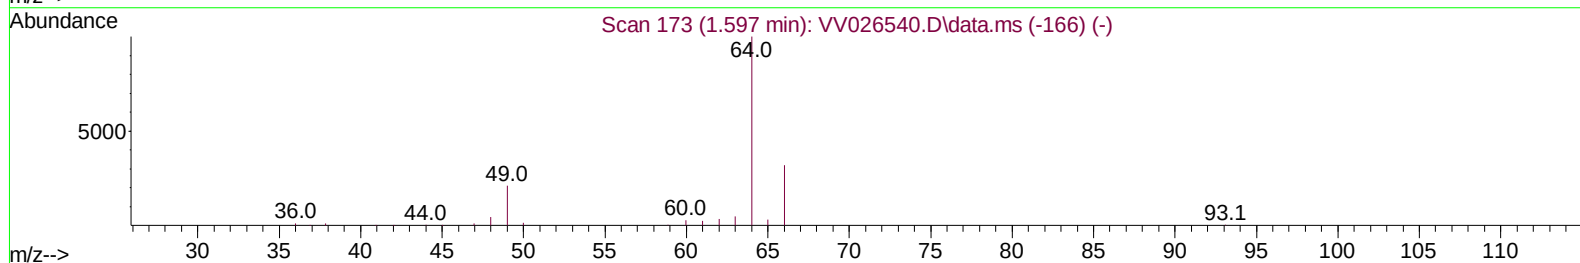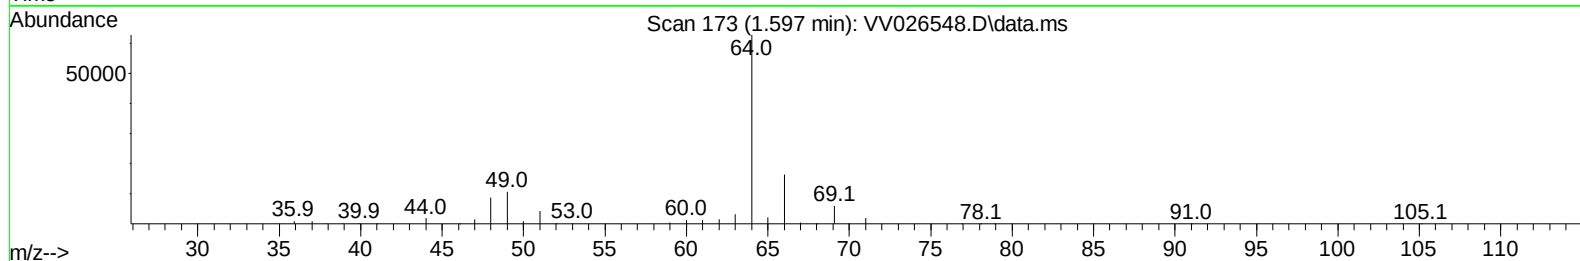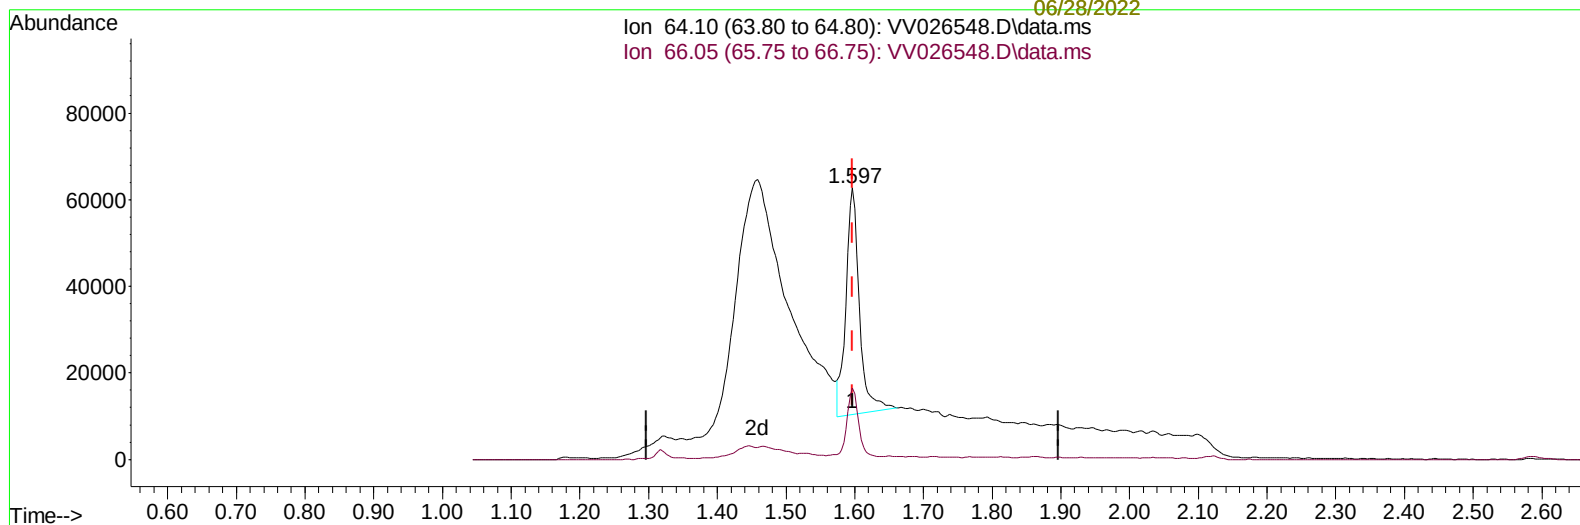

TIC: VV026548.D\data.ms

(8) Chloroethane (T)

1.597min (+ 0.000) 4.46 ug/L

response 71078

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	28.60	26.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026548.D
 Acq On : 24 Jun 2022 12:17
 Operator : SY/MD
 Sample : N3401-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1




Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Supervised By :Mahesh
 Dadoda
 06/28/2022

Quant Time: Jun 25 02:33:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

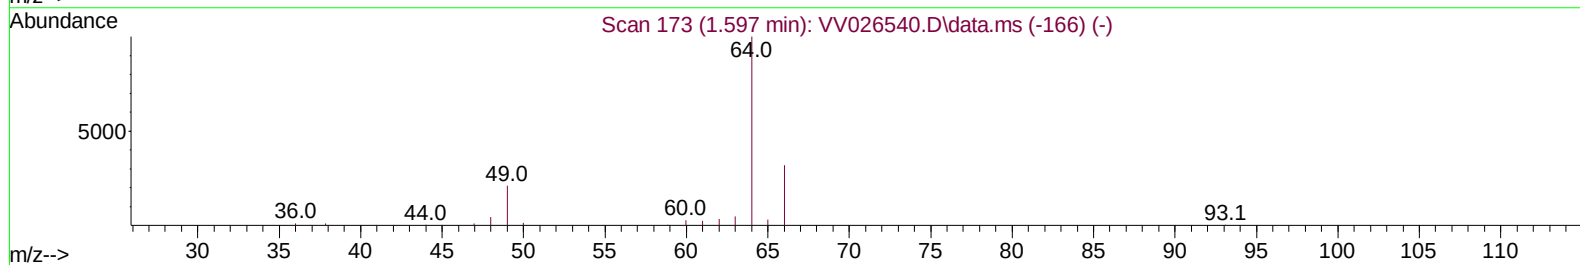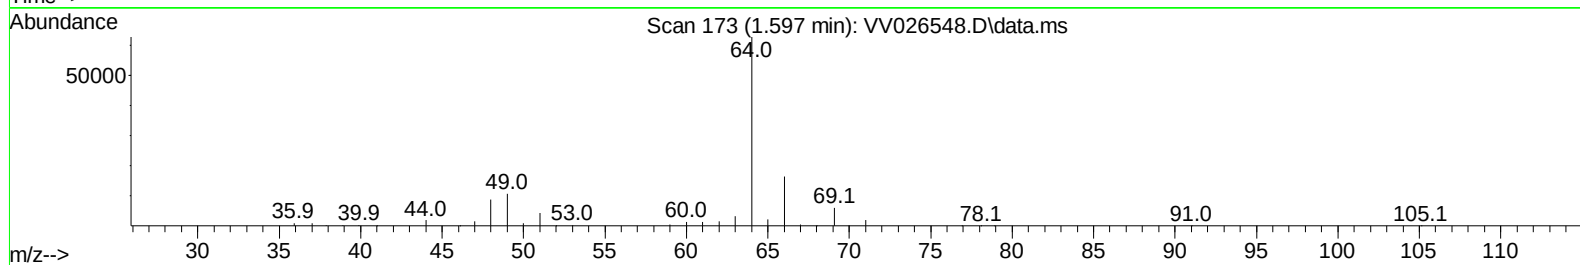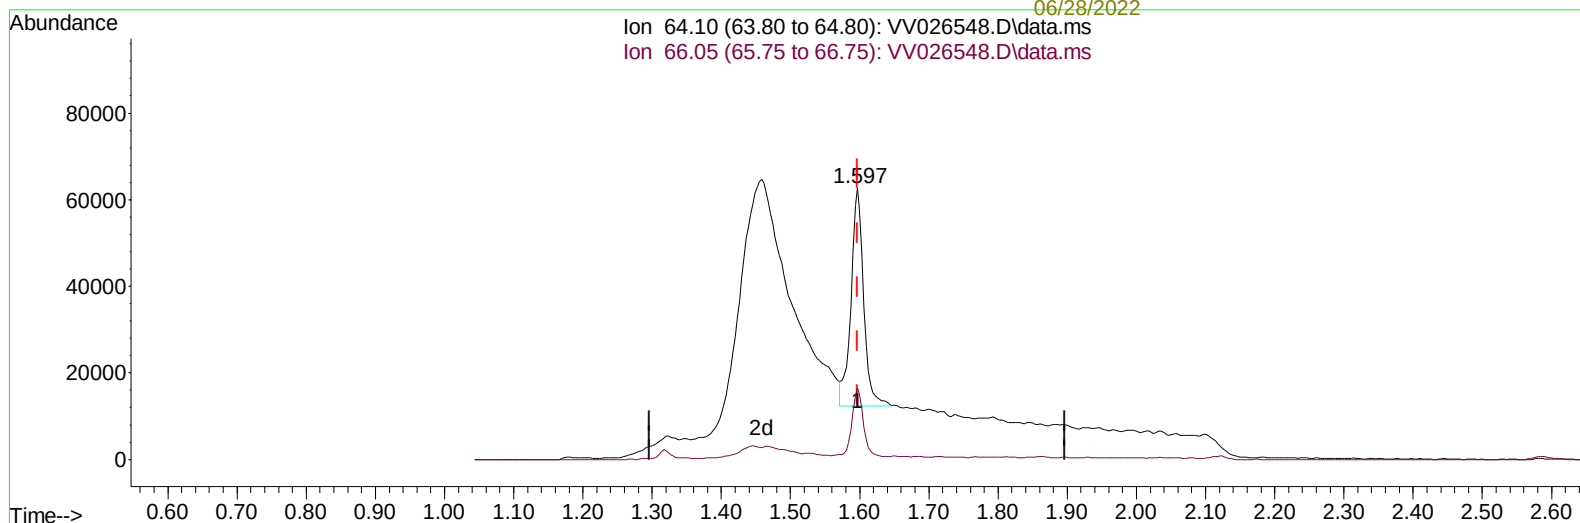

TIC: VV026548.D\data.ms

(8) Chloroethane (T)

1.597min (+ 0.000) 4.02 ug/L m

response 64138

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	28.60	26.36
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026548.D
 Acq On : 24 Jun 2022 12:17
 Operator : SY/MD
 Sample : N3401-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF2

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Supervised By :Mahesh
 Dadoda
 06/28/2022

Quant Time: Jun 25 02:33:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.622	114		264388	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		235304	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		118591	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.317	65		84459	3.972	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	79.400%	
7) Chloroethane-d5	1.581	69		70765	4.143	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	82.800%	
11) 1,1-Dichloroethene-d2	2.118	63		113666	3.009	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	60.200%	
20) 2-Butanone-d5	3.915	46		108247	51.207	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	102.420%	
24) Chloroform-d	4.359	84		145844	4.196	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	84.000%	
26) 1,2-Dichloroethane-d4	5.040	65		57843	4.321	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	86.400%	
32) Benzene-d6	5.056	84		312849	4.629	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	92.600%	
36) 1,2-Dichloropropane-d6	6.076	67		90198	4.853	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	97.000%	
41) Toluene-d8	7.317	98		293459	4.828	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	96.600%	
43) trans-1,3-Dichloroprop...	7.629	79		28853	6.006	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	120.200%	
46) 2-Hexanone-d5	8.092	63		95975	52.449	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	104.900%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		56088	4.613	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	92.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		97703	4.978	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	99.600%	
Target Compounds							
						Qvalue	
8) Chloroethane	1.597	64		64138m	4.023	ug/L	
30) Cyclohexane	4.687	56		1220478	53.239	ug/L	99
33) Benzene	5.111	78		85535	1.245	ug/L	100
35) Methylcyclohexane	6.137	83		1822004	68.189	ug/L	96
42) Toluene	7.394	91		103352	1.457	ug/L	99
51) Chlorobenzene	8.886	112		12334	0.265	ug/L	96
52) Ethylbenzene	9.011	91		1182356	16.119	ug/L	100
53) m,p-Xylene	9.140	106		178130	6.225	ug/L	97
54) o-Xylene	9.548	106		4524	0.168	ug/L	98
60) Isopropylbenzene	9.934	105		11349894	155.184	ug/L	96
63) 1,2,4-Trimethylbenzene	10.911	105		2099588	36.830	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

