




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026555.D
 Acq On : 24 Jun 2022 15:03
 Operator : SY/MD
 Sample : N3401-13DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:35:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

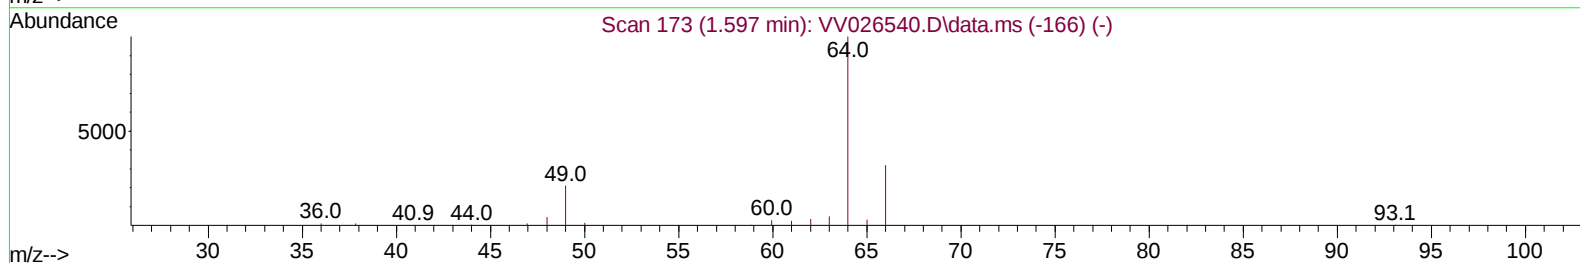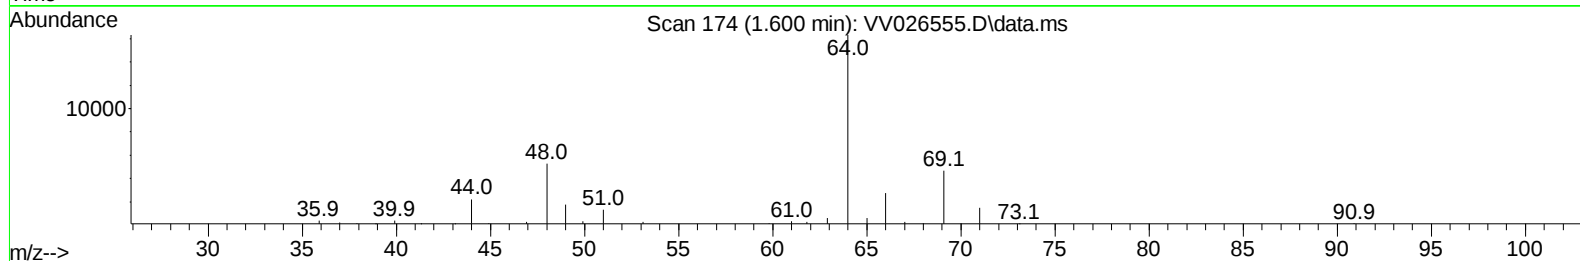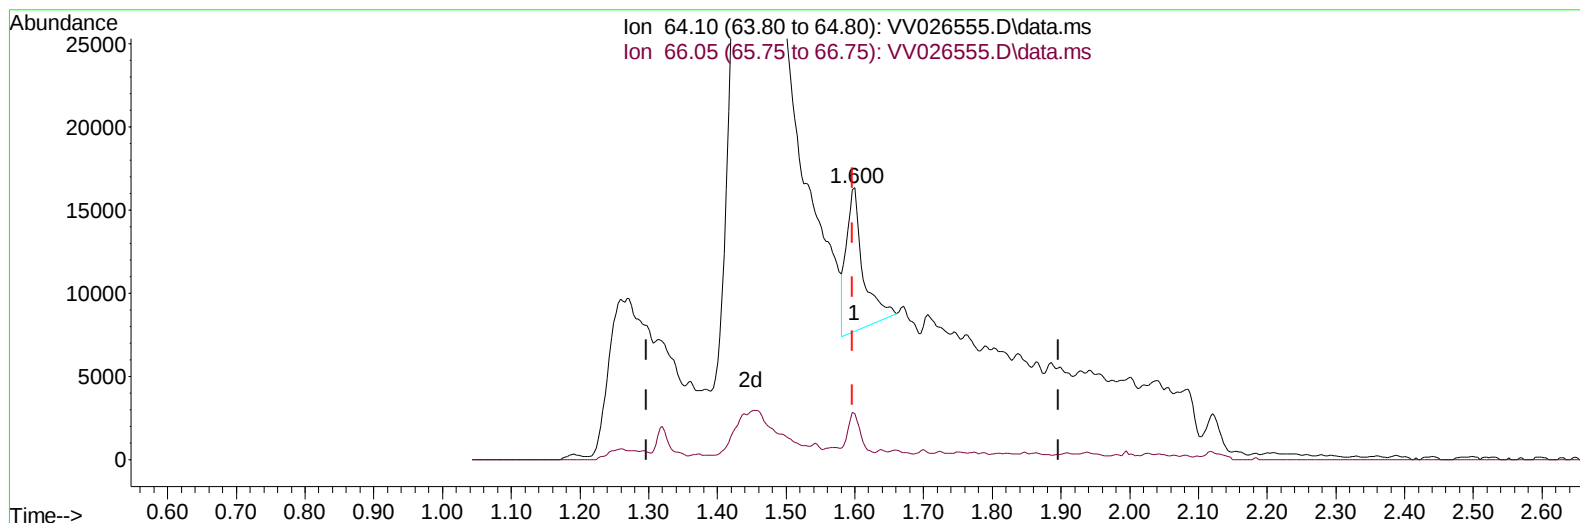

TIC: VV026555.D\data.ms

(8) Chloroethane (T)

1.600min (+ 0.003) 0.97 ug/L

response 14765

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	28.60	16.94#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026555.D
Acq On : 24 Jun 2022 15:03
Operator : SY/MD
Sample : N3401-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:35:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 02:21:54 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

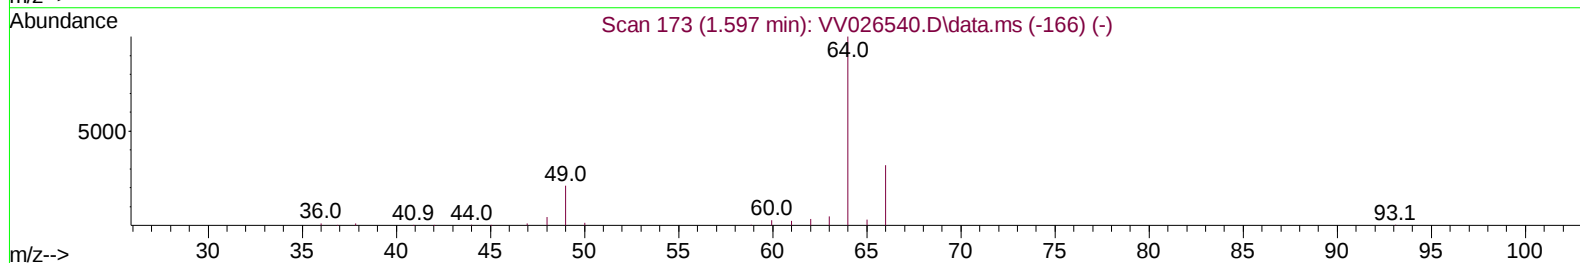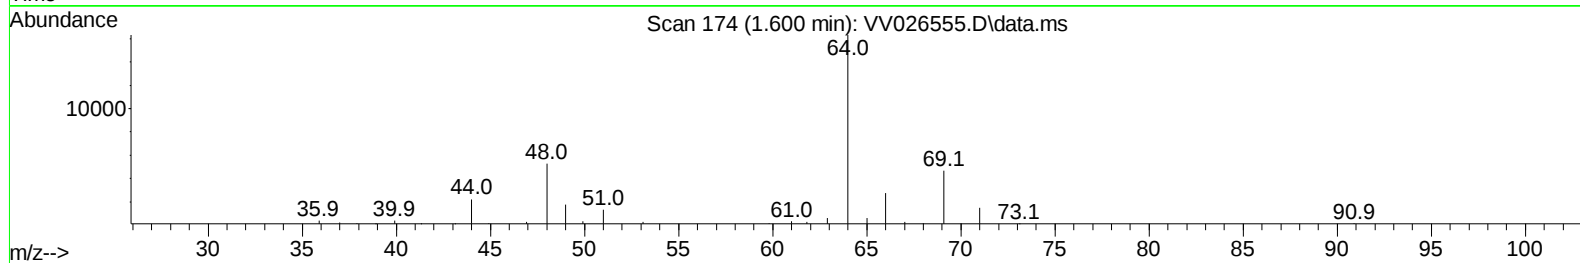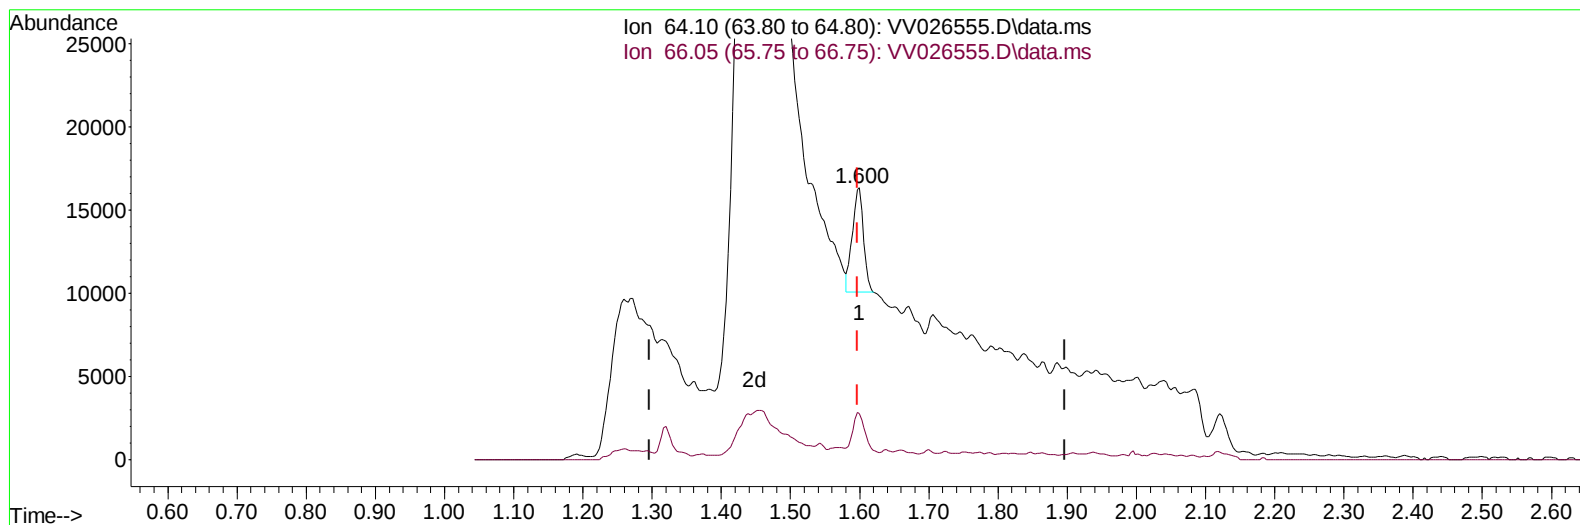

TIC: VV026555.D\data.ms

(8) Chloroethane (T)

1.600min (+ 0.003) 0.45 ug/L m

response 6885

Ion	Exp%	Act%
64.10	100.00	100.00
66.05	28.60	16.94#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
 Data File : VV026555.D
 Acq On : 24 Jun 2022 15:03
 Operator : SY/MD
 Sample : N3401-13DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF1DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:35:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/28/2022
 Supervised By :Mahesh Dadoda 06/28/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	252855	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	230719	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	101806	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	76000	3.737	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	74.800%	
7) Chloroethane-d5	1.580	69	66729	4.085	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	81.600%	
11) 1,1-Dichloroethene-d2	2.121	63	106283	2.941	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	58.800%#	
20) 2-Butanone-d5	3.908	46	115792	57.275	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	114.540%	
24) Chloroform-d	4.362	84	139739	4.204	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	84.000%	
26) 1,2-Dichloroethane-d4	5.043	65	57733	4.509	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	90.200%	
32) Benzene-d6	5.059	84	290713	4.387	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	87.800%	
36) 1,2-Dichloropropane-d6	6.075	67	85726	4.704	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	94.000%	
41) Toluene-d8	7.320	98	249027	4.179	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	83.600%	
43) trans-1,3-Dichloroprop...	7.628	79	22421	4.760	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	95.200%	
46) 2-Hexanone-d5	8.091	63	87971	49.031	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	98.060%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	52110	4.371	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	87.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	81593	4.843	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	96.800%	
Target Compounds						
					Qvalue	
8) Chloroethane	1.600	64	6885m	0.452	ug/L	
16) Methylene chloride	2.519	84	3991	0.220	ug/L	94
30) Cyclohexane	4.686	56	3849	0.171	ug/L	99
35) Methylcyclohexane	6.136	83	4274	0.163	ug/L	90
42) Toluene	7.390	91	564684	8.120	ug/L	100
52) Ethylbenzene	9.014	91	23344	0.325	ug/L	96
53) m,p-Xylene	9.140	106	24658	0.879	ug/L	100
54) o-Xylene	9.548	106	8141	0.309	ug/L	88
60) Isopropylbenzene	9.934	105	23202	0.370	ug/L	97
62) 1,3,5-Trimethylbenzene	10.545	105	3029	0.061	ug/L	99
63) 1,2,4-Trimethylbenzene	10.918	105	10897	0.223	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026555.D
Acq On : 24 Jun 2022 15:03
Operator : SY/MD
Sample : N3401-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF1DL

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 06/28/2022
Supervised By :Mahesh Dadoda 06/28/2022

Quant Time: Jun 25 02:35:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 02:21:54 2022
Response via : Initial Calibration

