

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062322\
 Data File : VW026529.D
 Acq On : 23 Jun 2022 21:07
 Operator : SY/MD
 Sample : N3400-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAFO

Quant Time: Jun 24 02:05:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 24 00:51:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	171995	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	161136	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67868	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	50367	3.641	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.800%
7) Chloroethane-d5	1.577	69	47595	4.283	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.117	63	76295	3.104	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.000%
20) 2-Butanone-d5	3.928	46	81142	59.004	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.000%
24) Chloroform-d	4.358	84	112277	4.966	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%
26) 1,2-Dichloroethane-d4	5.043	65	46467	5.335	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.800%
32) Benzene-d6	5.056	84	217122	4.691	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.800%
36) 1,2-Dichloropropane-d6	6.075	67	66782	5.247	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.000%
41) Toluene-d8	7.320	98	173914	4.178	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	7.628	79	11179	3.398	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.000%
46) 2-Hexanone-d5	8.091	63	65175	52.012	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44819	5.383	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	60099	5.351	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.000%
Target Compounds					Qvalue	
42) Toluene	7.400	91	9779	0.201	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026529.D
Acq On : 23 Jun 2022 21:07
Operator : SY/MD
Sample : N3400-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAFO

Quant Time: Jun 24 02:05:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 24 00:51:15 2022
Response via : Initial Calibration

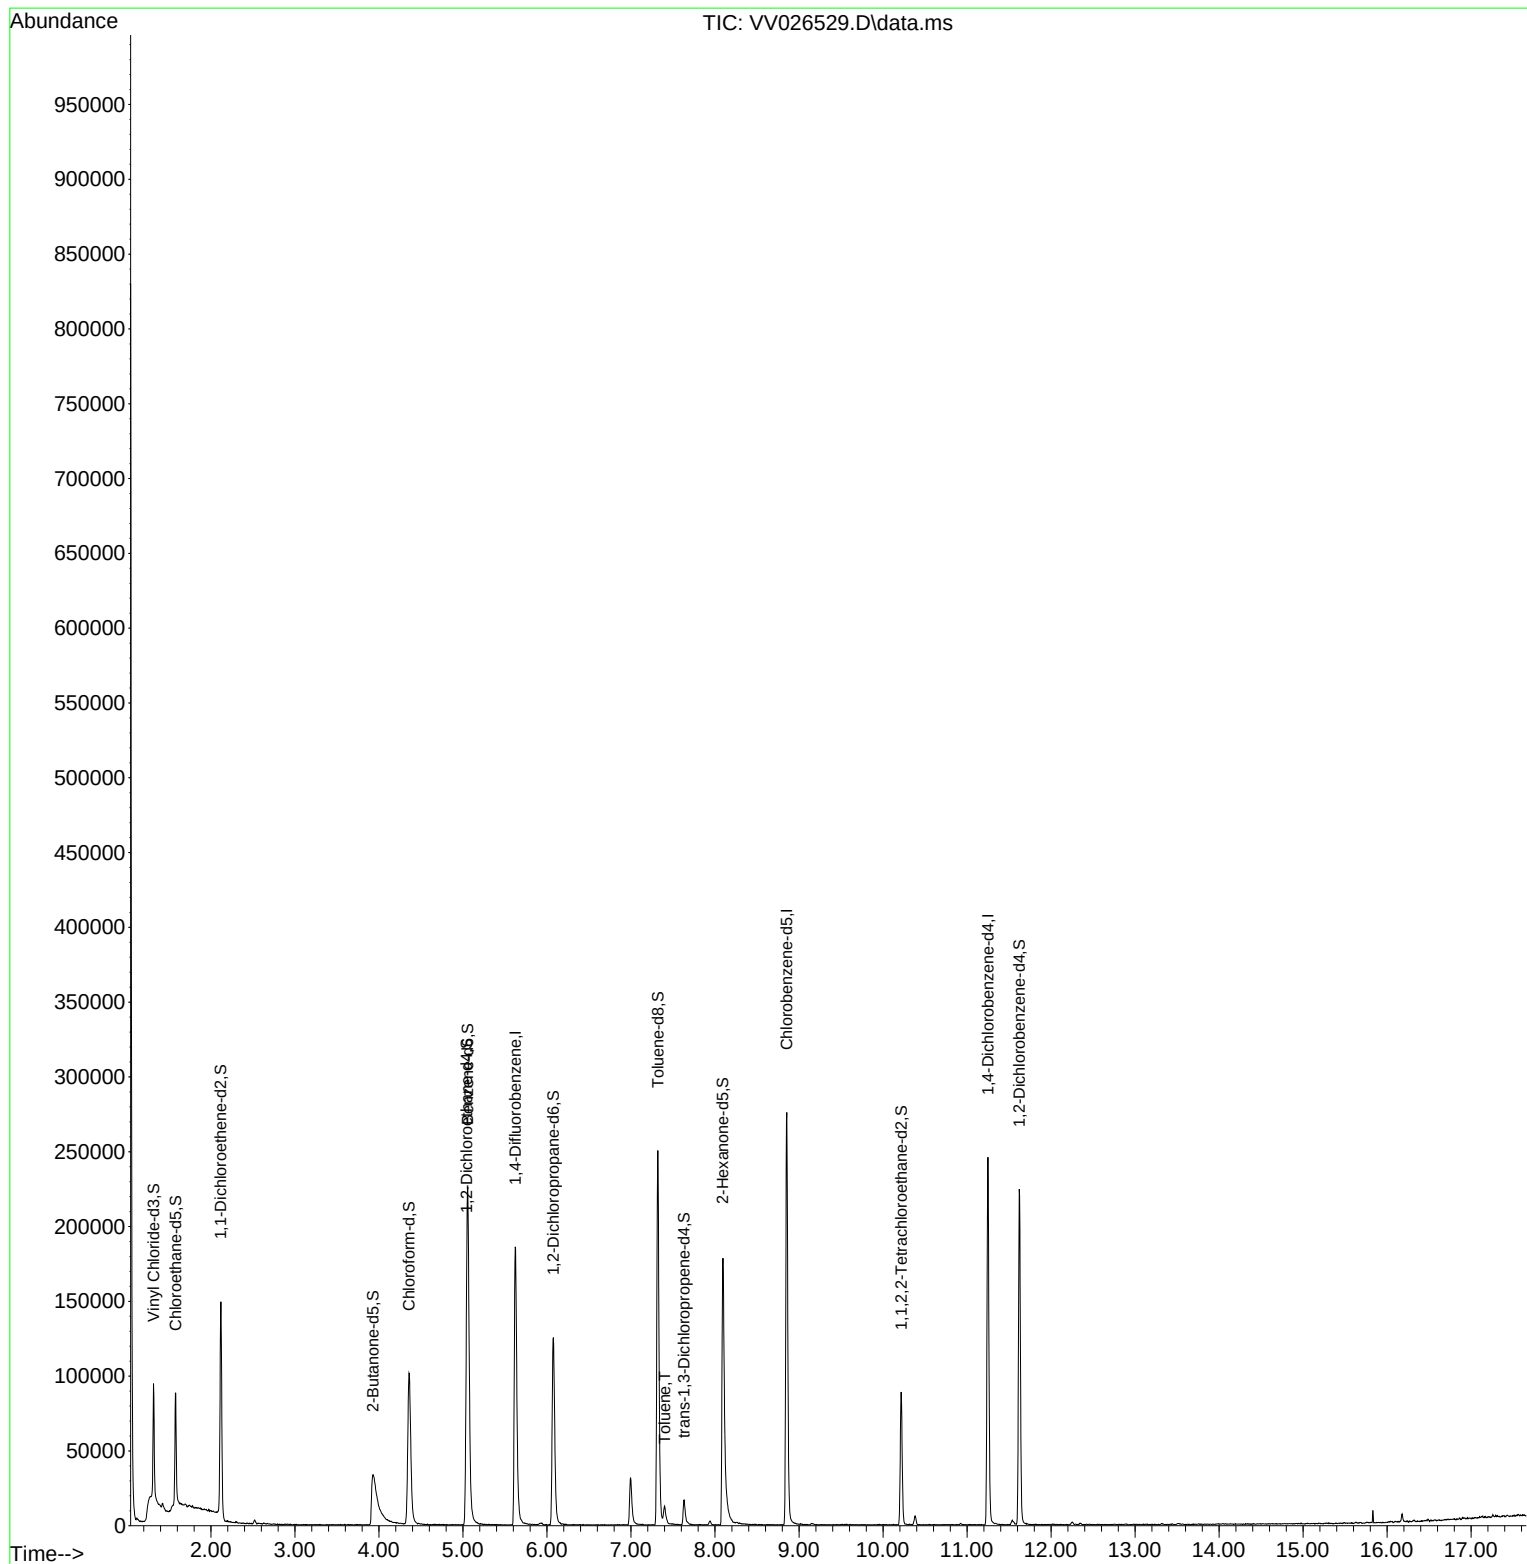

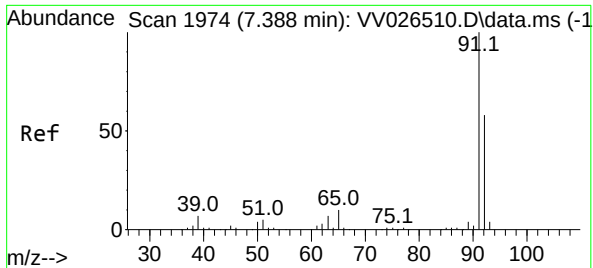

#42

Toluene

Concen: 0.201 ug/L

RT: 7.400 min Scan# 19

Delta R.T. 0.013 min

Lab File: VV026529.D


Acq: 23 Jun 2022 21:07

Instrument :

MSVOA_V

ClientSampleId :

C0AF0

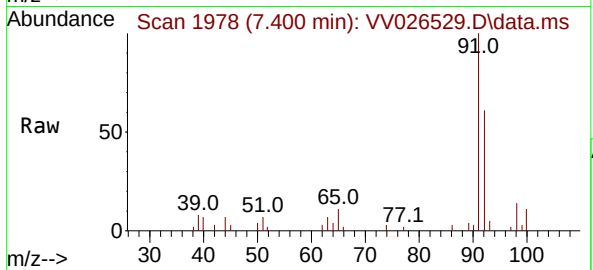

Tgt Ion: 91 Resp: 9779

Ion Ratio Lower Upper

91 100

92 60.6 40.3 74.9

