

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW062322\  
 Data File : VW026535.D  
 Acq On : 23 Jun 2022 23:30  
 Operator : SY/MD  
 Sample : N3474-02  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 34 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AA6

Quant Time: Jun 24 02:07:24 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR062322WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jun 24 00:51:15 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|-------|----------|
| -----                         |        |       |          |          |       |          |
| Internal Standards            |        |       |          |          |       |          |
| 1) 1,4-Difluorobenzene        | 5.622  | 114   | 237136   | 5.000    | ug/L  | 0.00     |
| 28) Chlorobenzene-d5          | 8.853  | 117   | 219392   | 5.000    | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   | 95251    | 5.000    | ug/L  | 0.00     |
|                               |        |       |          |          |       |          |
| System Monitoring Compounds   |        |       |          |          |       |          |
| 4) Vinyl Chloride-d3          | 1.317  | 65    | 82656    | 4.334    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =     | 86.600%  |
| 7) Chloroethane-d5            | 1.577  | 69    | 68421    | 4.466    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =     | 89.400%  |
| 11) 1,1-Dichloroethene-d2     | 2.117  | 63    | 111180   | 3.281    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =     | 65.600%  |
| 20) 2-Butanone-d5             | 3.924  | 46    | 107370   | 56.629   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =     | 113.260% |
| 24) Chloroform-d              | 4.358  | 84    | 140486   | 4.506    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 90.200%  |
| 26) 1,2-Dichloroethane-d4     | 5.040  | 65    | 56740    | 4.725    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 94.600%  |
| 32) Benzene-d6                | 5.056  | 84    | 291060   | 4.619    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =     | 92.400%  |
| 36) 1,2-Dichloropropane-d6    | 6.075  | 67    | 84628    | 4.884    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =     | 97.600%  |
| 41) Toluene-d8                | 7.317  | 98    | 243019   | 4.288    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =     | 85.800%  |
| 43) trans-1,3-Dichloroprop... | 7.628  | 79    | 15821    | 3.532    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =     | 70.600%  |
| 46) 2-Hexanone-d5             | 8.091  | 63    | 86976    | 50.979   | ug/L  | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =     | 101.960% |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84    | 53752    | 4.742    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =     | 94.800%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152   | 79536    | 5.046    | ug/L  | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =     | 101.000% |
|                               |        |       |          |          |       |          |
| Target Compounds              |        |       |          |          |       | Qvalue   |
| 13) Acetone                   | 2.211  | 43    | 8749     | 7.274    | ug/L  | 60       |
| 16) Methylene chloride        | 2.519  | 84    | 9513     | 0.560    | ug/L  | 96       |
| -----                         |        |       |          |          |       |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV062322\  
Data File : VV026535.D  
Acq On : 23 Jun 2022 23:30  
Operator : SY/MD  
Sample : N3474-02  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AA6

Quant Time: Jun 24 02:07:24 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR062322WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Fri Jun 24 00:51:15 2022  
Response via : Initial Calibration




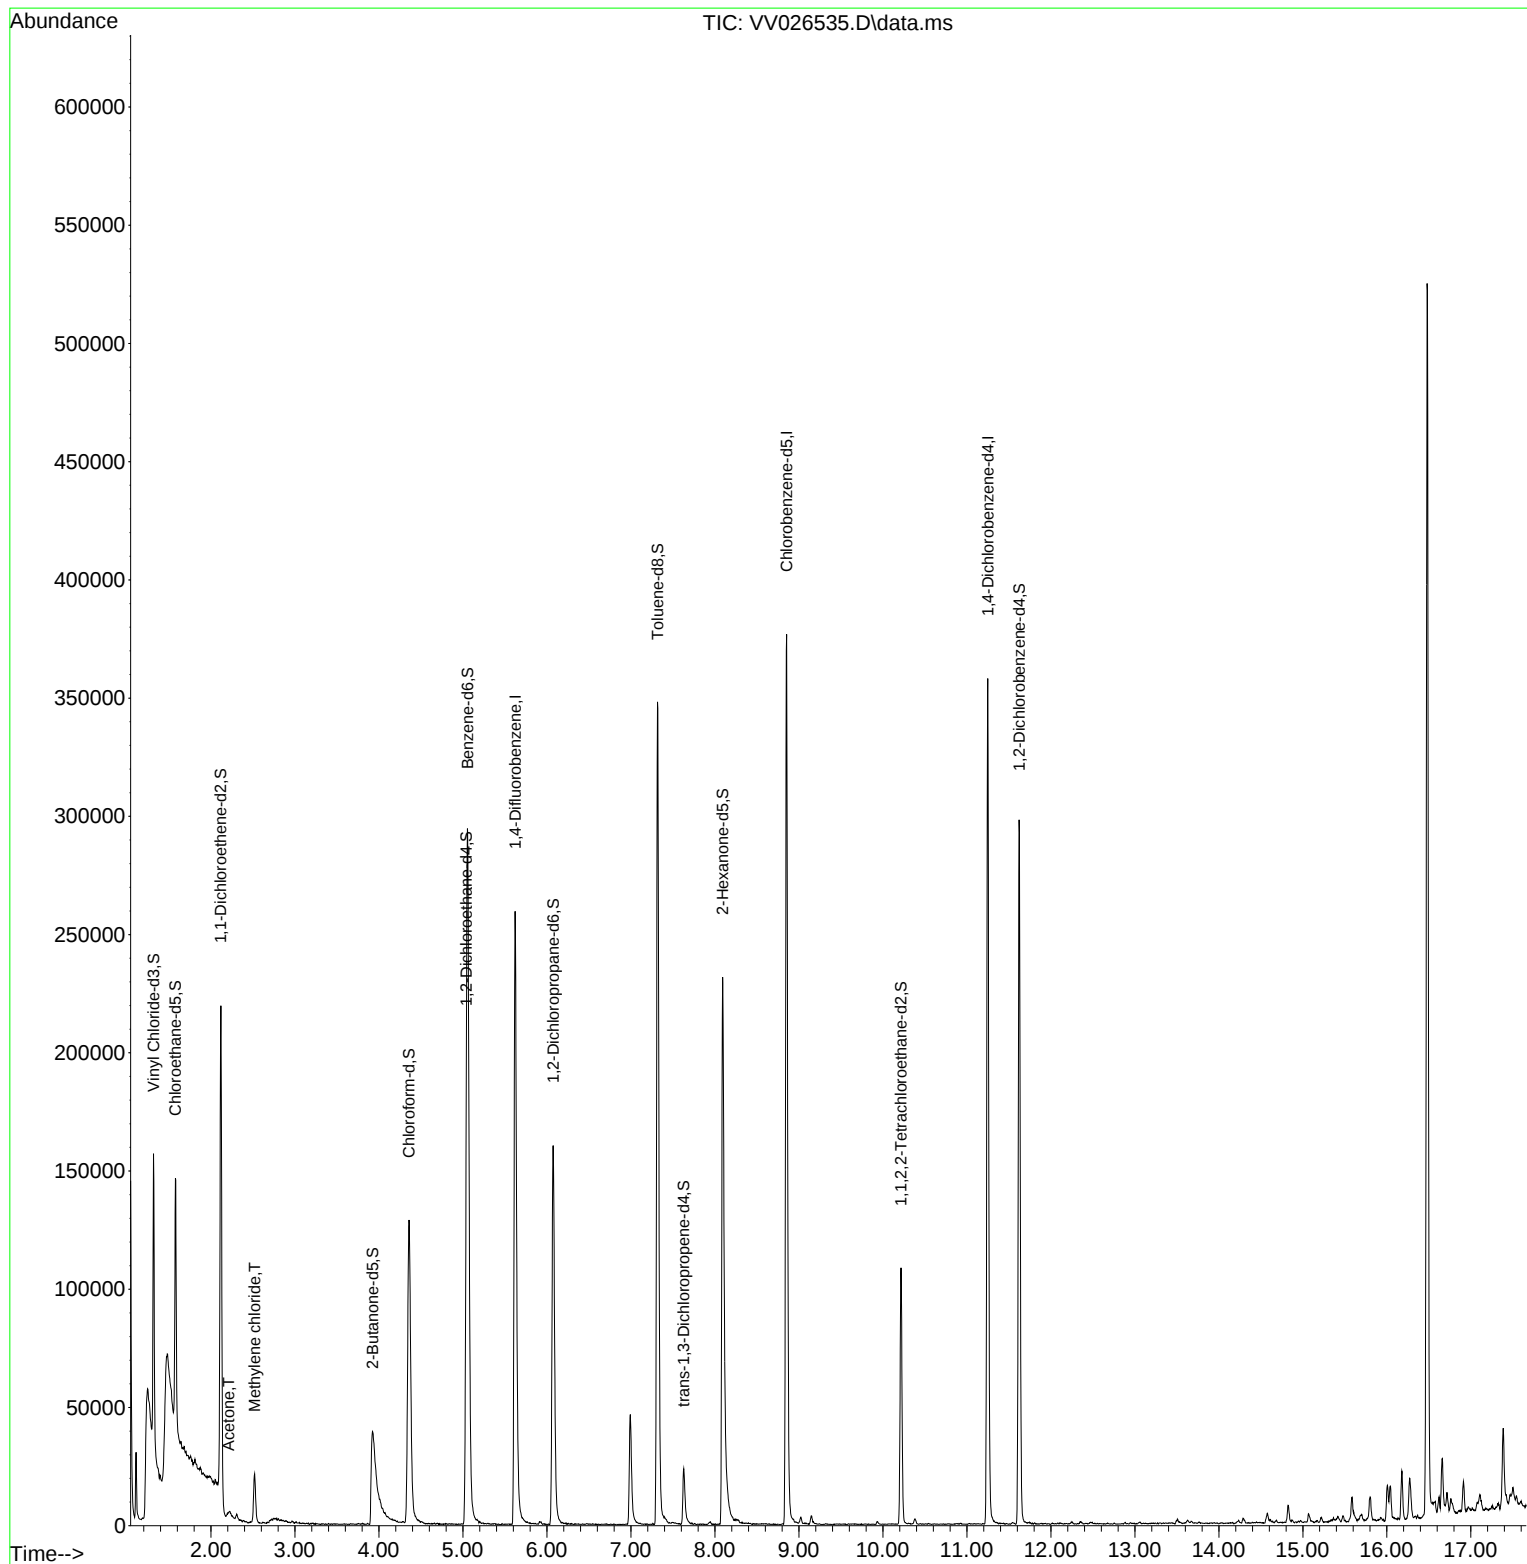


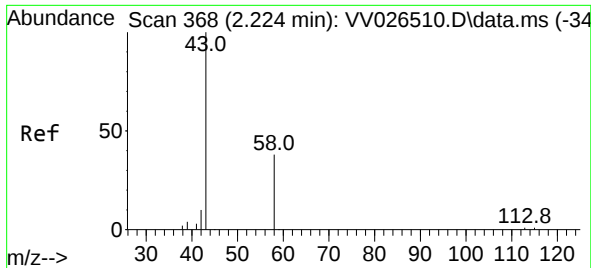

#13  
Acetone  
Concen: 7.274 ug/L  
RT: 2.211 min Scan# 30  
Delta R.T. -0.013 min  
Lab File: VV026535.D  
Acq: 23 Jun 2022 23:30

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AA6

Tgt Ion: 43 Resp: 8749  
Ion Ratio Lower Upper  
43 100  
58 13.3 0.0 75.0

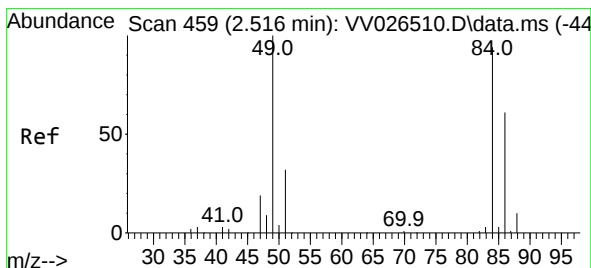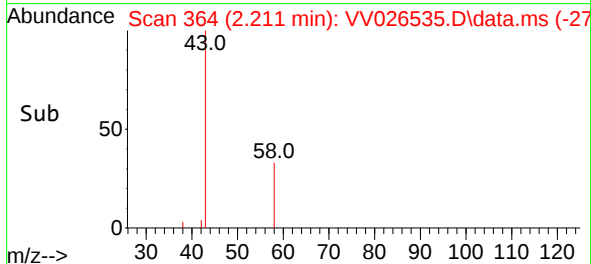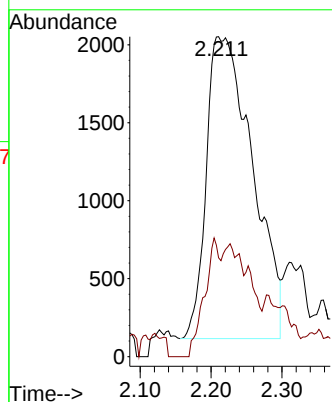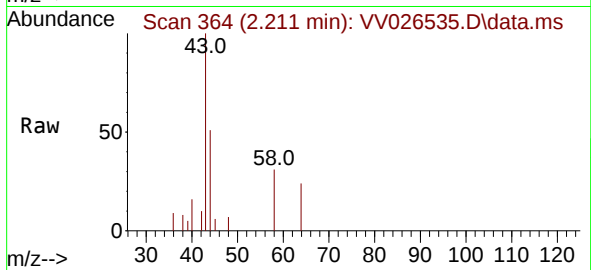

#16  
Methylene chloride  
Concen: 0.560 ug/L  
RT: 2.519 min Scan# 460  
Delta R.T. 0.003 min  
Lab File: VV026535.D  
Acq: 23 Jun 2022 23:30

Tgt Ion: 84 Resp: 9513  
Ion Ratio Lower Upper  
84 100  
86 62.9 46.0 85.4  
49 105.7 77.7 144.3

