

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062322\
 Data File : VW026543.D
 Acq On : 24 Jun 2022 10:17
 Operator : SY/MD
 Sample : N3401-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF8

Manual Integrations
 APPROVED

Reviewed By :Krupa
 Patel

06/28/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Jun 25 02:32:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	175052	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	160260	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	67008	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	50986	3.622	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.400%
7) Chloroethane-d5	1.581	69	48647	4.301	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.000%
11) 1,1-Dichloroethene-d2	2.118	63	78250	3.128	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.600%
20) 2-Butanone-d5	3.934	46	67757	48.411	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.820%
24) Chloroform-d	4.359	84	112915	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	5.043	65	45178	5.097	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%
32) Benzene-d6	5.060	84	218795	4.753	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	6.076	67	65715	5.191	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.800%
41) Toluene-d8	7.320	98	178868	4.321	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.400%
43) trans-1,3-Dichloroprop...	7.629	79	14070	4.300	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.000%
46) 2-Hexanone-d5	8.095	63	46532	37.337	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.680%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40254	4.861	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	56326	5.079	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%
Target Compounds						
					Qvalue	
13) Acetone	2.233	43	7479m	8.423	ug/L	
42) Toluene	7.397	91	27091	0.561	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026543.D
Acq On : 24 Jun 2022 10:17
Operator : SY/MD
Sample : N3401-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF8


Manual Integrations
APPROVED


Reviewed By :Krupa
Patel

06/28/2022
Supervised By :Mahesh
Dadoda

06/28/2022


Quant Time: Jun 25 02:32:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 02:21:54 2022
Response via : Initial Calibration

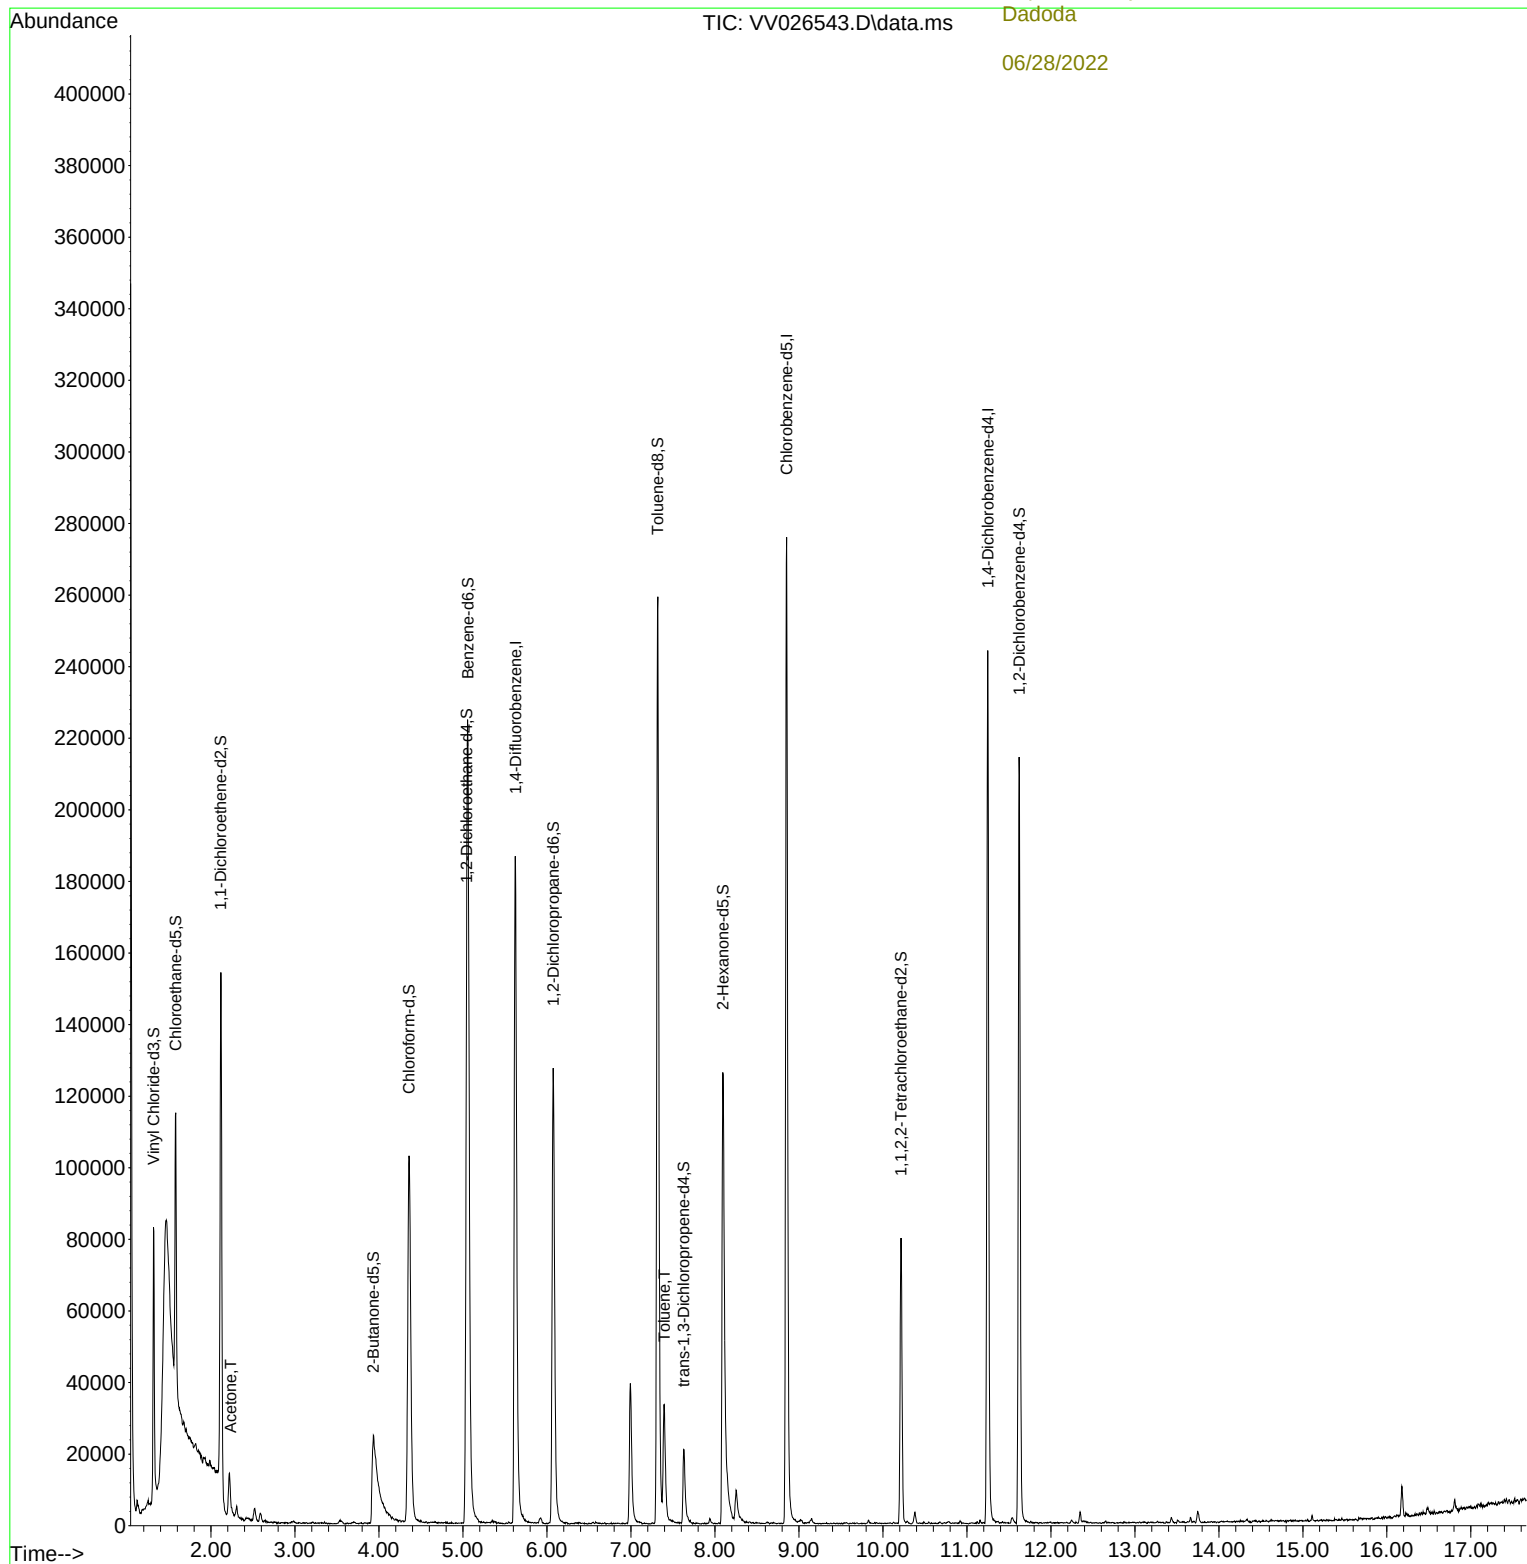

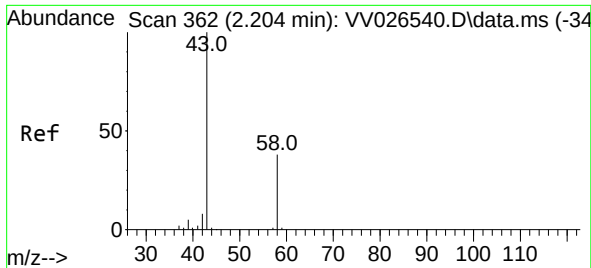

#13
Acetone
Concen: 8.423 ug/L m
RT: 2.233 min Scan# 31
Delta R.T. 0.029 min
Lab File: VV026543.D
Acq: 24 Jun 2022 10:17

Instrument :
MSVOA_V
ClientSampleId :
C0AF8

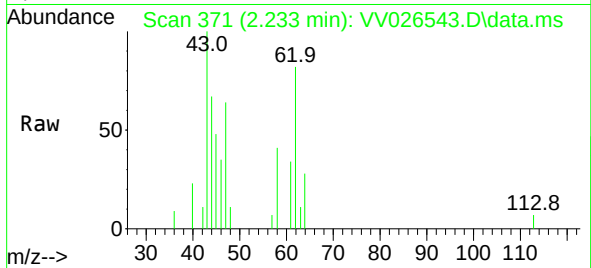




Tgt Ion: 43 Resp: 7479
Ion Ratio Lower Upper
43 100
58 22.0 0.0 75.0

Manual Integrations
APPROVED

Reviewed By :Krupa
Patel

06/28/2022
Supervised By :Mahesh
Dadoda

06/28/2022

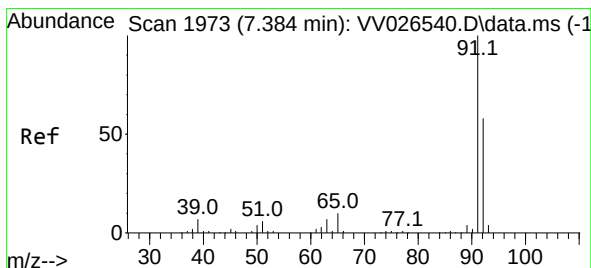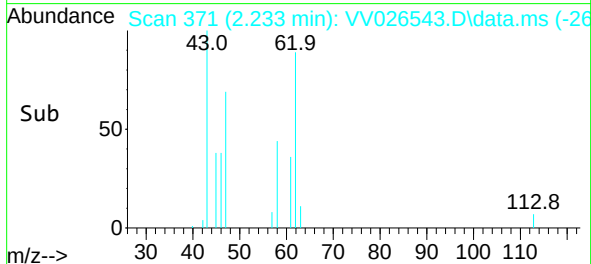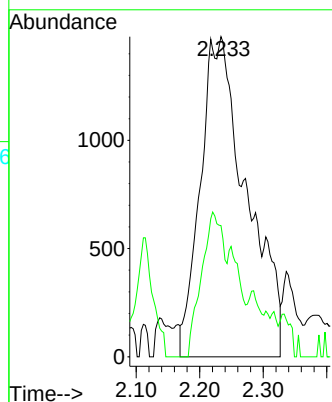

#42
Toluene
Concen: 0.561 ug/L
RT: 7.397 min Scan# 1977
Delta R.T. 0.013 min
Lab File: VV026543.D
Acq: 24 Jun 2022 10:17

Tgt Ion: 91 Resp: 27091
Ion Ratio Lower Upper
91 100
92 57.4 40.3 74.9

