

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062322\
 Data File : VW026559.D
 Acq On : 24 Jun 2022 16:41
 Operator : SY/MD
 Sample : N3425-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL7

Quant Time: Jun 25 02:36:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	228887	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	210410	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	89127	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	66661	3.621	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.400%
7) Chloroethane-d5	1.580	69	61031	4.127	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.600%
11) 1,1-Dichloroethene-d2	2.121	63	95131	2.908	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.200%#
20) 2-Butanone-d5	3.908	46	108556	59.318	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.640%
24) Chloroform-d	4.362	84	132024	4.388	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.043	65	52532	4.533	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
32) Benzene-d6	5.059	84	258447	4.276	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.075	67	77173	4.643	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.800%
41) Toluene-d8	7.320	98	215504	3.965	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%
43) trans-1,3-Dichloroprop...	7.628	79	19259	4.483	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.091	63	79460	48.562	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49797	4.580	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	70147	4.756	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.200%
Target Compounds						
					Qvalue	
13) Acetone	2.201	43	5952	5.127	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026559.D
Acq On : 24 Jun 2022 16:41
Operator : SY/MD
Sample : N3425-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL7


Quant Time: Jun 25 02:36:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 02:21:54 2022
Response via : Initial Calibration

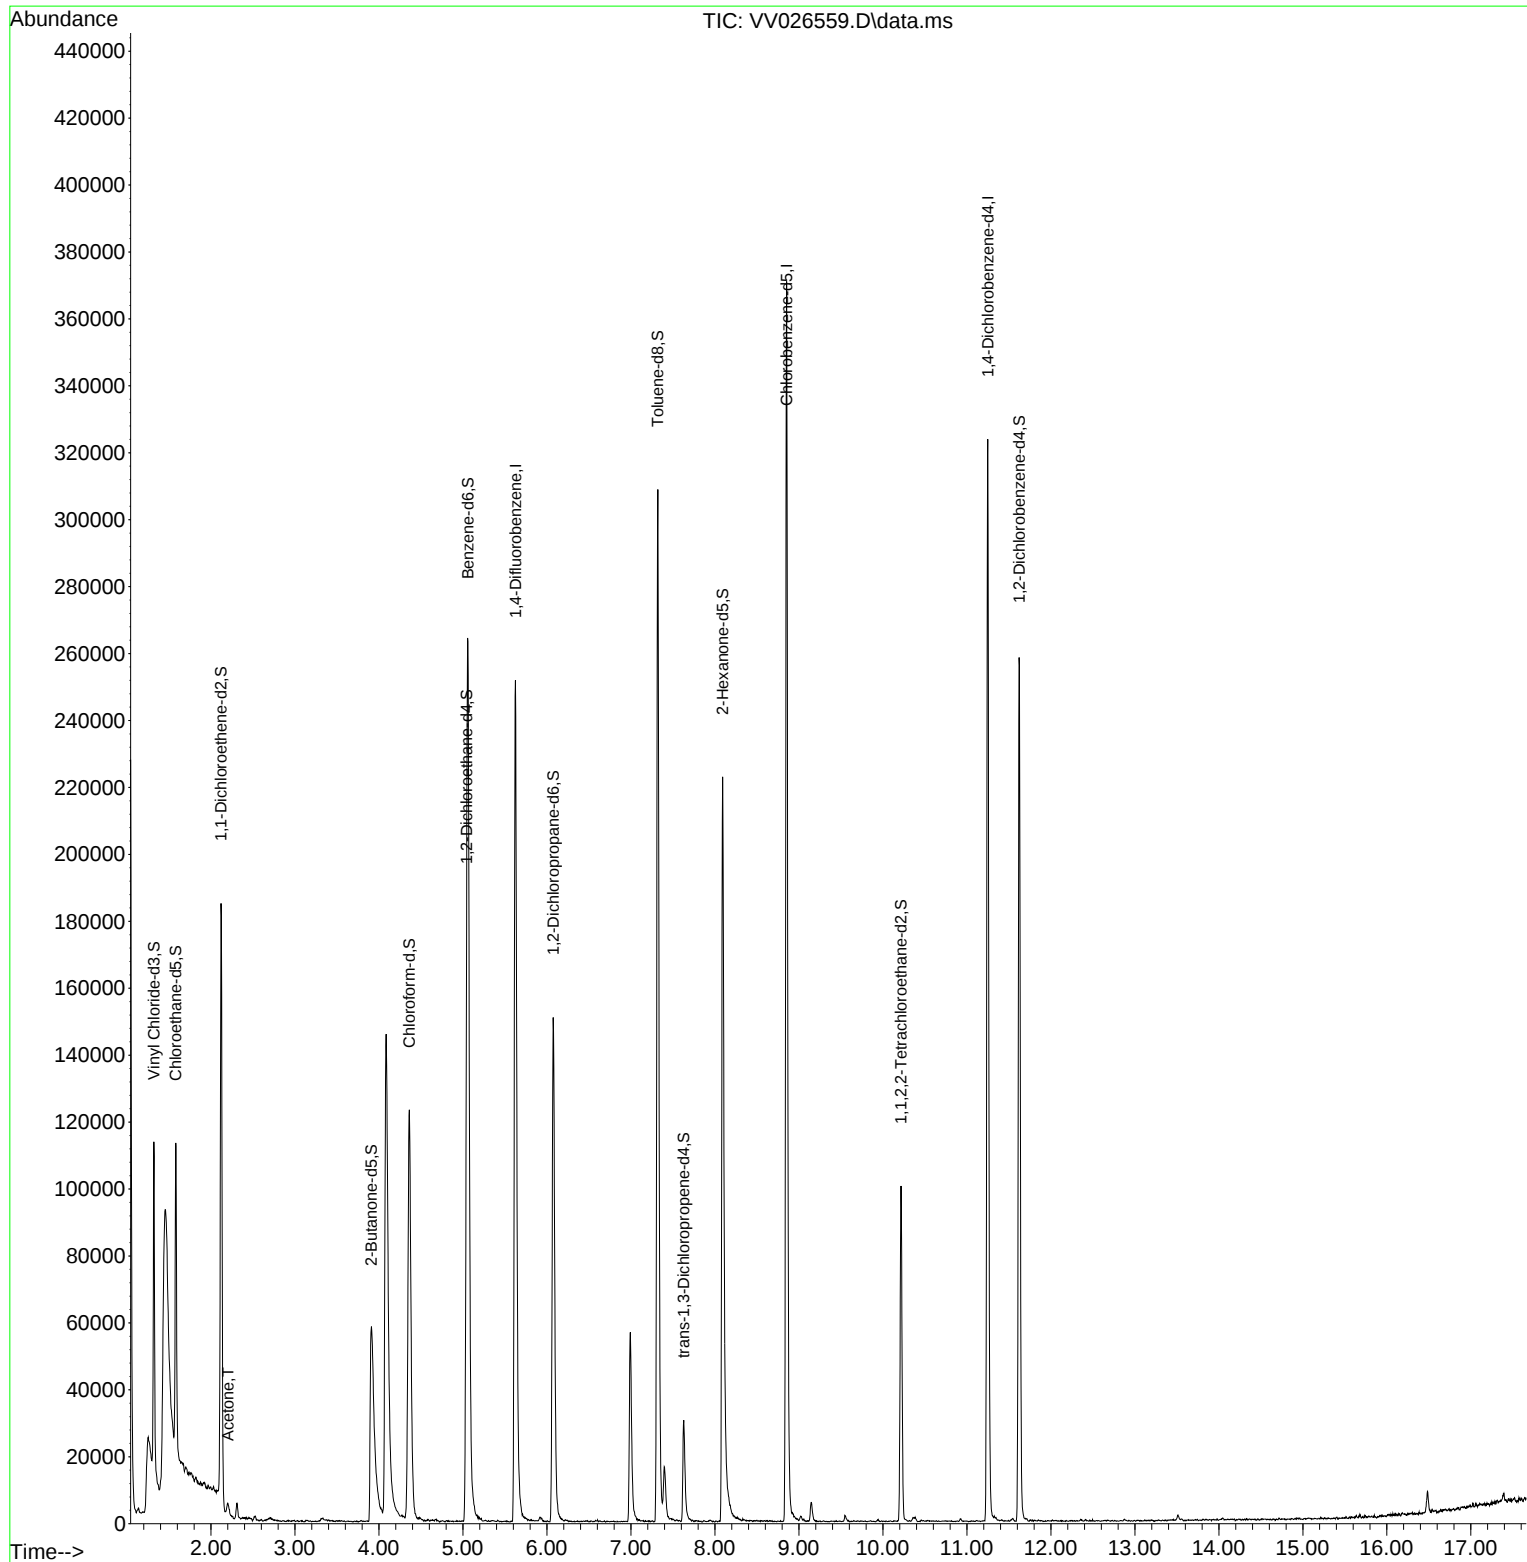

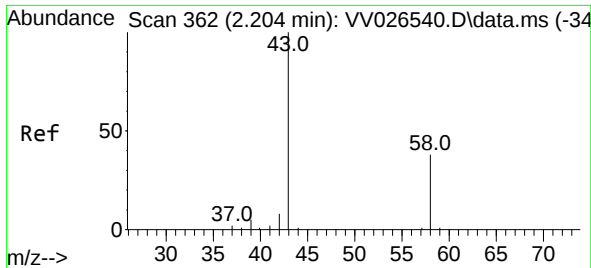

#13
 Acetone
 Concen: 5.127 ug/L
 RT: 2.201 min Scan# 30
 Delta R.T. -0.003 min
 Lab File: VV026559.D
 Acq: 24 Jun 2022 16:41

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL7

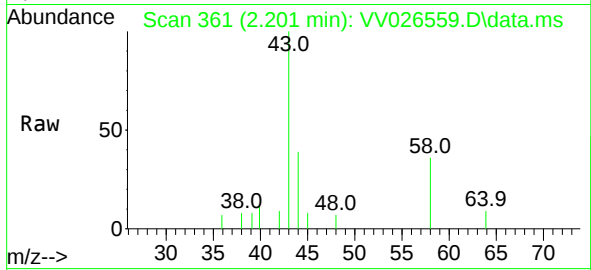

Tgt Ion: 43 Resp: 5952
 Ion Ratio Lower Upper
 43 100
 58 37.8 0.0 75.0

