

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW062322\
 Data File : VW026560.D
 Acq On : 24 Jun 2022 17:04
 Operator : SY/MD
 Sample : N3425-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL8

Quant Time: Jun 25 02:36:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 25 02:21:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.626	114	229174	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	211720	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	89166	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	67320	3.653	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.000%
7) Chloroethane-d5	1.584	69	61248	4.137	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.800%
11) 1,1-Dichloroethene-d2	2.121	63	93149	2.844	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.800%#
20) 2-Butanone-d5	3.905	46	105841	57.762	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.520%
24) Chloroform-d	4.365	84	129618	4.302	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.000%
26) 1,2-Dichloroethane-d4	5.044	65	52191	4.498	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
32) Benzene-d6	5.060	84	258721	4.254	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.000%
36) 1,2-Dichloropropane-d6	6.079	67	76293	4.562	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.200%
41) Toluene-d8	7.320	98	217283	3.973	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%
43) trans-1,3-Dichloroprop...	7.629	79	19558	4.525	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%
46) 2-Hexanone-d5	8.092	63	76700	46.585	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.160%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49036	4.482	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	68361	4.633	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.600%
Target Compounds						
					Qvalue	
13) Acetone	2.204	43	10295	8.856	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV062322\
Data File : VV026560.D
Acq On : 24 Jun 2022 17:04
Operator : SY/MD
Sample : N3425-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAL8

Quant Time: Jun 25 02:36:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR062322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 25 02:21:54 2022
Response via : Initial Calibration

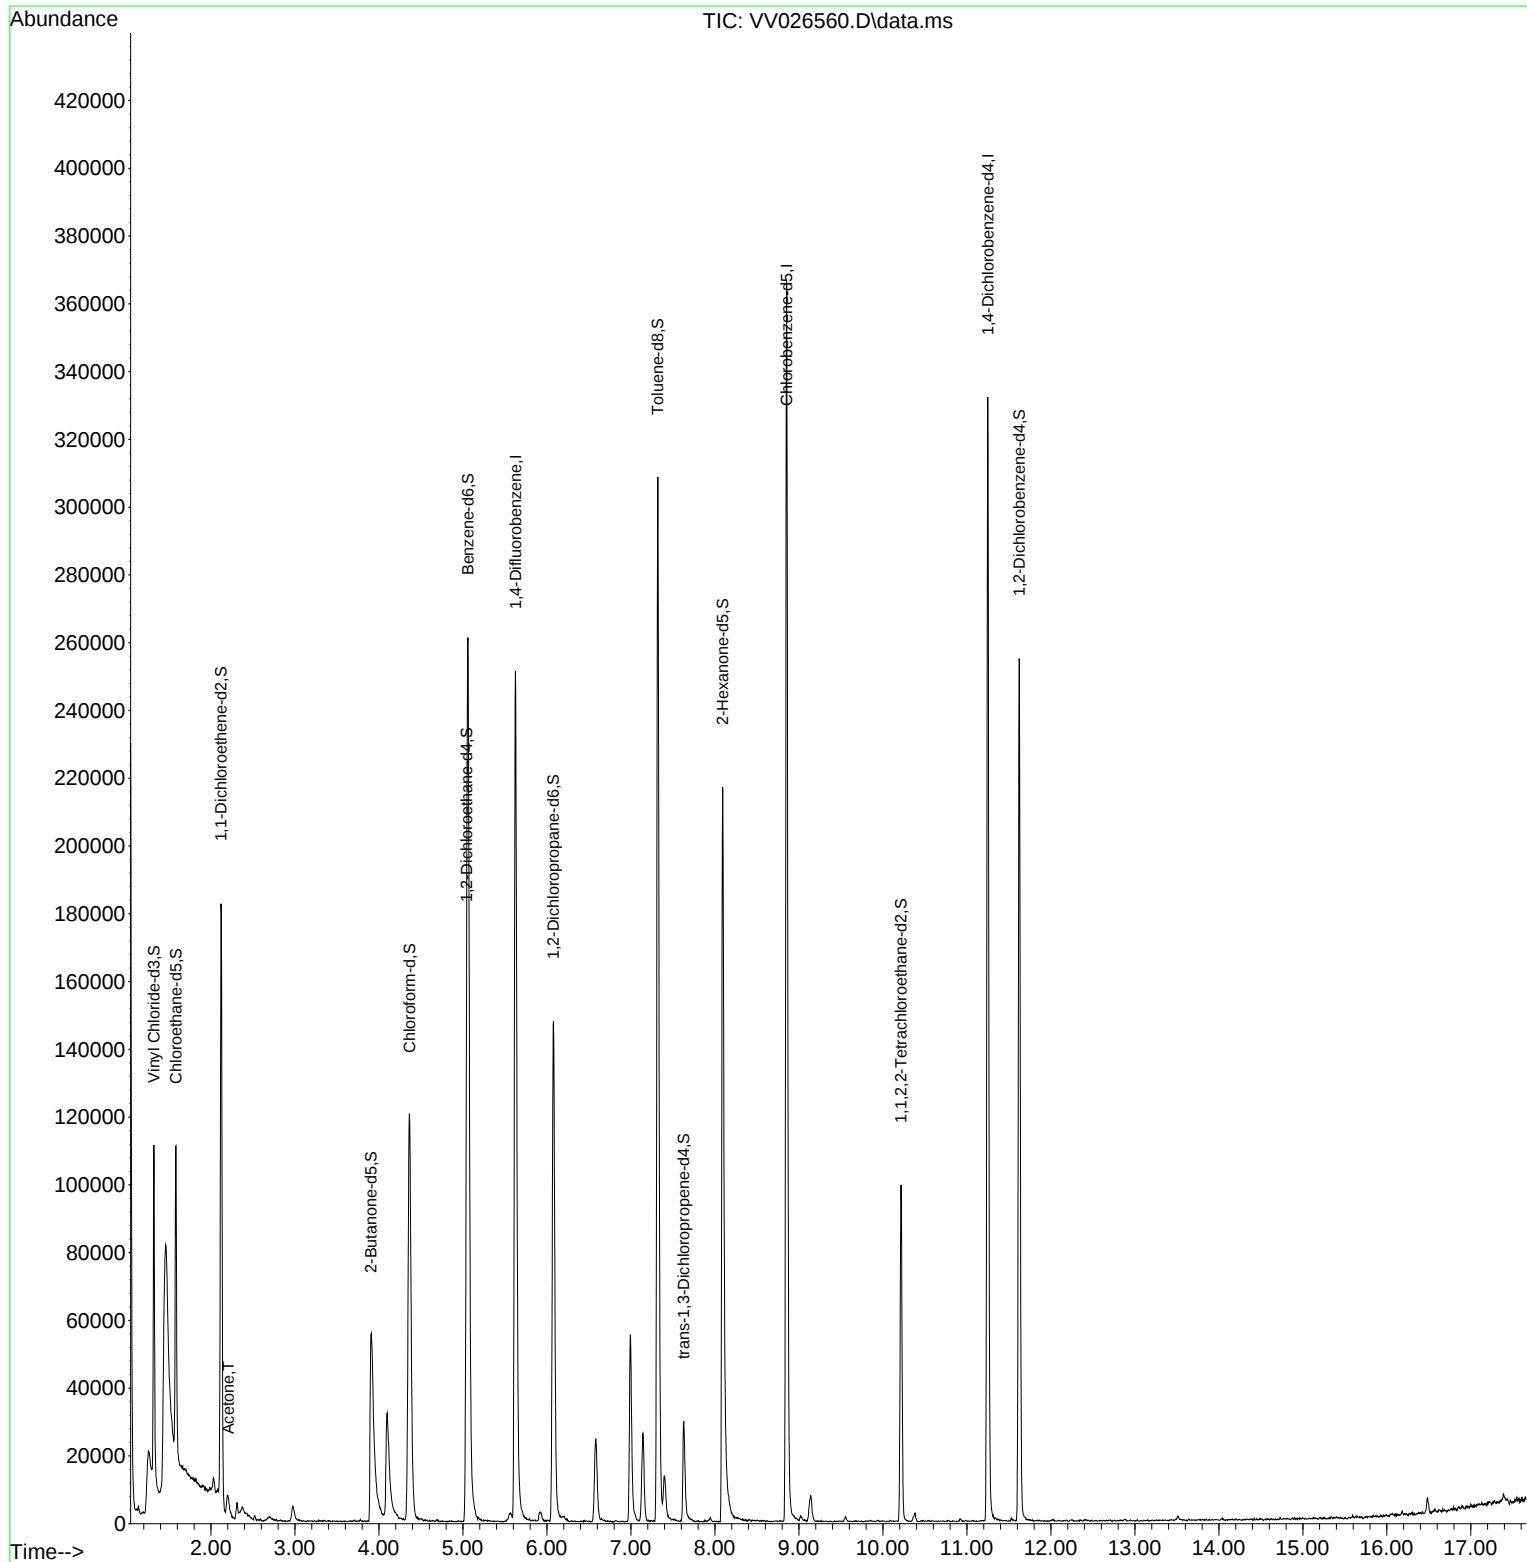

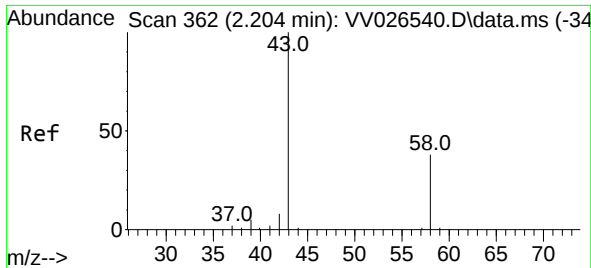

#13
 Acetone
 Concen: 8.856 ug/L
 RT: 2.204 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VV026560.D
 Acq: 24 Jun 2022 17:04

Instrument :
 MSVOA_V
 ClientSampleId :
 COAL8

Tgt Ion: 43 Resp: 10295
 Ion Ratio Lower Upper
 43 100
 58 36.5 0.0 75.0

